

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
 Data File : VX025969.D
 Acq On : 21 Dec 2021 20:02
 Operator : JC/MD
 Sample : M5126-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J12

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
 Title : VOC Analysis

Signal : TIC: VX025969.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	32	rBV	4004	7900	1.12%	0.156%
2	1.368	43	46	53	rVB	86753	85956	12.23%	1.700%
3	1.666	91	95	106	rBV	71135	97567	13.88%	1.930%
4	2.306	194	200	210	rBV	124548	203116	28.90%	4.018%
5	2.514	232	234	237	rVV2	309	351	0.05%	0.007%
6	2.550	237	240	242	rVV2	309	280	0.04%	0.006%
7	2.709	264	266	270	rVB2	332	316	0.04%	0.006%
8	2.788	276	279	286	rVB4	700	1132	0.16%	0.022%
9	2.940	300	304	306	rBV2	552	844	0.12%	0.017%
10	3.142	333	337	340	rVB2	232	200	0.03%	0.004%
11	3.270	355	358	359	rBV	207	232	0.03%	0.005%
12	3.312	362	365	367	rBV	270	260	0.04%	0.005%
13	3.477	390	392	395	rBV	234	218	0.03%	0.004%
14	3.617	409	415	419	rBV3	576	1013	0.14%	0.020%
15	3.928	463	466	468	rVB2	195	196	0.03%	0.004%
16	3.952	468	470	473	rBV2	150	172	0.02%	0.003%
17	4.050	484	486	489	rVB2	212	187	0.03%	0.004%
18	4.196	508	510	514	rVB	171	187	0.03%	0.004%
19	4.349	533	535	537	rBV2	215	218	0.03%	0.004%
20	4.458	544	553	570	rBV	48330	142685	20.30%	2.822%
21	4.696	591	592	597	rVB3	296	329	0.05%	0.007%
22	4.751	599	601	602	rVV2	225	225	0.03%	0.004%
23	4.867	618	620	624	rBV2	164	181	0.03%	0.004%
24	5.062	638	652	666	rBV	83887	265285	37.75%	5.248%
25	5.379	698	704	715	rVB3	810	2273	0.32%	0.045%
26	5.678	750	753	755	rBV2	225	243	0.03%	0.005%
27	5.733	759	762	763	rVB2	225	192	0.03%	0.004%
28	5.970	787	801	820	rBV2	217155	651031	92.64%	12.878%
29	6.263	846	849	851	rVV2	252	275	0.04%	0.005%
30	6.287	851	853	854	rVV2	215	208	0.03%	0.004%
31	6.367	864	866	869	rVB	205	197	0.03%	0.004%
32	6.458	879	881	883	rVB2	288	204	0.03%	0.004%
33	6.763	921	931	946	rBV	189305	425580	60.56%	8.418%
34	7.123	983	990	1000	rVV6	8274	20304	2.89%	0.402%
35	7.312	1011	1021	1037	rVB	170528	373201	53.11%	7.382%
36	7.434	1037	1041	1042	rBV2	667	829	0.12%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
 Data File : VX025969.D
 Acq On : 21 Dec 2021 20:02
 Operator : JC/MD
 Sample : M5126-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J12

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
 Title : VOC Analysis

37	7.604	1066	1069	1070	rBV	369	314	0.04%	0.006%
38	7.714	1086	1087	1090	rBV2	227	233	0.03%	0.005%
39	7.793	1098	1100	1101	rBV	297	255	0.04%	0.005%
40	7.927	1118	1122	1124	rBV2	398	455	0.06%	0.009%
41	8.324	1181	1187	1198	rBV	109684	172838	24.60%	3.419%
42	8.476	1209	1212	1213	rBV2	368	304	0.04%	0.006%
43	8.586	1227	1230	1233	rVB3	363	388	0.06%	0.008%
44	8.653	1234	1241	1248	rBV	430559	702719	100.00%	13.901%
45	8.952	1285	1290	1299	rBV	65013	92650	13.18%	1.833%
46	9.086	1311	1312	1315	rVB2	271	237	0.03%	0.005%
47	9.275	1338	1343	1347	rVB3	4290	5997	0.85%	0.119%
48	9.384	1356	1361	1384	rVV	198020	296059	42.13%	5.856%
49	9.579	1391	1393	1396	rVB	264	229	0.03%	0.005%
50	10.055	1465	1471	1485	rBV	307608	413642	58.86%	8.182%
51	10.244	1499	1502	1506	rVB2	629	800	0.11%	0.016%
52	10.299	1507	1511	1515	rBV3	496	711	0.10%	0.014%
53	10.354	1518	1520	1523	rVB	280	216	0.03%	0.004%
54	10.500	1542	1544	1546	rVV2	171	178	0.03%	0.004%
55	10.555	1549	1553	1554	rBV	186	260	0.04%	0.005%
56	10.622	1561	1564	1566	rBV2	212	291	0.04%	0.006%
57	10.689	1573	1575	1577	rVB2	248	203	0.03%	0.004%
58	10.872	1601	1605	1607	rBV2	208	254	0.04%	0.005%
59	11.085	1638	1640	1642	rBV2	239	259	0.04%	0.005%
60	11.122	1642	1646	1649	rVV2	1144	1421	0.20%	0.028%
61	11.195	1652	1658	1666	rVV	235443	301518	42.91%	5.964%
62	11.323	1677	1679	1681	rVB2	222	184	0.03%	0.004%
63	11.457	1697	1701	1702	rVV2	285	278	0.04%	0.005%
64	11.482	1702	1705	1708	rVV3	433	574	0.08%	0.011%
65	11.536	1712	1714	1718	rVV3	234	303	0.04%	0.006%
66	11.603	1721	1725	1728	rVB2	243	302	0.04%	0.006%
67	11.677	1735	1737	1743	rVB2	168	233	0.03%	0.005%
68	11.750	1743	1749	1753	rBV3	1095	1559	0.22%	0.031%
69	11.823	1756	1761	1762	rBV2	281	321	0.05%	0.006%
70	11.933	1776	1779	1782	rBV2	665	817	0.12%	0.016%
71	12.024	1789	1794	1802	rBV	279568	357996	50.94%	7.082%
72	12.116	1808	1809	1811	rBV	377	337	0.05%	0.007%
73	12.225	1823	1827	1833	rVB3	1126	1683	0.24%	0.033%
74	12.323	1837	1843	1855	rVB	318596	408247	58.10%	8.076%
75	12.439	1860	1862	1864	rVB	399	237	0.03%	0.005%
76	12.609	1888	1890	1892	rBV2	194	204	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
 Data File : VX025969.D
 Acq On : 21 Dec 2021 20:02
 Operator : JC/MD
 Sample : M5126-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J12

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
 Title : VOC Analysis

77	12.658	1897	1898	1902	rVV3	246	258	0.04%	0.005%
78	12.719	1906	1908	1911	rBV2	179	177	0.03%	0.004%
79	12.768	1913	1916	1918	rBV	257	243	0.03%	0.005%
80	13.158	1979	1980	1983	rBV2	239	211	0.03%	0.004%
81	13.268	1996	1998	2000	rBV	426	215	0.03%	0.004%
82	13.487	2032	2034	2038	rVB2	217	284	0.04%	0.006%
83	13.798	2083	2085	2087	rBV	325	171	0.02%	0.003%
84	13.877	2096	2098	2101	rVB	238	251	0.04%	0.005%
85	13.957	2109	2111	2114	rVV2	124	187	0.03%	0.004%
86	14.006	2117	2119	2122	rVV2	258	308	0.04%	0.006%
87	14.188	2146	2149	2152	rBV	301	341	0.05%	0.007%
88	14.414	2185	2186	2192	rVB2	273	319	0.05%	0.006%
89	14.615	2217	2219	2221	rBV	210	175	0.02%	0.003%
90	14.652	2224	2225	2228	rBV	209	223	0.03%	0.004%
91	14.908	2266	2267	2270	rVB2	197	177	0.03%	0.004%
92	15.018	2283	2285	2287	rVV2	202	189	0.03%	0.004%
93	15.164	2306	2309	2311	rBV	231	332	0.05%	0.007%
94	15.292	2327	2330	2335	rBV3	239	409	0.06%	0.008%
95	15.584	2377	2378	2384	rBV	241	514	0.07%	0.010%
96	15.920	2431	2433	2435	rBV2	169	180	0.03%	0.004%
97	15.938	2435	2436	2439	rBV2	175	186	0.03%	0.004%
98	16.414	2512	2514	2517	rVB2	284	236	0.03%	0.005%
99	16.444	2517	2519	2522	rBV2	197	225	0.03%	0.004%
100	16.584	2540	2542	2543	rBV	338	214	0.03%	0.004%




Sum of corrected areas: 5055318

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
Data File : VX025969.D
Acq On : 21 Dec 2021 20:02
Operator : JC/MD
Sample : M5126-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J12

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

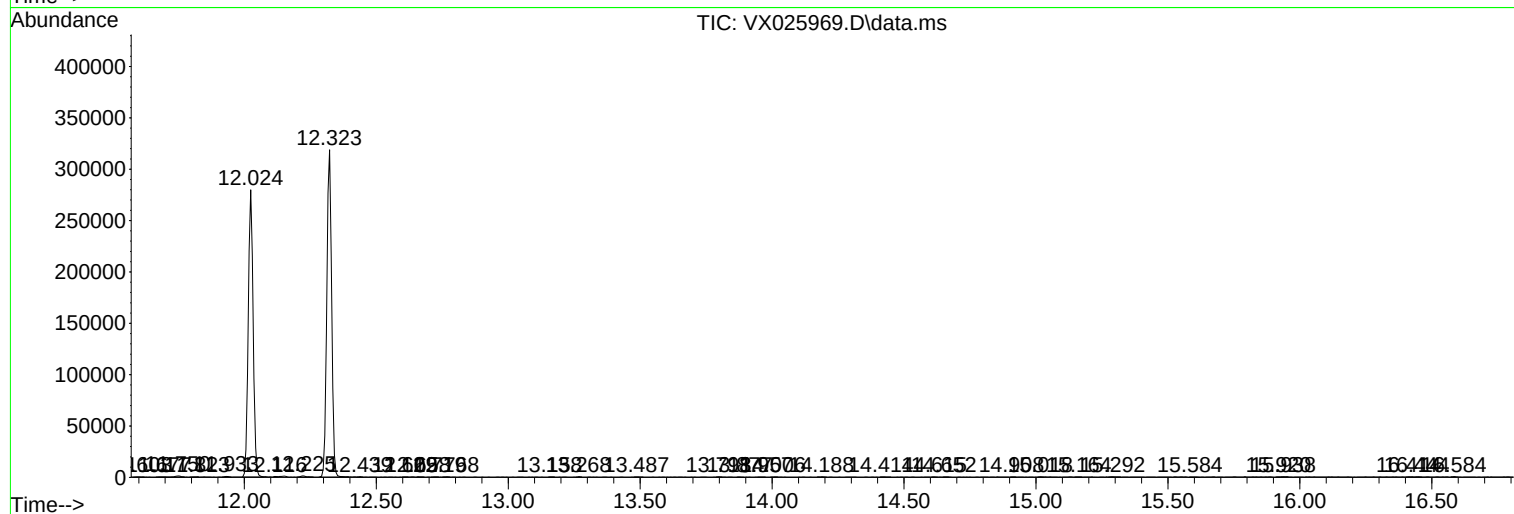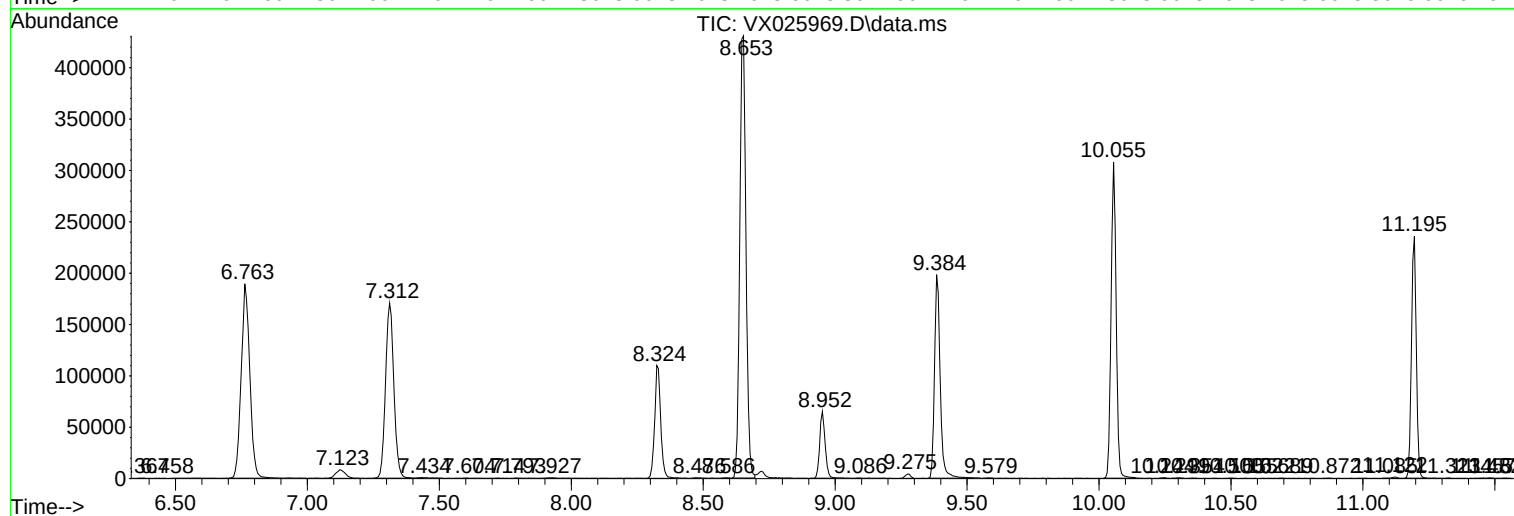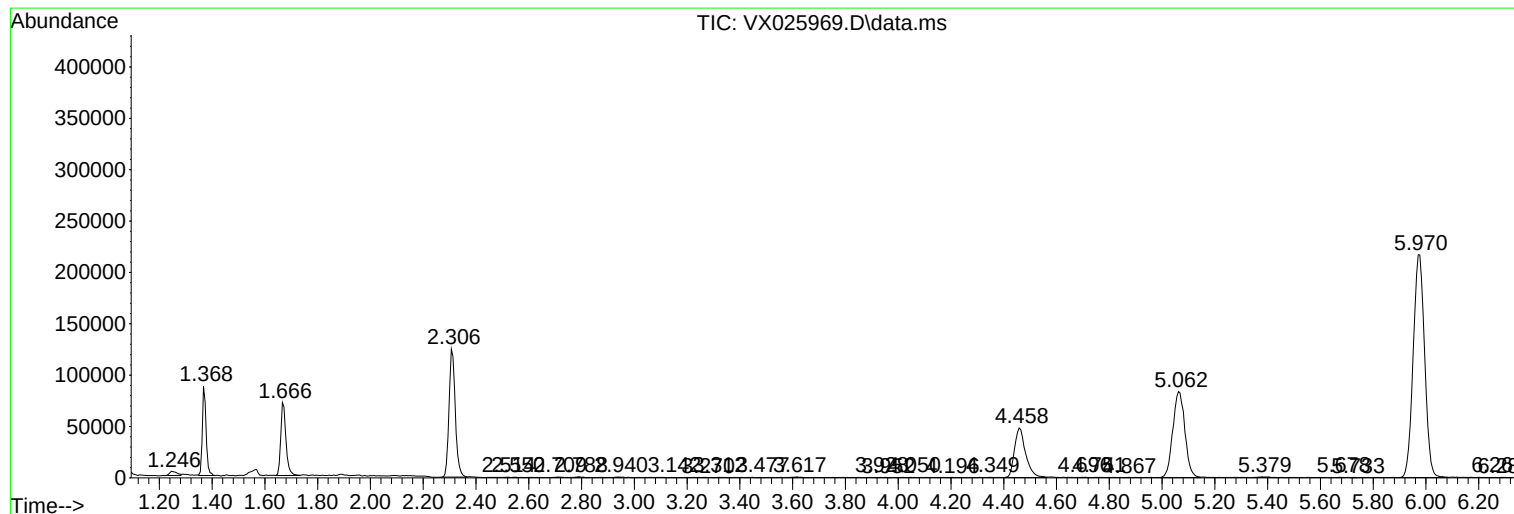

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
Data File : VX025969.D
Acq On : 21 Dec 2021 20:02
Operator : JC/MD
Sample : M5126-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J12

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
Data File : VX025969.D
Acq On : 21 Dec 2021 20:02
Operator : JC/MD
Sample : M5126-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J12

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc