

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
 Data File : VX025970.D
 Acq On : 21 Dec 2021 20:25
 Operator : JC/MD
 Sample : M5126-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J17

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
 Title : VOC Analysis

Signal : TIC: VX025970.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	54	rVB	85253	84500	11.15%	1.618%
2	1.666	91	95	104	rVB	69412	90733	11.98%	1.738%
3	2.306	194	200	210	rBV	131561	206069	27.20%	3.946%
4	2.538	234	238	244	rBV3	1382	2459	0.32%	0.047%
5	2.794	276	280	284	rVB3	947	1565	0.21%	0.030%
6	2.947	300	305	315	rVB3	1919	4675	0.62%	0.090%
7	3.020	315	317	318	rBV	222	169	0.02%	0.003%
8	3.197	344	346	349	rBV	267	283	0.04%	0.005%
9	3.270	356	358	362	rVB2	161	166	0.02%	0.003%
10	3.422	380	383	388	rBV2	204	362	0.05%	0.007%
11	3.642	418	419	423	rBB2	281	240	0.03%	0.005%
12	3.690	426	427	431	rBV	188	218	0.03%	0.004%
13	3.770	439	440	443	rVB2	212	136	0.02%	0.003%
14	3.794	443	444	446	rBV	247	136	0.02%	0.003%
15	3.818	446	448	450	rBV2	153	138	0.02%	0.003%
16	4.001	475	478	479	rBV2	204	203	0.03%	0.004%
17	4.056	485	487	491	rVB2	190	216	0.03%	0.004%
18	4.282	522	524	527	rBV2	188	184	0.02%	0.004%
19	4.458	544	553	566	rBV	50848	146025	19.27%	2.796%
20	4.965	634	636	638	rBV	218	139	0.02%	0.003%
21	5.062	640	652	668	rVV	92639	268326	35.42%	5.138%
22	5.269	684	686	687	rBV	191	133	0.02%	0.003%
23	5.373	698	703	705	rBV2	187	291	0.04%	0.006%
24	5.550	728	732	733	rBV2	330	440	0.06%	0.008%
25	5.647	746	748	749	rBV	184	158	0.02%	0.003%
26	5.690	753	755	758	rBV	202	187	0.02%	0.004%
27	5.970	789	801	823	rBV2	218700	654921	86.45%	12.542%
28	6.239	843	845	847	rVB2	260	222	0.03%	0.004%
29	6.257	847	848	850	rBV	253	202	0.03%	0.004%
30	6.318	857	858	861	rBV3	255	199	0.03%	0.004%
31	6.495	883	887	888	rBV2	140	159	0.02%	0.003%
32	6.763	922	931	945	rVV	136680	328000	43.30%	6.281%
33	7.110	981	988	996	rVV6	5571	12169	1.61%	0.233%
34	7.312	1012	1021	1032	rBV	175306	379831	50.14%	7.274%
35	7.507	1051	1053	1058	rVB2	315	298	0.04%	0.006%
36	7.568	1061	1063	1064	rBV	276	188	0.02%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
 Data File : VX025970.D
 Acq On : 21 Dec 2021 20:25
 Operator : JC/MD
 Sample : M5126-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J17

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
 Title : VOC Analysis

37	7.586	1064	1066	1067	rVB2	326	158	0.02%	0.003%
38	7.818	1102	1104	1106	rVB2	508	372	0.05%	0.007%
39	7.982	1129	1131	1134	rBV	165	149	0.02%	0.003%
40	8.324	1180	1187	1197	rBV	110898	176620	23.31%	3.382%
41	8.513	1216	1218	1221	rBV2	209	236	0.03%	0.005%
42	8.555	1221	1225	1226	rBV2	293	370	0.05%	0.007%
43	8.653	1233	1241	1248	rBV	474741	757591	100.00%	14.508%
44	8.720	1249	1252	1259	rVB	10356	16639	2.20%	0.319%
45	8.952	1284	1290	1301	rBV	64852	96062	12.68%	1.840%
46	9.220	1330	1334	1335	rBV	267	306	0.04%	0.006%
47	9.384	1356	1361	1375	rBV	317148	484109	63.90%	9.271%
48	9.781	1424	1426	1428	rVB	319	199	0.03%	0.004%
49	9.805	1428	1430	1433	rBV	266	219	0.03%	0.004%
50	10.055	1465	1471	1489	rBV	310073	420379	55.49%	8.050%
51	10.244	1498	1502	1507	rBV2	810	1225	0.16%	0.023%
52	10.299	1509	1511	1518	rVB4	677	1125	0.15%	0.022%
53	10.476	1538	1540	1543	rVB2	278	291	0.04%	0.006%
54	10.592	1556	1559	1560	rBV2	219	241	0.03%	0.005%
55	10.646	1565	1568	1570	rVB2	452	539	0.07%	0.010%
56	10.835	1597	1599	1600	rBV	219	137	0.02%	0.003%
57	10.921	1610	1613	1614	rVV2	145	153	0.02%	0.003%
58	11.073	1635	1638	1640	rVB2	194	189	0.02%	0.004%
59	11.128	1643	1647	1650	rBV3	1079	1414	0.19%	0.027%
60	11.195	1652	1658	1664	rBV	237766	299976	39.60%	5.745%
61	11.366	1683	1686	1687	rBV2	170	182	0.02%	0.003%
62	11.469	1700	1703	1704	rBV	449	398	0.05%	0.008%
63	11.506	1708	1709	1710	rVB	385	141	0.02%	0.003%
64	11.530	1710	1713	1715	rBV	206	196	0.03%	0.004%
65	11.567	1715	1719	1723	rVB2	204	345	0.05%	0.007%
66	11.658	1732	1734	1736	rBV2	224	202	0.03%	0.004%
67	11.750	1746	1749	1753	rVB2	1060	1136	0.15%	0.022%
68	11.847	1762	1765	1768	rVB	532	540	0.07%	0.010%
69	11.872	1768	1769	1773	rBV2	220	278	0.04%	0.005%
70	11.927	1775	1778	1782	rVV3	527	650	0.09%	0.012%
71	12.024	1789	1794	1805	rVB	293148	360997	47.65%	6.913%
72	12.152	1812	1815	1820	rVB3	849	1069	0.14%	0.020%
73	12.225	1823	1827	1831	rVV3	780	930	0.12%	0.018%
74	12.323	1837	1843	1851	rBV	313843	405621	53.54%	7.768%
75	12.481	1867	1869	1871	rBV	438	427	0.06%	0.008%
76	12.506	1871	1873	1875	rVV	334	311	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
 Data File : VX025970.D
 Acq On : 21 Dec 2021 20:25
 Operator : JC/MD
 Sample : M5126-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J17

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
 Title : VOC Analysis

77	12.536	1876	1878	1879	rVB	256	162	0.02%	0.003%
78	12.622	1887	1892	1893	rBV2	195	305	0.04%	0.006%
79	12.664	1896	1899	1900	rBV2	185	218	0.03%	0.004%
80	12.975	1948	1950	1952	rBV2	260	152	0.02%	0.003%
81	13.493	2033	2035	2039	rVB	203	237	0.03%	0.005%
82	13.561	2042	2046	2052	rVV2	143	291	0.04%	0.006%
83	13.841	2089	2092	2093	rBV	160	152	0.02%	0.003%
84	14.274	2161	2163	2165	rBV2	208	223	0.03%	0.004%
85	14.615	2216	2219	2221	rBV2	133	147	0.02%	0.003%
86	14.694	2231	2232	2235	rBV2	156	157	0.02%	0.003%
87	14.963	2274	2276	2279	rVB2	316	203	0.03%	0.004%
88	14.987	2279	2280	2284	rBV	308	258	0.03%	0.005%
89	15.115	2299	2301	2303	rBV	345	440	0.06%	0.008%
90	15.207	2314	2316	2319	rBV	226	202	0.03%	0.004%
91	15.383	2343	2345	2348	rVB2	286	248	0.03%	0.005%
92	15.414	2348	2350	2352	rBV2	224	180	0.02%	0.003%
93	15.530	2367	2369	2371	rBV	279	177	0.02%	0.003%
94	15.725	2399	2401	2403	rBV	190	134	0.02%	0.003%
95	15.749	2403	2405	2407	rBV2	275	274	0.04%	0.005%
96	15.792	2410	2412	2416	rVB	212	243	0.03%	0.005%
97	16.066	2455	2457	2458	rBV	309	257	0.03%	0.005%
98	16.127	2465	2467	2470	rBV2	261	381	0.05%	0.007%
99	16.414	2513	2514	2516	rBV2	323	136	0.02%	0.003%
100	16.651	2551	2553	2556	rBV3	208	255	0.03%	0.005%




Sum of corrected areas: 5221894

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
Data File : VX025970.D
Acq On : 21 Dec 2021 20:25
Operator : JC/MD
Sample : M5126-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J17

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

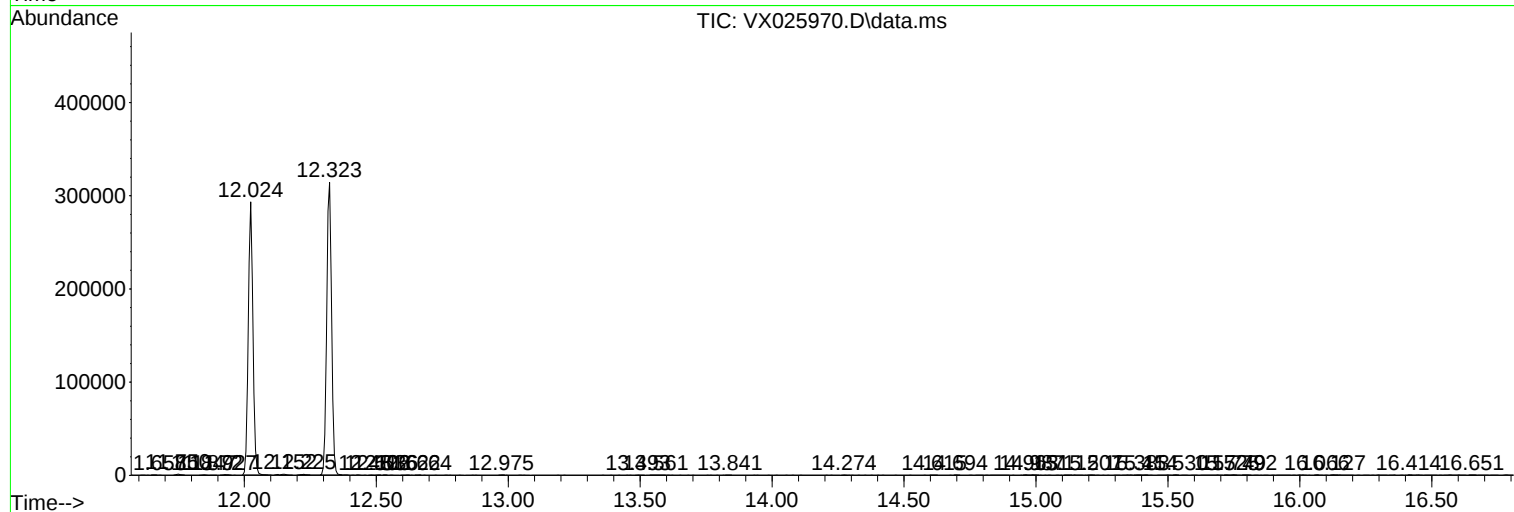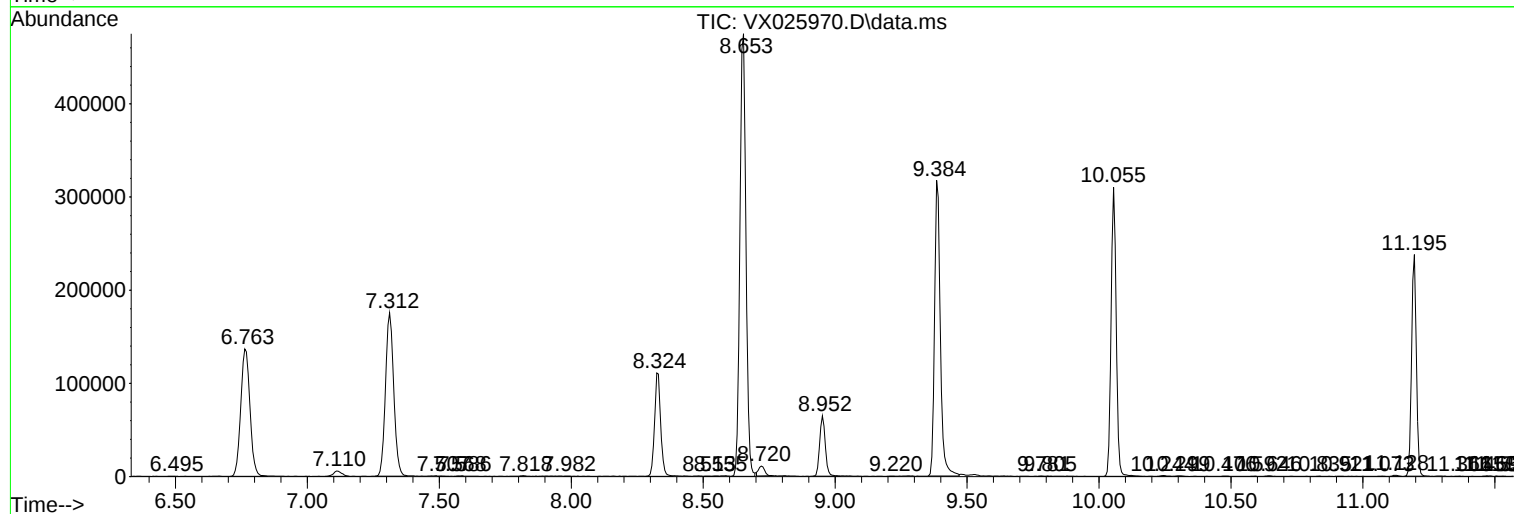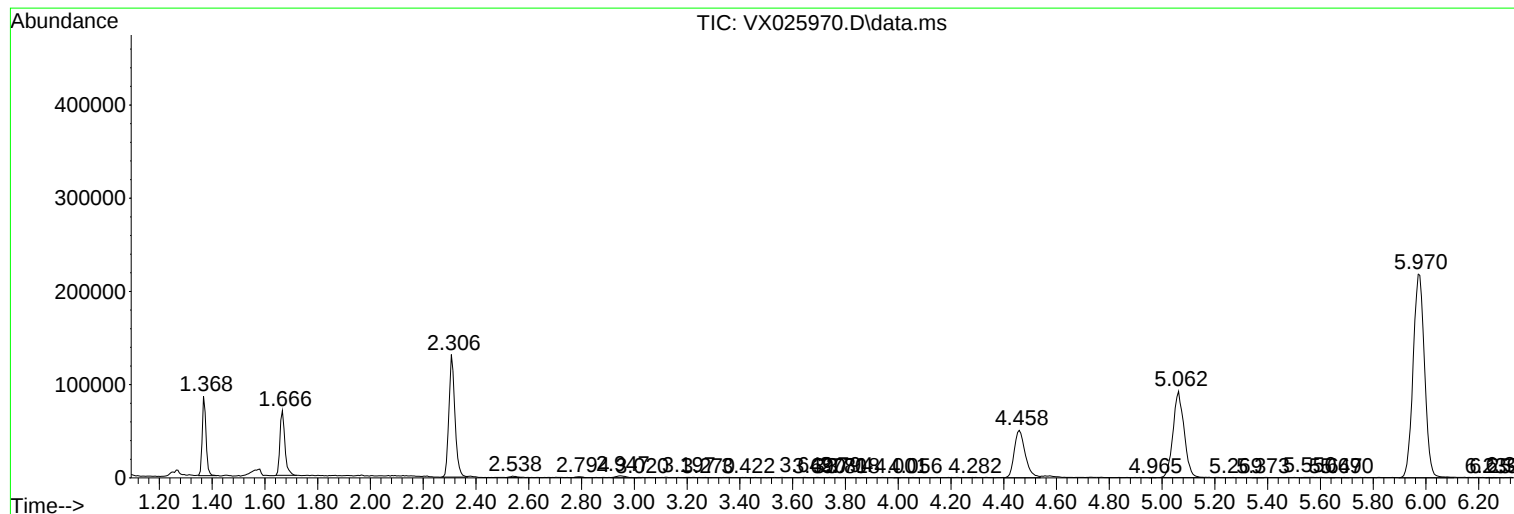

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
Data File : VX025970.D
Acq On : 21 Dec 2021 20:25
Operator : JC/MD
Sample : M5126-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J17

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
Data File : VX025970.D
Acq On : 21 Dec 2021 20:25
Operator : JC/MD
Sample : M5126-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J17

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------