




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122123\
 Data File : VX039423.D
 Acq On : 21 Dec 2023 12:47
 Operator : JC/MD
 Sample : 05808-10
 Misc : 4.90g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0B04ME

Manual IntegrationsAPPROVED

Quant Time: Dec 22 00:43:53 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 22 00:41:09 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/22/2023
 Supervised By :Mahesh Dadoda 12/22/2023

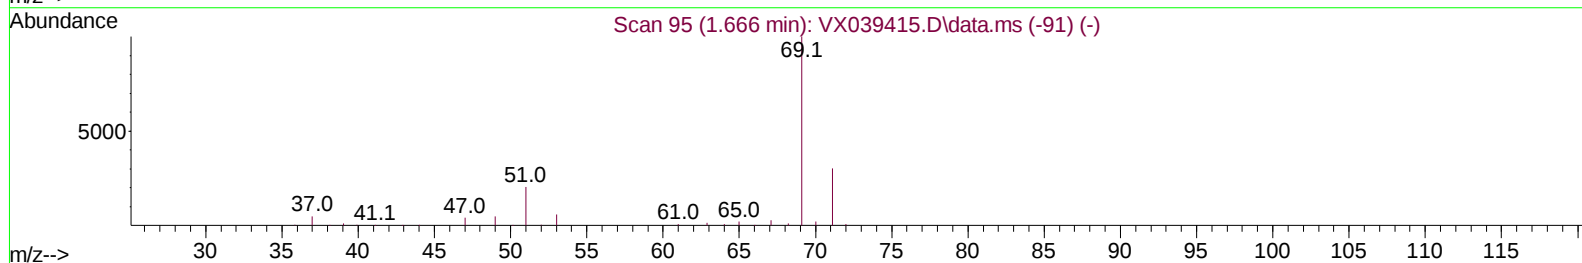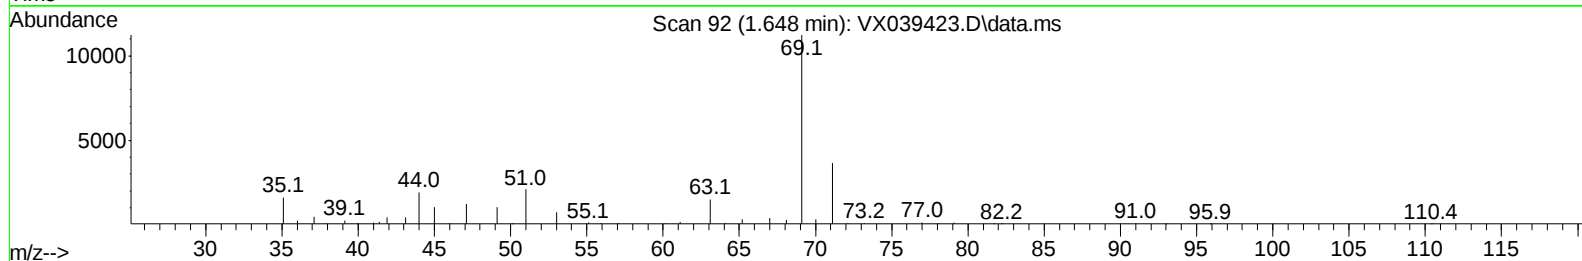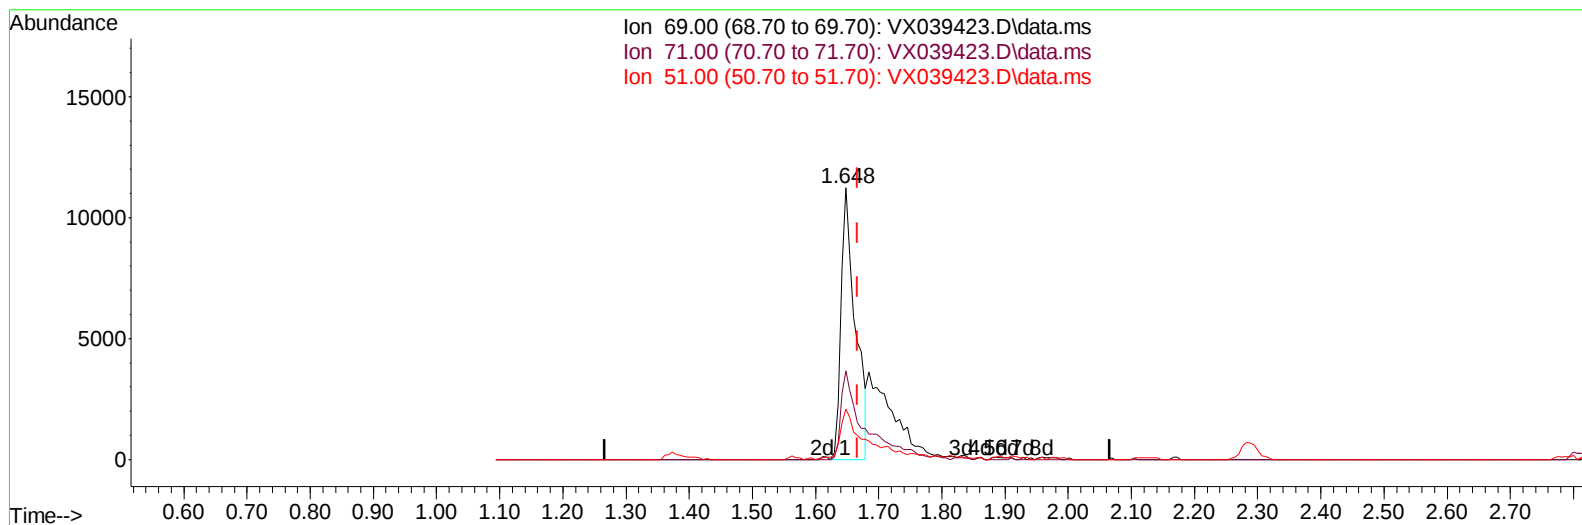

TIC: VX039423.D\data.ms

(7) Chloroethane-d5 (S)

1.648min (-0.018) 13.56 ug/L

response 17677

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.10	38.21
51.00	27.90	23.22
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122123\
 Data File : VX039423.D
 Acq On : 21 Dec 2023 12:47
 Operator : JC/MD
 Sample : 05808-10
 Misc : 4.90g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0B04ME

Manual IntegrationsAPPROVED

Quant Time: Dec 22 00:43:53 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 22 00:41:09 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/22/2023
 Supervised By :Mahesh Dadoda 12/22/2023

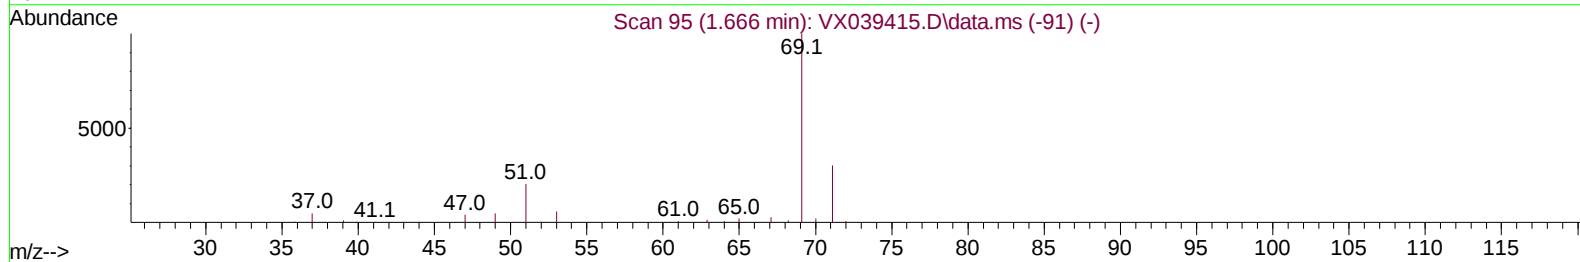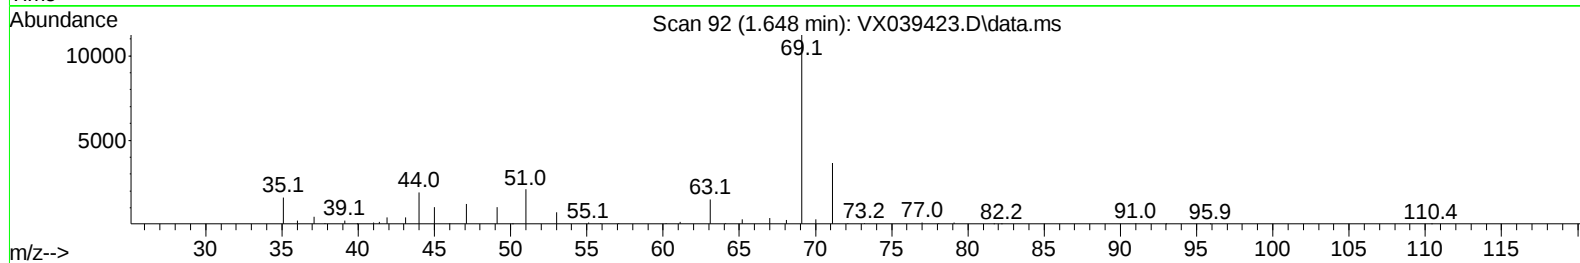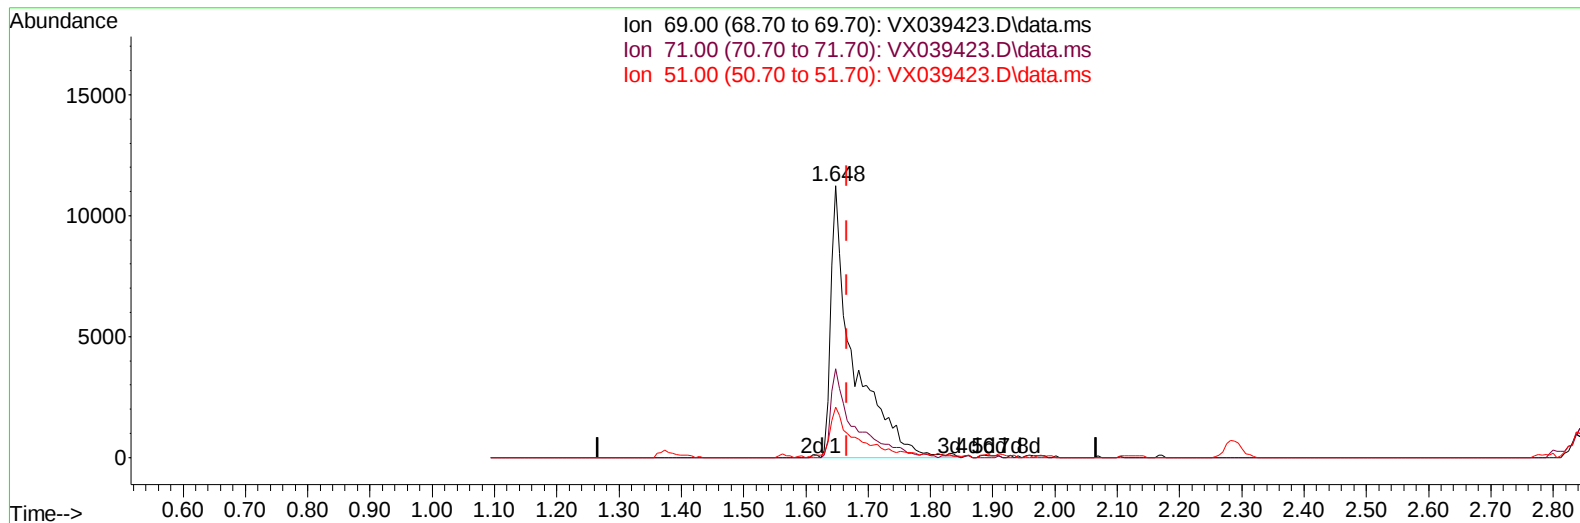

TIC: VX039423.D\data.ms

(7) Chloroethane-d5 (S)

1.648min (-0.018) 21.69 ug/L m

response 28277

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.10	23.89
51.00	27.90	14.52#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122123\
 Data File : VX039423.D
 Acq On : 21 Dec 2023 12:47
 Operator : JC/MD
 Sample : 05808-10
 Misc : 4.90g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0B04ME

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/22/2023
 Supervised By :Mahesh Dadoda 12/22/2023

Quant Time: Dec 22 00:43:53 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 22 00:41:09 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	224880	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	203972	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	100785	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	66221	37.544	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	75.080%	
7) Chloroethane-d5	1.648	69	28277m	21.689	ug/L	-0.02
Spiked Amount 50.000	Range 70	- 130	Recovery	=	43.380%#	
11) 1,1-Dichloroethene-d2	2.288	65	32350	41.782	ug/L	-0.02
Spiked Amount 50.000	Range 60	- 125	Recovery	=	83.560%	
21) 2-Butanone-d5	4.483	46	138288	86.613	ug/L	0.04
Spiked Amount 100.000	Range 40	- 130	Recovery	=	86.610%	
24) Chloroform-d	5.062	84	143883	46.081	ug/L	0.01
Spiked Amount 50.000	Range 70	- 125	Recovery	=	92.160%	
26) 1,2-Dichloroethane-d4	5.952	65	107807	53.313	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	106.620%	
32) Benzene-d6	5.964	84	303191	48.164	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	96.320%	
36) 1,2-Dichloropropane-d6	7.306	67	99228	48.981	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	97.960%	
41) Toluene-d8	8.647	98	263251	46.146	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	92.300%	
43) trans-1,3-Dichloroprop...	8.952	79	40568	39.351	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	78.700%	
47) 2-Hexanone-d5	9.397	63	107729	89.034	ug/L	0.02
Spiked Amount 100.000	Range 45	- 130	Recovery	=	89.030%	
56) 1,1,2,2-Tetrachloroeth...	11.195	84	133789	46.554	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	93.100%	
66) 1,2-Dichlorobenzene-d4	12.323	152	95514	50.138	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	100.280%	
Target Compounds						
					Qvalue	
64) 1,3-Dichlorobenzene	11.969	146	28483	9.036	ug/L	96
65) 1,4-Dichlorobenzene	12.043	146	27472	8.601	ug/L	93
67) 1,2-Dichlorobenzene	12.335	146	61800	20.496	ug/L	100
70) 1,2,4-trichlorobenzene	13.585	180	109648	55.795	ug/L	100
72) 1,2,3-Trichlorobenzene	13.963	180	35349	18.577	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122123\
Data File : VX039423.D
Acq On : 21 Dec 2023 12:47
Operator : JC/MD
Sample : 05808-10
Misc : 4.90g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0B04ME

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/22/2023
Supervised By :Mahesh Dadoda 12/22/2023

Quant Time: Dec 22 00:43:53 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 22 00:41:09 2023
Response via : Initial Calibration

