

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122123\
 Data File : VX039417.D
 Acq On : 21 Dec 2023 10:18
 Operator : JC/MD
 Sample : VX1221WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK657

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039417.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	56	rVB	98185	105858	13.18%	1.706%
2	1.672	91	96	108	rBV	64491	94177	11.72%	1.518%
3	2.307	194	200	216	rVB	178591	271300	33.78%	4.373%
4	2.514	230	234	239	rVV2	838	1320	0.16%	0.021%
5	2.556	239	241	243	rVB	281	242	0.03%	0.004%
6	2.794	275	280	287	rVB4	1542	2615	0.33%	0.042%
7	2.941	297	304	311	rVV3	2030	4343	0.54%	0.070%
8	3.020	316	317	320	rBV	222	193	0.02%	0.003%
9	3.093	324	329	332	rBV3	552	922	0.11%	0.015%
10	3.593	407	411	412	rVB2	199	197	0.02%	0.003%
11	3.660	420	422	424	rBV2	182	216	0.03%	0.003%
12	3.770	439	440	442	rBV	304	227	0.03%	0.004%
13	3.788	442	443	446	rVB	294	203	0.03%	0.003%
14	3.818	446	448	451	rBV2	259	274	0.03%	0.004%
15	3.910	457	463	466	rBV2	125	238	0.03%	0.004%
16	3.959	470	471	475	rVB2	196	214	0.03%	0.003%
17	4.001	475	478	481	rBV2	261	428	0.05%	0.007%
18	4.129	496	499	500	rBB2	276	199	0.02%	0.003%
19	4.367	535	538	542	rBV2	220	315	0.04%	0.005%
20	4.446	542	551	566	rBV	74716	211689	26.35%	3.412%
21	4.837	612	615	616	rBV3	294	296	0.04%	0.005%
22	5.056	638	651	669	rBV	97428	322155	40.11%	5.193%
23	5.300	688	691	692	rBV	216	236	0.03%	0.004%
24	5.532	726	729	730	rBV	390	407	0.05%	0.007%
25	5.672	750	752	756	rVB2	308	207	0.03%	0.003%
26	5.964	788	800	821	rBV2	264859	803235	100.00%	12.948%
27	6.184	834	836	839	rVB3	373	301	0.04%	0.005%
28	6.288	850	853	856	rBV2	258	277	0.03%	0.004%
29	6.464	881	882	887	rVV2	191	251	0.03%	0.004%
30	6.507	887	889	892	rVV	279	300	0.04%	0.005%
31	6.757	921	930	949	rBV	186416	450617	56.10%	7.264%
32	6.915	955	956	958	rBV2	375	190	0.02%	0.003%
33	7.074	980	982	983	rBV	323	254	0.03%	0.004%
34	7.104	984	987	996	rVB3	1341	3041	0.38%	0.049%
35	7.226	1006	1007	1010	rVB	297	220	0.03%	0.004%
36	7.306	1010	1020	1037	rBV	170542	371634	46.27%	5.991%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122123\
 Data File : VX039417.D
 Acq On : 21 Dec 2023 10:18
 Operator : JC/MD
 Sample : VX1221WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK657

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	7.421	1037	1039	1043	rVB3	314	374	0.05%	0.006%
38	7.769	1092	1096	1099	rVB2	183	233	0.03%	0.004%
39	7.812	1101	1103	1105	rBV	247	193	0.02%	0.003%
40	7.958	1124	1127	1129	rVV2	276	409	0.05%	0.007%
41	7.976	1129	1130	1132	rVB	428	199	0.02%	0.003%
42	8.251	1173	1175	1178	rBV2	236	264	0.03%	0.004%
43	8.324	1181	1187	1202	rBV	113210	189012	23.53%	3.047%
44	8.647	1234	1240	1251	rBV	379505	615309	76.60%	9.919%
45	8.860	1273	1275	1276	rBV2	226	199	0.02%	0.003%
46	8.952	1285	1290	1298	rBV	78817	123052	15.32%	1.984%
47	9.092	1311	1313	1317	rVB3	325	271	0.03%	0.004%
48	9.275	1340	1343	1348	rBV2	488	689	0.09%	0.011%
49	9.378	1355	1360	1381	rBV	329475	492351	61.30%	7.937%
50	9.610	1396	1398	1400	rBV3	280	201	0.03%	0.003%
51	9.671	1404	1408	1409	rBV	282	247	0.03%	0.004%
52	9.689	1409	1411	1412	rBV	281	208	0.03%	0.003%
53	9.732	1417	1418	1423	rVB	263	322	0.04%	0.005%
54	9.823	1431	1433	1435	rBV2	274	194	0.02%	0.003%
55	10.049	1465	1470	1484	rBV	385078	558640	69.55%	9.005%
56	10.311	1509	1513	1516	rBV3	446	534	0.07%	0.009%
57	10.646	1564	1568	1569	rBV2	688	585	0.07%	0.009%
58	10.963	1617	1620	1625	rVB3	623	827	0.10%	0.013%
59	11.049	1633	1634	1636	rBV2	227	186	0.02%	0.003%
60	11.189	1652	1657	1671	rVB	314393	404237	50.33%	6.516%
61	11.305	1674	1676	1681	rBV3	794	927	0.12%	0.015%
62	11.457	1698	1701	1707	rBV2	411	679	0.08%	0.011%
63	11.756	1747	1750	1753	rVB2	536	517	0.06%	0.008%
64	11.927	1773	1778	1780	rBV2	222	283	0.04%	0.005%
65	11.969	1782	1785	1788	rBV3	710	770	0.10%	0.012%
66	12.018	1788	1793	1801	rBV	437335	575694	71.67%	9.280%
67	12.317	1837	1842	1856	rBV	438754	564544	70.28%	9.100%
68	12.524	1874	1876	1880	rVB2	243	310	0.04%	0.005%
69	12.646	1894	1896	1900	rVV2	207	276	0.03%	0.004%
70	12.701	1903	1905	1909	rVB	375	355	0.04%	0.006%
71	12.762	1909	1915	1922	rBV2	3667	5061	0.63%	0.082%
72	12.957	1943	1947	1950	rBV2	410	478	0.06%	0.008%
73	13.024	1954	1958	1959	rVV2	168	224	0.03%	0.004%
74	13.042	1959	1961	1964	rVB2	222	229	0.03%	0.004%
75	13.079	1964	1967	1968	rBV	245	194	0.02%	0.003%
76	13.116	1971	1973	1978	rVB2	437	508	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122123\
 Data File : VX039417.D
 Acq On : 21 Dec 2023 10:18
 Operator : JC/MD
 Sample : VX1221WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK657

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

77	13.158	1978	1980	1982	rVB2	292	217	0.03%	0.003%
78	13.177	1982	1983	1987	rVB	261	222	0.03%	0.004%
79	13.256	1994	1996	2000	rVB	232	258	0.03%	0.004%
80	13.292	2000	2002	2004	rBV2	277	274	0.03%	0.004%
81	13.353	2009	2012	2013	rBV2	225	233	0.03%	0.004%
82	13.542	2041	2043	2046	rBV	299	257	0.03%	0.004%
83	13.591	2049	2051	2055	rVB4	637	893	0.11%	0.014%
84	13.786	2081	2083	2090	rVB3	763	897	0.11%	0.014%
85	13.859	2092	2095	2097	rBV2	245	210	0.03%	0.003%
86	13.963	2107	2112	2117	rVB3	623	1094	0.14%	0.018%
87	14.128	2134	2139	2145	rVB	4463	6450	0.80%	0.104%
88	14.304	2166	2168	2171	rBV	247	237	0.03%	0.004%
89	14.384	2178	2181	2184	rBV3	173	285	0.04%	0.005%
90	14.816	2250	2252	2253	rBV2	349	284	0.04%	0.005%
91	14.835	2253	2255	2258	rVV2	250	278	0.03%	0.004%
92	14.877	2261	2262	2265	rVB	258	192	0.02%	0.003%
93	14.908	2265	2267	2269	rVB2	424	386	0.05%	0.006%
94	14.944	2269	2273	2274	rBV3	213	308	0.04%	0.005%
95	15.005	2282	2283	2284	rBV	357	202	0.03%	0.003%
96	15.688	2393	2395	2397	rBV2	349	242	0.03%	0.004%
97	16.072	2456	2458	2463	rVB2	343	526	0.07%	0.008%
98	16.286	2491	2493	2495	rVB2	435	336	0.04%	0.005%
99	16.316	2495	2498	2501	rBV2	384	499	0.06%	0.008%
100	16.645	2550	2552	2554	rVB	335	206	0.03%	0.003%




Sum of corrected areas: 6203562

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122123\
Data File : VX039417.D
Acq On : 21 Dec 2023 10:18
Operator : JC/MD
Sample : VX1221WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK657

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

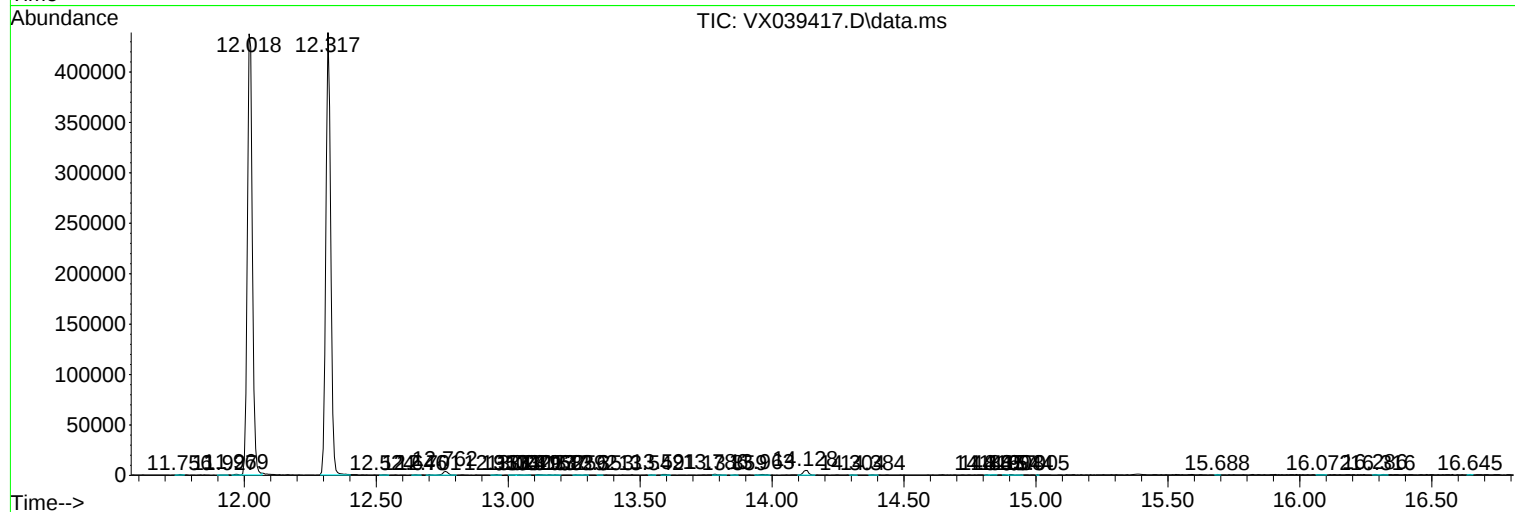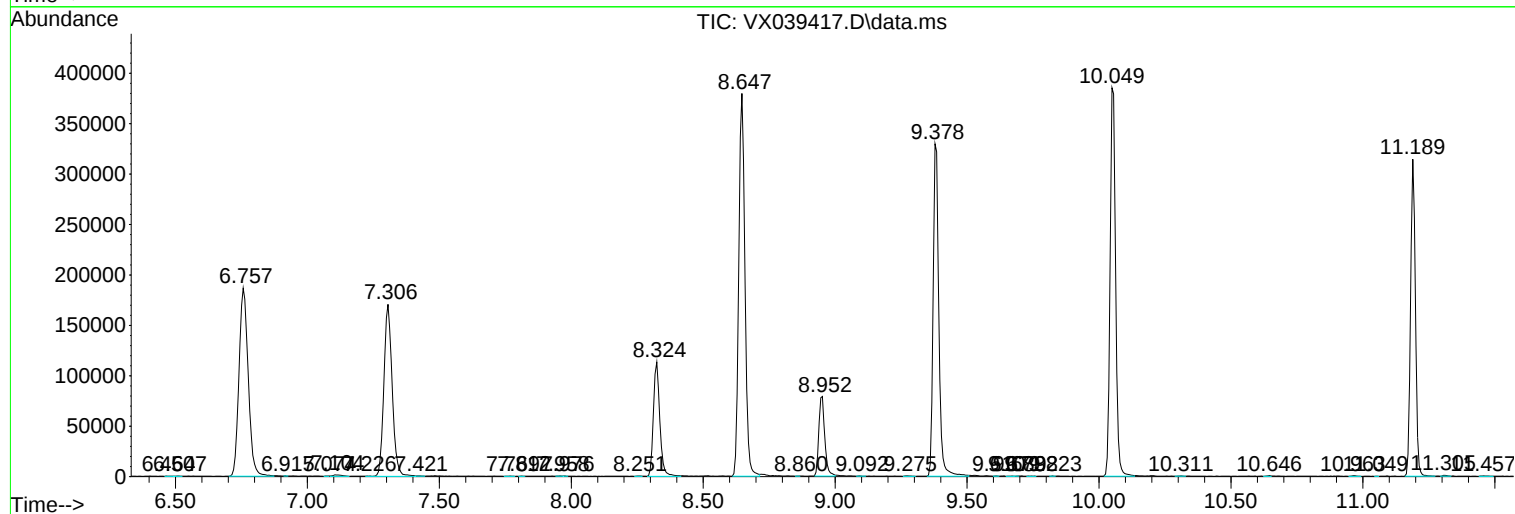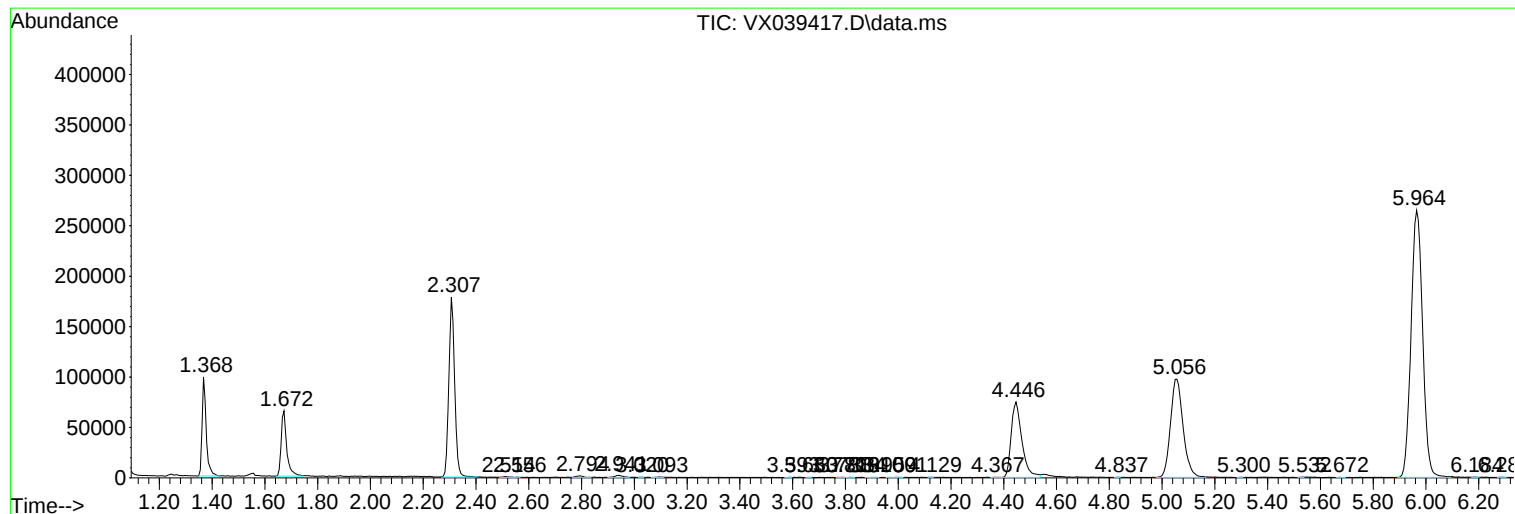

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122123\
Data File : VX039417.D
Acq On : 21 Dec 2023 10:18
Operator : JC/MD
Sample : VX1221WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK657

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122123\
Data File : VX039417.D
Acq On : 21 Dec 2023 10:18
Operator : JC/MD
Sample : VX1221WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK657

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc