

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122123\
 Data File : VX039421.D
 Acq On : 21 Dec 2023 12:01
 Operator : JC/MD
 Sample : 05807-15 10X
 Misc : 1.92g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0B00

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039421.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	58	rVB	88854	97504	11.53%	1.544%
2	1.666	90	95	112	rVB	55791	90881	10.74%	1.439%
3	2.307	194	200	209	rBV	164669	258113	30.51%	4.086%
4	2.459	224	225	228	rVB2	518	304	0.04%	0.005%
5	2.788	275	279	285	rVB4	1475	2767	0.33%	0.044%
6	2.855	288	290	291	rBV	379	353	0.04%	0.006%
7	2.947	297	305	313	rBV2	7265	17062	2.02%	0.270%
8	3.087	326	328	330	rBV	320	372	0.04%	0.006%
9	3.294	360	362	364	rBV	181	181	0.02%	0.003%
10	3.361	371	373	374	rBV2	242	198	0.02%	0.003%
11	3.556	403	405	407	rBV	289	260	0.03%	0.004%
12	3.611	412	414	417	rVV2	315	296	0.03%	0.005%
13	3.709	429	430	433	rVB	367	252	0.03%	0.004%
14	3.971	470	473	474	rBV	339	383	0.05%	0.006%
15	4.007	477	479	481	rVB2	206	191	0.02%	0.003%
16	4.044	484	485	487	rBV	261	179	0.02%	0.003%
17	4.184	506	508	509	rBV	188	178	0.02%	0.003%
18	4.270	521	522	524	rVB	286	161	0.02%	0.003%
19	4.446	543	551	567	rBV	74839	218094	25.78%	3.453%
20	5.056	639	651	667	rBV	98526	323406	38.23%	5.120%
21	5.190	672	673	677	rVB3	417	295	0.03%	0.005%
22	5.391	703	706	711	rVB4	550	860	0.10%	0.014%
23	5.446	713	715	716	rBV2	210	161	0.02%	0.003%
24	5.465	716	718	722	rVB2	363	481	0.06%	0.008%
25	5.562	730	734	739	rVB3	445	827	0.10%	0.013%
26	5.745	763	764	767	rBV2	189	194	0.02%	0.003%
27	5.824	774	777	779	rBV	219	209	0.02%	0.003%
28	5.964	788	800	821	rBV2	266772	845977	100.00%	13.393%
29	6.257	847	848	851	rBV	279	245	0.03%	0.004%
30	6.281	851	852	857	rVB2	338	371	0.04%	0.006%
31	6.324	857	859	860	rBV	217	170	0.02%	0.003%
32	6.464	880	882	885	rVB2	299	240	0.03%	0.004%
33	6.757	921	930	942	rBV	176415	430150	50.85%	6.810%
34	7.001	968	970	972	rVB	298	222	0.03%	0.004%
35	7.062	978	980	983	rBV2	277	274	0.03%	0.004%
36	7.111	983	988	997	rVB6	1249	2994	0.35%	0.047%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122123\
 Data File : VX039421.D
 Acq On : 21 Dec 2023 12:01
 Operator : JC/MD
 Sample : 05807-15 10X
 Misc : 1.92g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0B00

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	7.190	999	1001	1006	rVB2	191	289	0.03%	0.005%
38	7.306	1011	1020	1035	rBV	172197	379479	44.86%	6.007%
39	7.995	1132	1133	1137	rVB2	300	270	0.03%	0.004%
40	8.037	1139	1140	1143	rBV2	242	236	0.03%	0.004%
41	8.177	1162	1163	1165	rVB	310	177	0.02%	0.003%
42	8.251	1174	1175	1178	rVB2	334	252	0.03%	0.004%
43	8.324	1181	1187	1199	rVV	111566	186997	22.10%	2.960%
44	8.586	1225	1230	1234	rBV3	682	1252	0.15%	0.020%
45	8.647	1234	1240	1257	rBV	403675	631476	74.64%	9.997%
46	8.836	1268	1271	1274	rBV2	418	430	0.05%	0.007%
47	8.946	1284	1289	1303	rBV	79746	124153	14.68%	1.965%
48	9.226	1334	1335	1337	rBV	217	176	0.02%	0.003%
49	9.281	1341	1344	1346	rVB2	306	394	0.05%	0.006%
50	9.330	1350	1352	1355	rBV	209	249	0.03%	0.004%
51	9.385	1355	1361	1378	rBV	353678	514406	60.81%	8.144%
52	9.555	1388	1389	1392	rBV2	421	275	0.03%	0.004%
53	9.695	1410	1412	1417	rVB3	1042	1430	0.17%	0.023%
54	9.836	1434	1435	1437	rBV2	209	203	0.02%	0.003%
55	10.055	1465	1471	1473	rBV	386301	578189	68.35%	9.153%
56	10.195	1491	1494	1498	rVB3	930	1251	0.15%	0.020%
57	10.317	1510	1514	1515	rBV2	504	608	0.07%	0.010%
58	10.646	1565	1568	1570	rBV2	535	622	0.07%	0.010%
59	10.671	1570	1572	1575	rVB2	383	302	0.04%	0.005%
60	10.896	1607	1609	1611	rBV	268	218	0.03%	0.003%
61	10.964	1617	1620	1624	rVB	399	487	0.06%	0.008%
62	11.189	1652	1657	1668	rVV	331482	422609	49.96%	6.690%
63	11.317	1672	1678	1682	rBV3	1186	1886	0.22%	0.030%
64	11.457	1697	1701	1704	rBV	584	855	0.10%	0.014%
65	11.482	1704	1705	1708	rVB	370	277	0.03%	0.004%
66	11.537	1712	1714	1717	rBV2	210	222	0.03%	0.004%
67	11.750	1747	1749	1751	rBV	343	380	0.04%	0.006%
68	11.908	1773	1775	1776	rBV	174	162	0.02%	0.003%
69	11.976	1783	1786	1788	rBV2	846	890	0.11%	0.014%
70	12.018	1788	1793	1807	rVV	428727	554321	65.52%	8.775%
71	12.219	1824	1826	1829	rVV2	209	167	0.02%	0.003%
72	12.317	1837	1842	1850	rBV	456427	589044	69.63%	9.325%
73	12.482	1868	1869	1873	rBV2	219	255	0.03%	0.004%
74	12.524	1875	1876	1878	rVB	387	162	0.02%	0.003%
75	12.762	1911	1915	1920	rVB2	3515	4530	0.54%	0.072%
76	12.981	1950	1951	1953	rVB2	243	176	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122123\
 Data File : VX039421.D
 Acq On : 21 Dec 2023 12:01
 Operator : JC/MD
 Sample : 05807-15 10X
 Misc : 1.92g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0B00

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

77	13.116	1971	1973	1976	rVB3	491	498	0.06%	0.008%
78	13.164	1979	1981	1983	rBV	366	349	0.04%	0.006%
79	13.311	2004	2005	2009	rBV2	237	323	0.04%	0.005%
80	13.555	2042	2045	2046	rBV	227	257	0.03%	0.004%
81	13.591	2047	2051	2059	rVB2	4598	6389	0.76%	0.101%
82	13.646	2059	2060	2063	rBV2	278	260	0.03%	0.004%
83	13.695	2066	2068	2070	rBV	244	176	0.02%	0.003%
84	13.780	2079	2082	2083	rBV2	652	525	0.06%	0.008%
85	13.957	2109	2111	2116	rVB2	1295	1589	0.19%	0.025%
86	14.128	2135	2139	2144	rVB	4342	5547	0.66%	0.088%
87	14.286	2161	2165	2166	rVB2	193	196	0.02%	0.003%
88	14.615	2217	2219	2223	rBV3	183	185	0.02%	0.003%
89	14.810	2249	2251	2253	rBV	247	264	0.03%	0.004%
90	14.890	2262	2264	2267	rBV3	244	262	0.03%	0.004%
91	14.957	2273	2275	2276	rBB	328	178	0.02%	0.003%
92	15.048	2286	2290	2292	rBV	346	416	0.05%	0.007%
93	15.091	2295	2297	2300	rVB2	358	232	0.03%	0.004%
94	15.243	2318	2322	2329	rBV5	1538	2952	0.35%	0.047%
95	15.316	2332	2334	2336	rBV2	344	313	0.04%	0.005%
96	15.365	2341	2342	2343	rBV	298	182	0.02%	0.003%
97	15.707	2396	2398	2399	rBV	418	188	0.02%	0.003%
98	15.871	2423	2425	2427	rBV	401	367	0.04%	0.006%
99	16.395	2509	2511	2514	rBV3	209	232	0.03%	0.004%
100	16.505	2526	2529	2530	rBV2	375	325	0.04%	0.005%

Sum of corrected areas: 6316767




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122123\
Data File : VX039421.D
Acq On : 21 Dec 2023 12:01
Operator : JC/MD
Sample : 05807-15 10X
Misc : 1.92g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0B00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

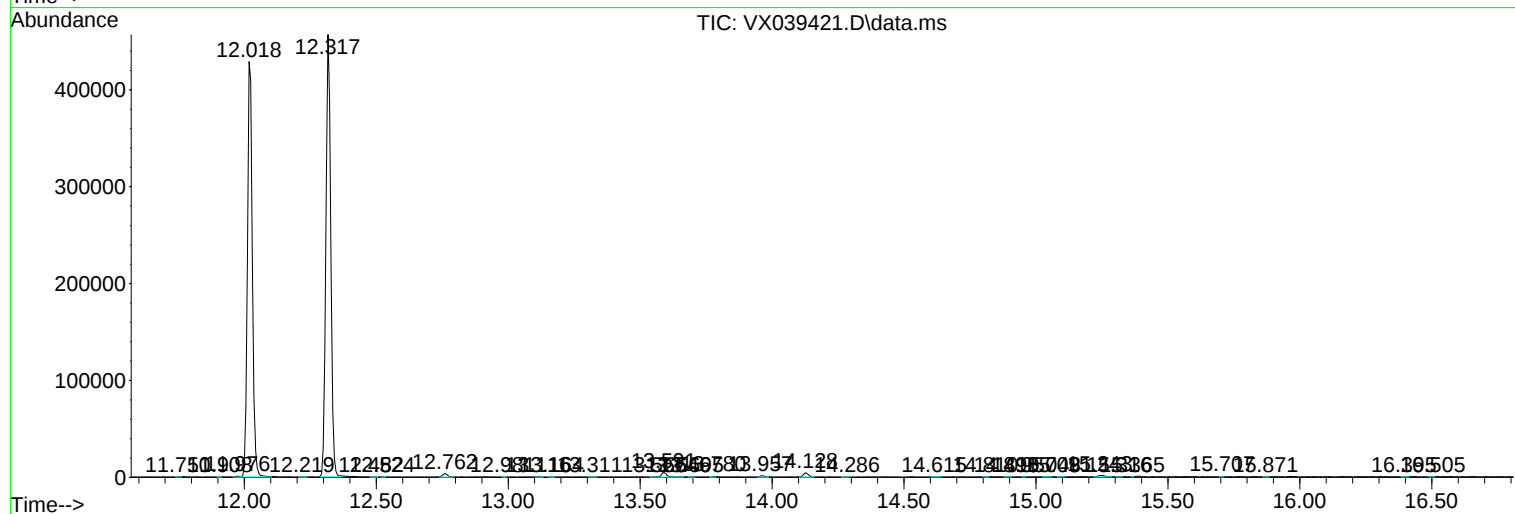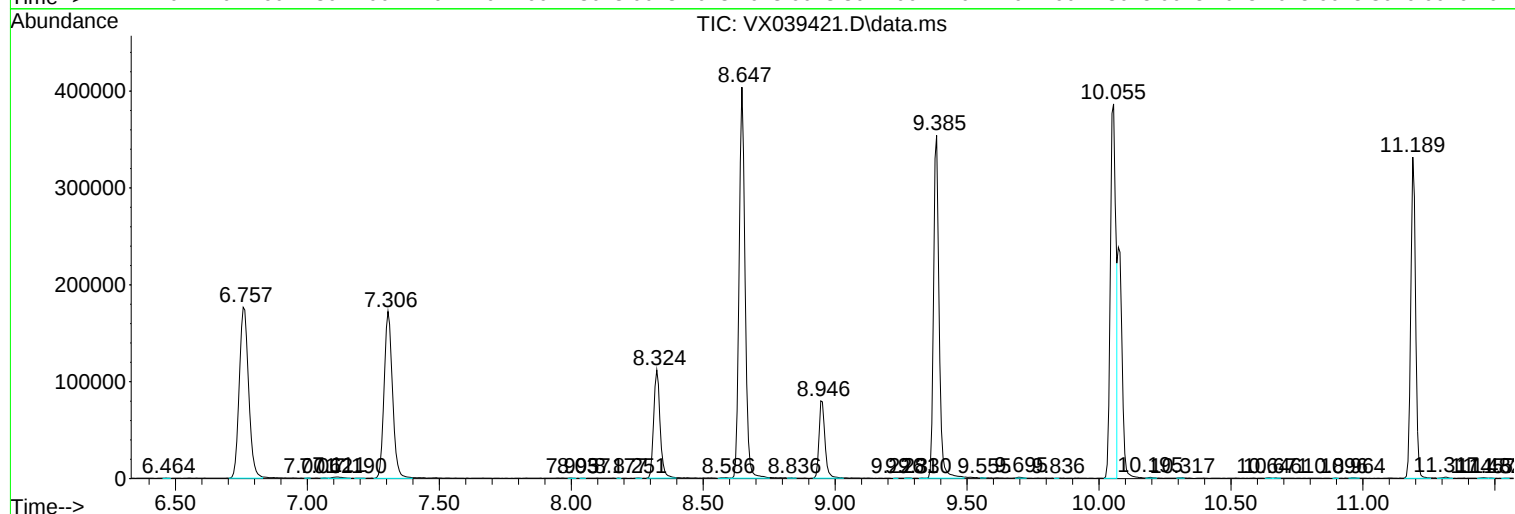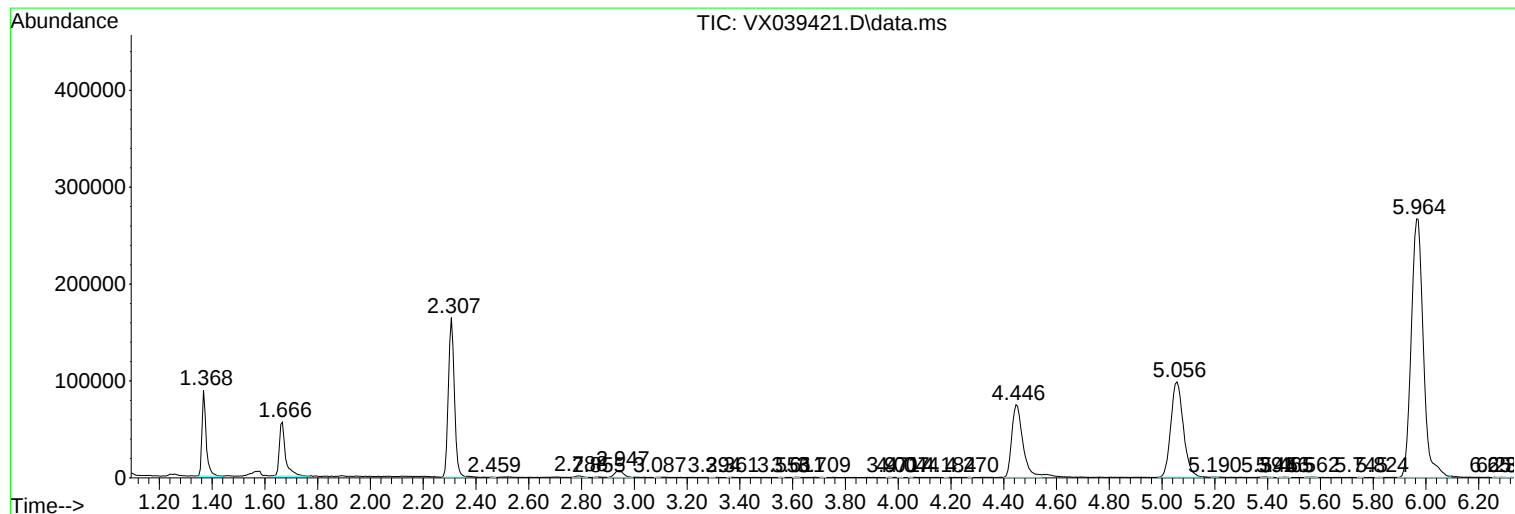

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122123\
Data File : VX039421.D
Acq On : 21 Dec 2023 12:01
Operator : JC/MD
Sample : 05807-15 10X
Misc : 1.92g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0B00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122123\
Data File : VX039421.D
Acq On : 21 Dec 2023 12:01
Operator : JC/MD
Sample : 05807-15 10X
Misc : 1.92g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0B00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------