

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122123\
 Data File : VX039424.D
 Acq On : 21 Dec 2023 13:10
 Operator : JC/MD
 Sample : 05808-02ME
 Misc : 1.92g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COB23ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039424.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	59	rBV	87650	139392	11.74%	1.510%
2	1.648	89	92	99	rVB	26628	36548	3.08%	0.396%
3	2.288	191	197	210	rBV	229784	361908	30.49%	3.920%
4	2.398	212	215	229	rVB4	3499	8519	0.72%	0.092%
5	2.715	260	267	274	rBV	7976	16565	1.40%	0.179%
6	2.776	275	277	284	rVB5	1884	3505	0.30%	0.038%
7	2.947	298	305	317	rVB2	10418	26969	2.27%	0.292%
8	3.117	331	333	339	rVB3	808	1253	0.11%	0.014%
9	3.428	379	384	385	rBV	436	581	0.05%	0.006%
10	3.520	396	399	400	rVB2	249	234	0.02%	0.003%
11	3.544	400	403	405	rBV2	217	277	0.02%	0.003%
12	3.818	447	448	452	rBV3	395	500	0.04%	0.005%
13	3.898	457	461	465	rVB2	201	390	0.03%	0.004%
14	3.940	465	468	471	rBV2	231	337	0.03%	0.004%
15	3.983	474	475	479	rVB2	200	221	0.02%	0.002%
16	4.044	482	485	486	rBV2	199	221	0.02%	0.002%
17	4.471	547	555	584	rBV	68533	311917	26.28%	3.378%
18	4.965	635	636	638	rBV	265	242	0.02%	0.003%
19	5.056	638	651	670	rVV2	136352	469270	39.53%	5.082%
20	5.379	701	704	706	rBV3	355	386	0.03%	0.004%
21	5.538	728	730	732	rBV	305	353	0.03%	0.004%
22	5.574	732	736	738	rVV2	388	399	0.03%	0.004%
23	5.666	747	751	752	rBV3	170	218	0.02%	0.002%
24	5.763	765	767	769	rBV	310	293	0.02%	0.003%
25	5.964	788	800	807	rBV2	404769	1187025	100.00%	12.856%
26	6.184	834	836	840	rVB3	443	500	0.04%	0.005%
27	6.361	860	865	867	rBV3	948	1471	0.12%	0.016%
28	6.757	920	930	945	rBV	282241	694645	58.52%	7.523%
29	7.117	982	989	997	rVB5	1973	5368	0.45%	0.058%
30	7.214	1000	1005	1011	rVV5	1525	3526	0.30%	0.038%
31	7.306	1012	1020	1036	rVB	245531	545242	45.93%	5.905%
32	7.482	1045	1049	1051	rBV4	699	991	0.08%	0.011%
33	7.653	1075	1077	1079	rBV	351	305	0.03%	0.003%
34	7.964	1123	1128	1131	rBV4	977	1562	0.13%	0.017%
35	8.263	1173	1177	1178	rBV3	473	641	0.05%	0.007%
36	8.324	1181	1187	1200	rBV	149176	263564	22.20%	2.855%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122123\
 Data File : VX039424.D
 Acq On : 21 Dec 2023 13:10
 Operator : JC/MD
 Sample : 05808-02ME
 Misc : 1.92g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0B23ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

37	8.433	1203	1205	1208	rVB4	293	285	0.02%	0.003%
38	8.494	1212	1215	1216	rBV2	382	441	0.04%	0.005%
39	8.598	1227	1232	1233	rBV3	577	883	0.07%	0.010%
40	8.647	1233	1240	1250	rBV	571361	907441	76.45%	9.828%
41	8.854	1273	1274	1277	rBV	313	316	0.03%	0.003%
42	8.903	1280	1282	1283	rBV	353	253	0.02%	0.003%
43	8.952	1284	1290	1304	rBV	106974	175622	14.80%	1.902%
44	9.165	1323	1325	1330	rVB2	455	476	0.04%	0.005%
45	9.275	1340	1343	1348	rBV3	774	1095	0.09%	0.012%
46	9.397	1356	1363	1385	rBV	399872	717722	60.46%	7.773%
47	9.708	1411	1414	1418	rVB3	1420	1870	0.16%	0.020%
48	9.884	1442	1443	1447	rBV2	201	295	0.02%	0.003%
49	10.055	1465	1471	1473	rBV	601170	895550	75.44%	9.699%
50	10.268	1505	1506	1509	rVB2	414	260	0.02%	0.003%
51	10.311	1509	1513	1521	rVB3	948	1829	0.15%	0.020%
52	10.409	1526	1529	1532	rVB2	241	278	0.02%	0.003%
53	10.494	1541	1543	1547	rVV2	231	246	0.02%	0.003%
54	10.525	1547	1548	1553	rVB2	310	333	0.03%	0.004%
55	10.646	1564	1568	1578	rVB5	975	2414	0.20%	0.026%
56	10.738	1581	1583	1585	rBV	182	222	0.02%	0.002%
57	10.829	1595	1598	1602	rBV2	260	375	0.03%	0.004%
58	10.970	1615	1621	1625	rBV4	897	1394	0.12%	0.015%
59	11.098	1640	1642	1646	rVB2	442	377	0.03%	0.004%
60	11.195	1652	1658	1670	rBV	464402	585779	49.35%	6.344%
61	11.311	1673	1677	1682	rVB2	2785	3831	0.32%	0.041%
62	11.372	1683	1687	1691	rVB	1882	2169	0.18%	0.023%
63	11.427	1694	1696	1697	rBV	598	458	0.04%	0.005%
64	11.451	1698	1700	1704	rVB2	654	711	0.06%	0.008%
65	11.591	1720	1723	1726	rBV	327	288	0.02%	0.003%
66	11.677	1735	1737	1740	rBB2	292	326	0.03%	0.004%
67	11.707	1740	1742	1744	rBV	389	349	0.03%	0.004%
68	11.750	1746	1749	1753	rBV3	872	1426	0.12%	0.015%
69	11.884	1769	1771	1773	rBV	488	267	0.02%	0.003%
70	11.975	1781	1786	1788	rBV2	4133	4894	0.41%	0.053%
71	12.024	1788	1794	1807	rVB	681122	941214	79.29%	10.194%
72	12.225	1823	1827	1831	rBV3	2463	4189	0.35%	0.045%
73	12.323	1837	1843	1857	rVB	635861	835857	70.42%	9.053%
74	12.506	1870	1873	1874	rBV2	359	278	0.02%	0.003%
75	12.634	1892	1894	1895	rBV	409	225	0.02%	0.002%
76	12.762	1909	1915	1922	rVB2	10385	14153	1.19%	0.153%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122123\
 Data File : VX039424.D
 Acq On : 21 Dec 2023 13:10
 Operator : JC/MD
 Sample : 05808-02ME
 Misc : 1.92g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0B23ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	12.872	1928	1933	1934	rVV2	267	406	0.03%	0.004%
78	12.908	1937	1939	1941	rVB	331	253	0.02%	0.003%
79	13.116	1970	1973	1977	rVB	1019	1084	0.09%	0.012%
80	13.158	1977	1980	1983	rBV2	182	295	0.02%	0.003%
81	13.268	1994	1998	2003	rVB2	615	915	0.08%	0.010%
82	13.335	2006	2009	2014	rVV3	1086	1458	0.12%	0.016%
83	13.591	2047	2051	2061	rBV3	4866	7091	0.60%	0.077%
84	13.750	2075	2077	2079	rVV	606	332	0.03%	0.004%
85	13.786	2079	2083	2085	rBV2	544	711	0.06%	0.008%
86	13.963	2108	2112	2116	rBV2	2430	2961	0.25%	0.032%
87	14.128	2134	2139	2148	rVB	10064	13621	1.15%	0.148%
88	14.280	2160	2164	2165	rBV	228	251	0.02%	0.003%
89	14.707	2231	2234	2235	rBV	181	233	0.02%	0.003%
90	14.871	2259	2261	2262	rBV	346	328	0.03%	0.004%
91	15.249	2318	2323	2328	rBV3	5209	7699	0.65%	0.083%
92	15.633	2384	2386	2389	rBV2	318	356	0.03%	0.004%
93	15.755	2404	2406	2408	rBV	331	392	0.03%	0.004%
94	15.993	2443	2445	2449	rBV2	261	313	0.03%	0.003%
95	16.048	2452	2454	2457	rBV2	363	445	0.04%	0.005%
96	16.310	2495	2497	2499	rBV	395	335	0.03%	0.004%
97	16.450	2518	2520	2522	rVB2	458	321	0.03%	0.003%
98	16.505	2526	2529	2532	rVB3	826	1078	0.09%	0.012%
99	16.639	2550	2551	2553	rBV2	337	280	0.02%	0.003%
100	16.731	2564	2566	2567	rVB	430	250	0.02%	0.003%


Sum of corrected areas: 9233137

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122123\
Data File : VX039424.D
Acq On : 21 Dec 2023 13:10
Operator : JC/MD
Sample : 05808-02ME
Misc : 1.92g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0B23ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

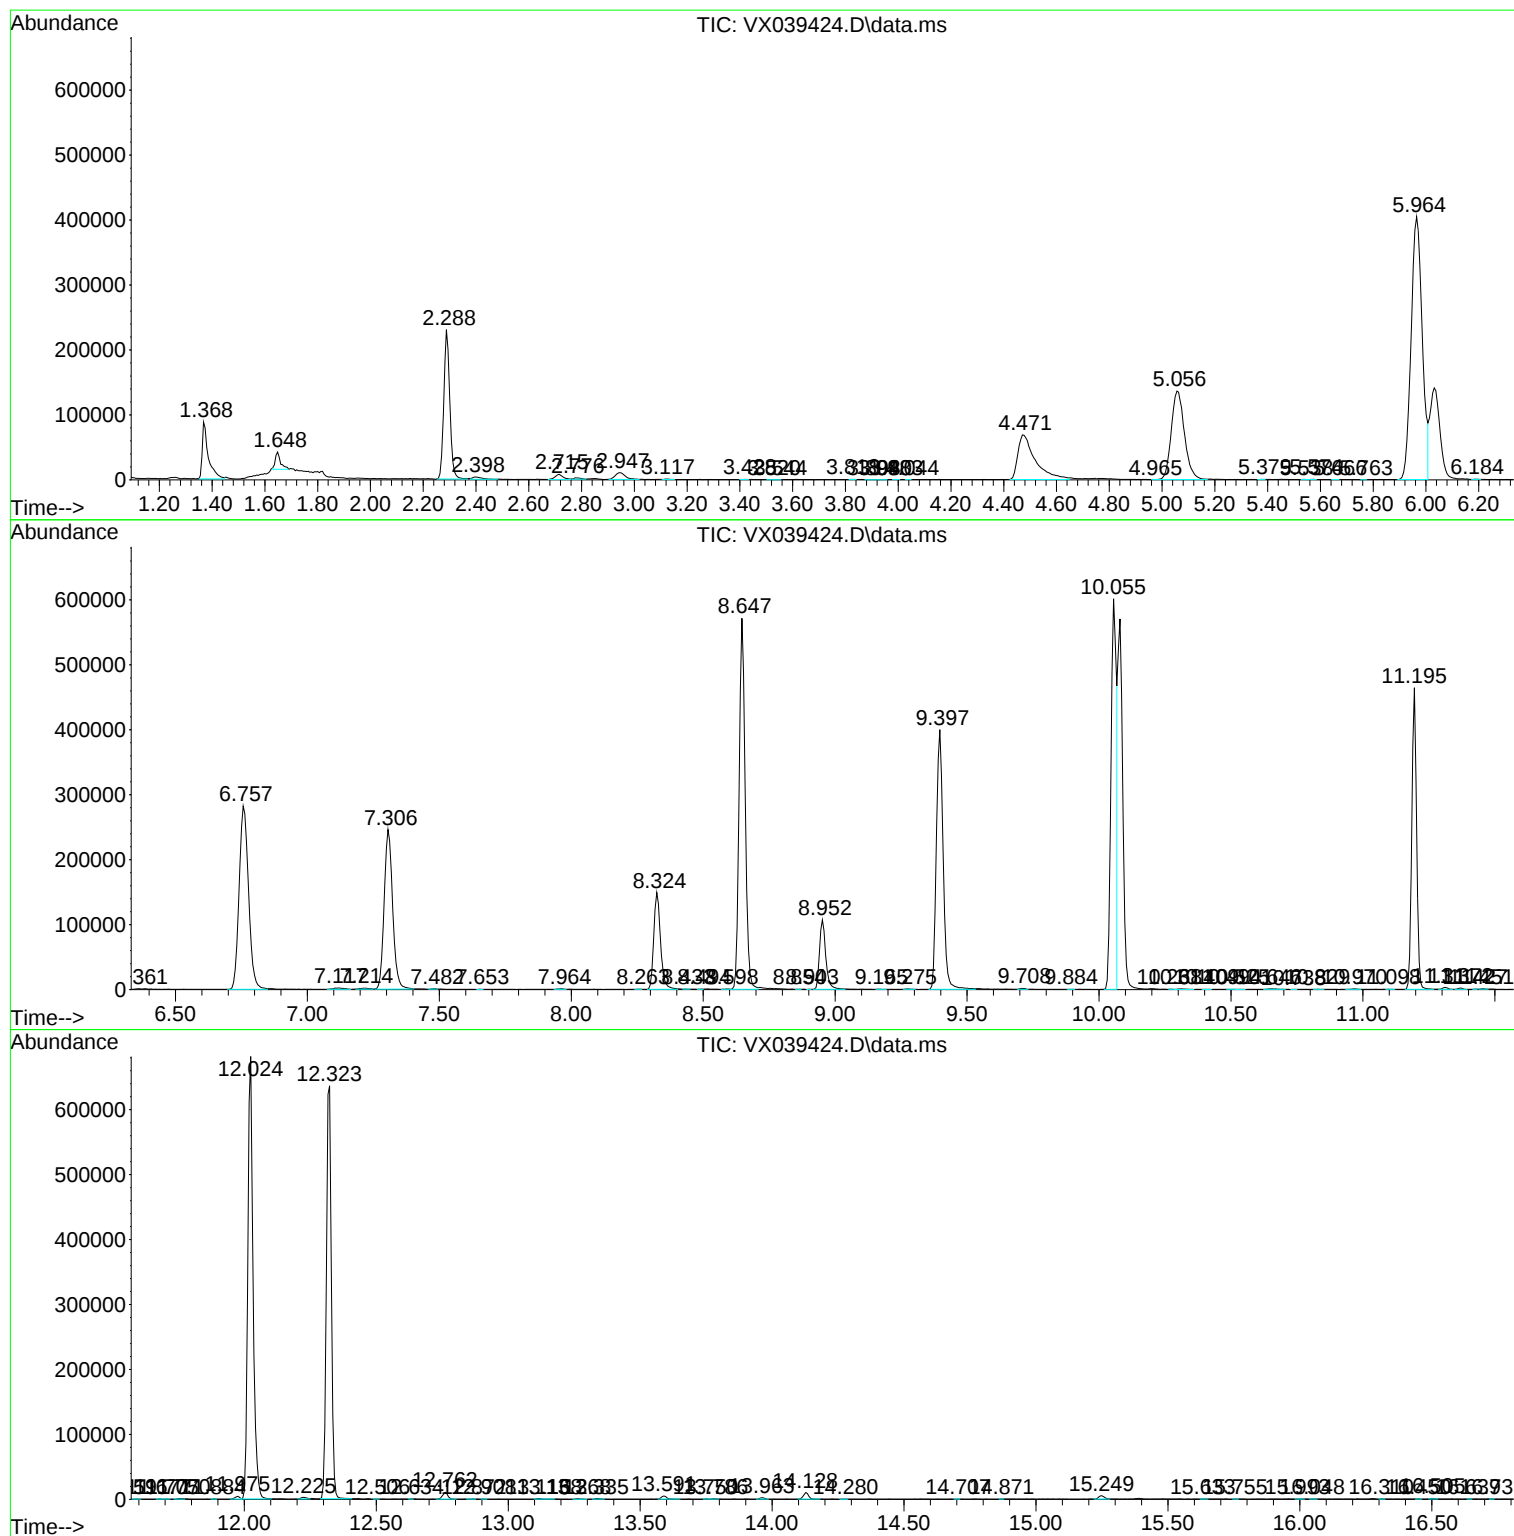

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122123\
Data File : VX039424.D
Acq On : 21 Dec 2023 13:10
Operator : JC/MD
Sample : 05808-02ME
Misc : 1.92g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0B23ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122123\
Data File : VX039424.D
Acq On : 21 Dec 2023 13:10
Operator : JC/MD
Sample : 05808-02ME
Misc : 1.92g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0B23ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------