

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122123\
 Data File : VX039428.D
 Acq On : 21 Dec 2023 15:09
 Operator : JC/MD
 Sample : 05807-15 4X
 Misc : 1.92g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0B00

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039428.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	23	25	27	rBV	2481	2785	0.19%	0.034%
2	1.368	43	46	57	rVB	89144	109556	7.55%	1.355%
3	1.648	89	92	104	rVB	49187	79570	5.49%	0.984%
4	2.300	193	199	208	rBV	182020	279415	19.26%	3.456%
5	2.496	230	231	233	rBV	323	268	0.02%	0.003%
6	2.709	260	266	270	rVB3	863	1608	0.11%	0.020%
7	2.782	274	278	287	rVB4	1910	3645	0.25%	0.045%
8	2.861	287	291	293	rBV2	305	507	0.03%	0.006%
9	2.941	296	304	312	rBV	11256	27087	1.87%	0.335%
10	3.099	328	330	336	rVV3	581	935	0.06%	0.012%
11	3.148	336	338	340	rVV2	206	247	0.02%	0.003%
12	3.172	340	342	344	rVV	305	234	0.02%	0.003%
13	3.319	362	366	370	rBV2	260	442	0.03%	0.005%
14	3.367	370	374	376	rVB	260	274	0.02%	0.003%
15	3.605	409	413	414	rVV3	247	258	0.02%	0.003%
16	3.666	422	423	428	rVB	289	248	0.02%	0.003%
17	3.818	445	448	450	rVB2	205	279	0.02%	0.003%
18	3.977	471	474	476	rBV2	205	281	0.02%	0.003%
19	4.007	476	479	481	rBV	315	252	0.02%	0.003%
20	4.282	522	524	526	rVB	285	262	0.02%	0.003%
21	4.446	542	551	570	rBV	89138	263714	18.18%	3.262%
22	5.050	638	650	675	rBV	109225	363043	25.03%	4.490%
23	5.379	700	704	705	rBV	330	338	0.02%	0.004%
24	5.477	717	720	724	rVB2	352	480	0.03%	0.006%
25	5.538	727	730	732	rBV2	213	306	0.02%	0.004%
26	5.623	740	744	745	rBV2	181	226	0.02%	0.003%
27	5.812	774	775	780	rVB2	246	250	0.02%	0.003%
28	5.958	787	799	808	rBV2	299178	918898	63.36%	11.365%
29	6.318	856	858	860	rBV2	366	372	0.03%	0.005%
30	6.568	897	899	902	rVB2	239	244	0.02%	0.003%
31	6.751	920	929	945	rBV	227884	547707	37.76%	6.774%
32	6.922	954	957	962	rBV3	362	733	0.05%	0.009%
33	7.074	980	982	983	rBV	271	261	0.02%	0.003%
34	7.104	983	987	988	rBV2	1231	1475	0.10%	0.018%
35	7.196	1001	1002	1006	rVB	262	251	0.02%	0.003%
36	7.300	1010	1019	1037	rBV	185707	422228	29.11%	5.222%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122123\
 Data File : VX039428.D
 Acq On : 21 Dec 2023 15:09
 Operator : JC/MD
 Sample : 05807-15 4X
 Misc : 1.92g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0B00

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	7.470	1044	1047	1048	rBV3	305	298	0.02%	0.004%
38	7.708	1084	1086	1090	rVB2	279	278	0.02%	0.003%
39	7.751	1090	1093	1096	rBV	294	272	0.02%	0.003%
40	7.793	1096	1100	1102	rBV2	238	286	0.02%	0.004%
41	7.824	1104	1105	1107	rBV	322	253	0.02%	0.003%
42	8.062	1143	1144	1147	rBV	262	273	0.02%	0.003%
43	8.214	1167	1169	1171	rBV2	250	283	0.02%	0.004%
44	8.251	1171	1175	1180	rVV2	3020	3649	0.25%	0.045%
45	8.318	1180	1186	1199	rBV	121973	205816	14.19%	2.545%
46	8.513	1212	1218	1222	rBV5	406	1072	0.07%	0.013%
47	8.580	1225	1229	1233	rBV2	840	1429	0.10%	0.018%
48	8.647	1233	1240	1260	rBV	418066	685816	47.28%	8.482%
49	8.946	1284	1289	1303	rBV	90928	138217	9.53%	1.709%
50	9.159	1322	1324	1327	rBV	204	249	0.02%	0.003%
51	9.275	1338	1343	1345	rBV3	521	648	0.04%	0.008%
52	9.385	1355	1361	1378	rBV	428726	623035	42.96%	7.706%
53	9.702	1410	1413	1417	rVB3	1024	1420	0.10%	0.018%
54	9.964	1454	1456	1460	rBV2	221	266	0.02%	0.003%
55	10.073	1472	1474	1491	rVB	1110126	1450389	100.00%	17.938%
56	10.305	1508	1512	1518	rVV4	823	1310	0.09%	0.016%
57	10.421	1529	1531	1533	rVB2	274	242	0.02%	0.003%
58	10.439	1533	1534	1537	rBV	234	249	0.02%	0.003%
59	10.470	1537	1539	1542	rBV2	237	216	0.01%	0.003%
60	10.610	1561	1562	1565	rVB	326	217	0.01%	0.003%
61	10.640	1565	1567	1569	rBV2	854	963	0.07%	0.012%
62	10.963	1616	1620	1623	rVB2	633	873	0.06%	0.011%
63	11.110	1640	1644	1645	rBV	345	241	0.02%	0.003%
64	11.189	1652	1657	1671	rVV	377852	488238	33.66%	6.038%
65	11.311	1671	1677	1681	rVB3	1812	2299	0.16%	0.028%
66	11.451	1697	1700	1704	rBV2	710	820	0.06%	0.010%
67	11.549	1714	1716	1718	rVB2	272	217	0.01%	0.003%
68	11.585	1718	1722	1723	rBV	195	279	0.02%	0.003%
69	11.604	1723	1725	1730	rVB2	239	264	0.02%	0.003%
70	11.658	1732	1734	1738	rBV2	162	266	0.02%	0.003%
71	11.750	1747	1749	1755	rVB3	577	743	0.05%	0.009%
72	11.969	1782	1785	1788	rVV3	1185	1349	0.09%	0.017%
73	12.018	1788	1793	1806	rVV	557039	730338	50.35%	9.033%
74	12.128	1810	1811	1815	rVV4	592	725	0.05%	0.009%
75	12.177	1817	1819	1824	rVV3	348	457	0.03%	0.006%
76	12.317	1837	1842	1856	rBV	541642	683017	47.09%	8.447%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122123\
 Data File : VX039428.D
 Acq On : 21 Dec 2023 15:09
 Operator : JC/MD
 Sample : 05807-15 4X
 Misc : 1.92g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0B00

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	12.762	1910	1915	1920	rVB	5478	7154	0.49%	0.088%
78	12.811	1920	1923	1925	rBV2	249	247	0.02%	0.003%
79	12.896	1934	1937	1940	rVB2	254	314	0.02%	0.004%
80	12.963	1946	1948	1952	rVB2	217	301	0.02%	0.004%
81	13.122	1970	1974	1978	rVB4	249	431	0.03%	0.005%
82	13.518	2036	2039	2040	rBV2	211	278	0.02%	0.003%
83	13.591	2047	2051	2058	rBV2	1271	1908	0.13%	0.024%
84	13.780	2080	2082	2085	rVB2	397	451	0.03%	0.006%
85	13.963	2110	2112	2115	rBV2	757	860	0.06%	0.011%
86	14.128	2135	2139	2145	rVB	10027	12554	0.87%	0.155%
87	14.201	2149	2151	2154	rBV2	207	275	0.02%	0.003%
88	14.402	2180	2184	2185	rBV2	181	247	0.02%	0.003%
89	14.640	2219	2223	2225	rBV2	185	220	0.02%	0.003%
90	14.999	2278	2282	2285	rBV2	252	501	0.03%	0.006%
91	15.249	2321	2323	2324	rBV	305	232	0.02%	0.003%
92	15.383	2341	2345	2350	rVV3	625	1128	0.08%	0.014%
93	15.682	2393	2394	2396	rBV	392	280	0.02%	0.003%
94	15.822	2415	2417	2419	rVB	442	285	0.02%	0.004%
95	15.926	2433	2434	2437	rBV2	387	310	0.02%	0.004%
96	16.017	2448	2449	2452	rBV	354	332	0.02%	0.004%
97	16.200	2477	2479	2482	rBV2	299	321	0.02%	0.004%
98	16.536	2532	2534	2537	rBV3	393	493	0.03%	0.006%
99	16.664	2552	2555	2556	rBV2	251	248	0.02%	0.003%
100	16.731	2564	2566	2567	rBV	347	236	0.02%	0.003%




Sum of corrected areas: 8085557

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122123\
Data File : VX039428.D
Acq On : 21 Dec 2023 15:09
Operator : JC/MD
Sample : 05807-15 4X
Misc : 1.92g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0B00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

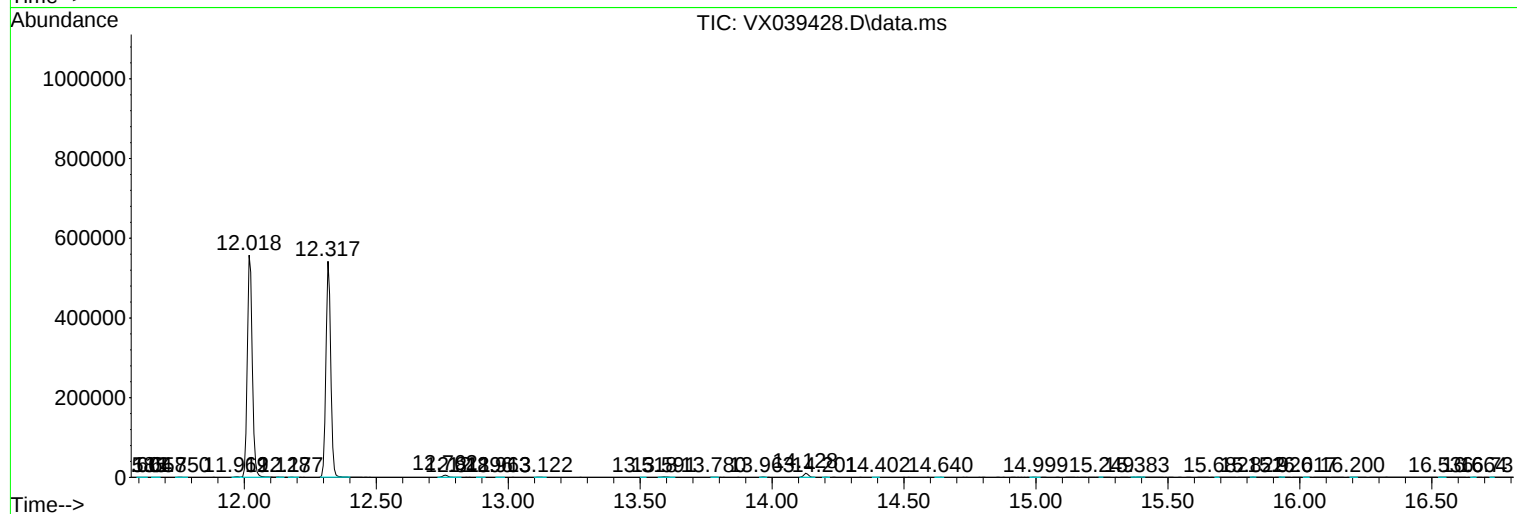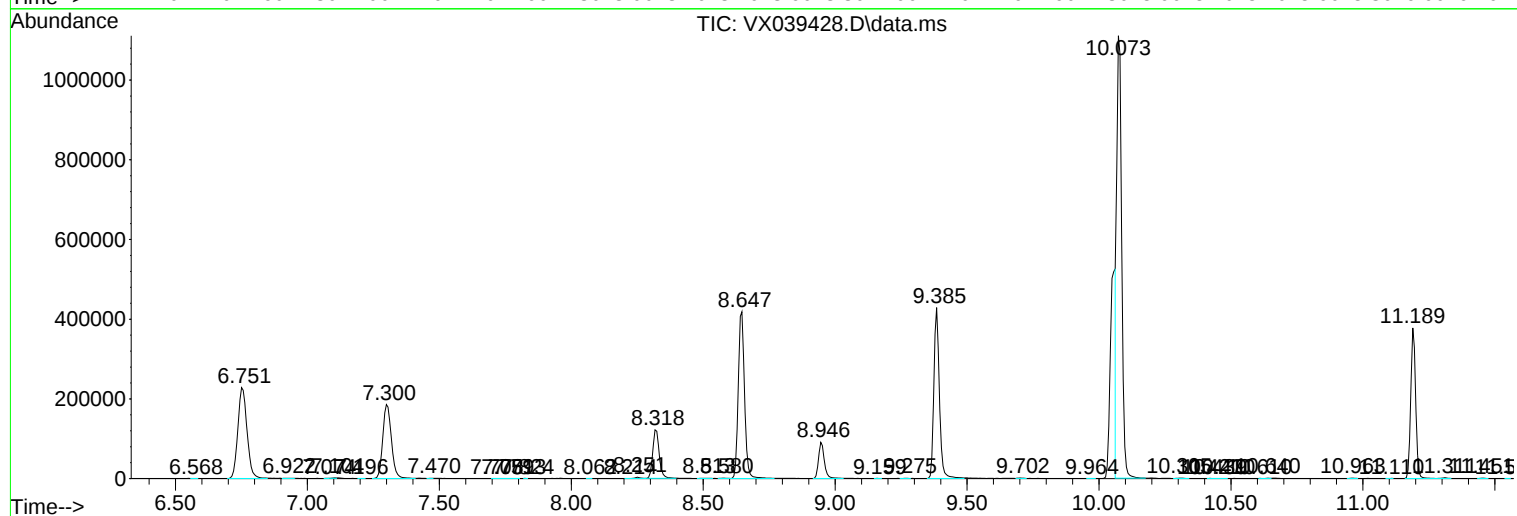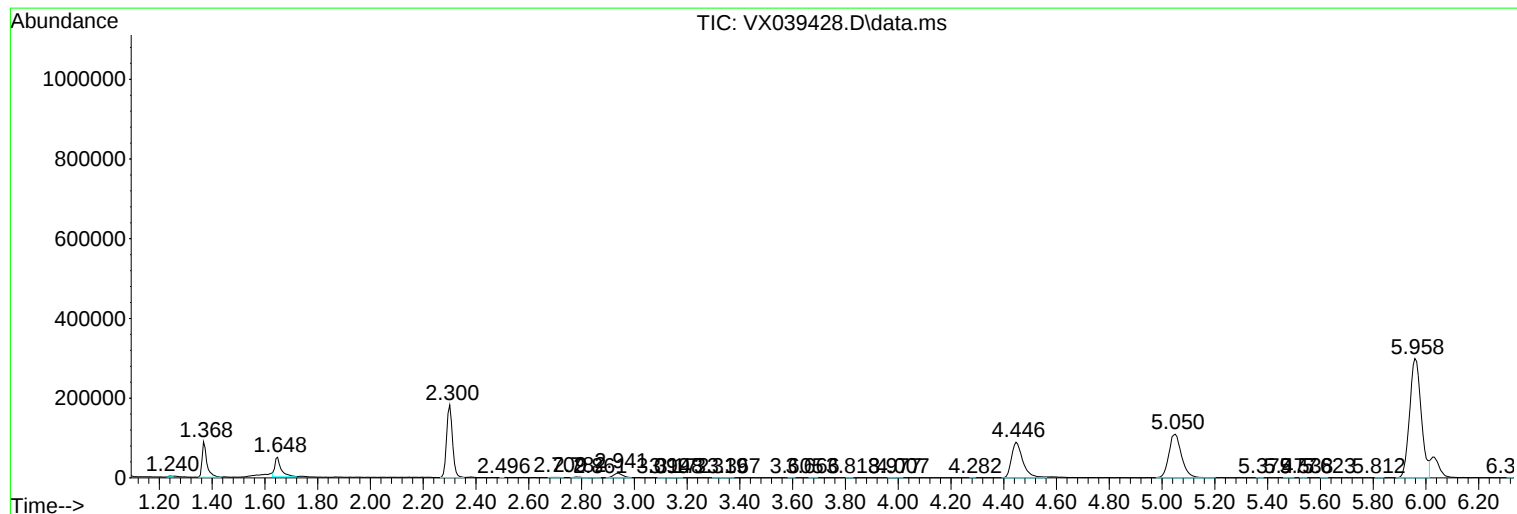

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122123\
Data File : VX039428.D
Acq On : 21 Dec 2023 15:09
Operator : JC/MD
Sample : 05807-15 4X
Misc : 1.92g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0B00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122123\
Data File : VX039428.D
Acq On : 21 Dec 2023 15:09
Operator : JC/MD
Sample : 05807-15 4X
Misc : 1.92g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0B00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc