
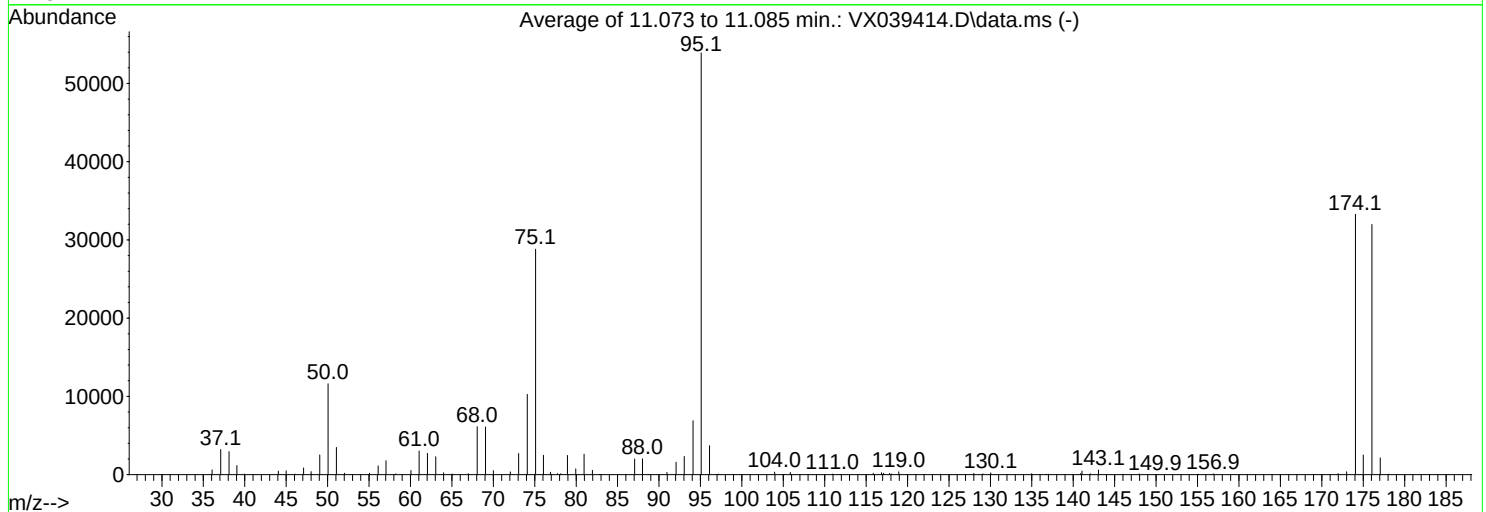


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122123\
Data File : VX039414.D
Acq On : 21 Dec 2023 08:43
Operator : JC/MD
Sample : BFB659
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB659

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Title : VOC Analysis
Last Update : Fri Dec 22 00:41:09 2023

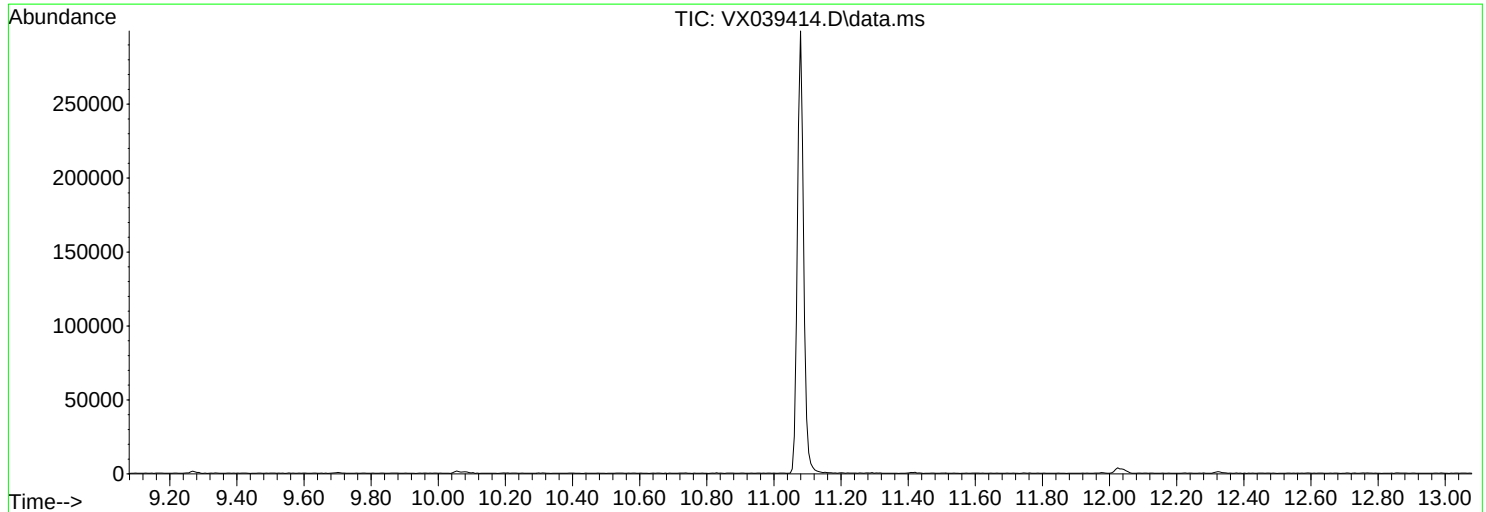

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.5	11614	PASS
75	95	30	80	53.4	28813	PASS
95	95	100	100	100.0	53912	PASS
96	95	5	9	6.9	3711	PASS
173	174	0.00	2	1.1	360	PASS
174	95	50	120	61.7	33267	PASS
175	174	5	9	7.5	2506	PASS
176	174	95	101	96.2	31992	PASS
177	176	5	9	6.7	2157	PASS

m/z	Abundance
40.00	274.0
44.10	172.0

Instrument :
MSVOA_X
ClientSampleId :
BFB659

m/z	Abundance
36.00	595.0
37.10	3226.0
38.10	3017.0
39.10	1256.0
40.00	359.0
44.10	656.0
45.00	580.0
46.10	105.0
47.10	725.0
48.00	422.0
49.10	2444.0
50.10	11296.0
51.00	3520.0
52.10	219.0
55.10	207.0
56.10	995.0
57.00	1783.0
58.30	141.0
60.00	558.0
61.10	2827.0
62.00	2645.0
63.10	2152.0
64.00	258.0
65.10	56.0
67.10	77.0
68.00	6002.0
69.00	5961.0
70.00	561.0
72.00	261.0
73.10	2860.0
74.10	10083.0
75.10	28640.0
76.00	2517.0
77.00	244.0
77.70	148.0
78.20	211.0
78.90	2373.0
79.90	703.0
81.00	2533.0
82.00	573.0
82.80	57.0
87.00	2086.0
88.00	2130.0
90.90	251.0
92.00	1475.0
93.10	2068.0
94.10	6747.0
95.10	51704.0
96.10	3659.0
97.20	122.0
104.00	284.0
105.10	83.0
105.80	185.0
110.90	86.0
116.00	153.0
116.80	431.0
118.10	231.0
118.90	312.0
124.00	94.0
128.00	179.0
128.90	78.0
130.10	173.0
135.00	102.0
137.00	54.0
140.90	465.0
142.10	125.0
143.10	548.0
148.00	127.0
157.10	52.0
159.00	62.0
172.00	130.0
173.00	306.0
174.10	26480.0
175.00	1929.0
176.00	26480.0
177.00	1867.0

Instrument :
MSVOA_X
ClientSampleId :
BFB659

m/z	Abundance
36.10	710.0
37.10	3892.0
38.10	3524.0
39.00	1366.0
39.90	340.0
44.00	648.0
45.00	549.0
46.00	120.0
47.10	869.0
48.00	481.0
49.10	2858.0
50.10	13844.0
51.10	4337.0
52.10	177.0
54.90	177.0
56.10	1295.0
57.00	2163.0
58.20	78.0
60.10	489.0
61.10	3501.0
62.00	3313.0
63.00	2928.0
63.90	304.0
65.00	78.0
66.90	118.0
68.10	7420.0
69.00	7038.0
70.00	587.0
72.10	495.0
73.00	3156.0
74.10	12157.0
75.10	33824.0
76.00	2847.0
76.90	404.0
77.80	202.0
78.90	3070.0
80.00	848.0
81.00	3100.0
81.90	589.0
83.00	69.0
86.00	68.0
87.10	2154.0
88.00	2168.0
90.90	360.0
92.10	1811.0
93.00	2741.0
94.10	8084.0
95.10	64392.0
96.10	4386.0
97.00	51.0
104.00	386.0
105.10	62.0
105.90	432.0
111.00	116.0
111.90	61.0
115.80	247.0
117.10	568.0
117.80	352.0
118.90	448.0
124.00	84.0
128.00	159.0
129.10	196.0
130.10	259.0
135.00	155.0
136.70	147.0
141.10	690.0
142.00	85.0
143.00	591.0
146.10	100.0
148.00	96.0
155.10	119.0
156.90	90.0
159.00	53.0
172.00	123.0
173.00	320.0
174.00	39784.0
175.00	3298.0
176.10	37512.0
177.10	2643.0
178.10	95.0

Instrument :
MSVOA_X
ClientSampleId :
BFB659

m/z	Abundance
36.00	511.0
37.10	2516.0
38.10	2275.0
39.10	883.0
40.00	363.0
44.00	580.0
45.10	343.0
46.90	508.0
47.20	502.0
47.90	286.0
49.00	2243.0
50.00	9703.0
51.00	2597.0
52.00	176.0
55.10	196.0
56.10	1102.0
57.10	1369.0
58.20	91.0
60.10	555.0
61.00	2752.0
62.10	2200.0
63.10	1808.0
64.10	186.0
65.00	87.0
67.00	169.0
68.00	5007.0
69.10	5260.0
70.00	381.0
72.10	320.0
73.10	2064.0
74.10	8582.0
75.10	23976.0
76.10	2046.0
76.80	258.0
78.10	147.0
79.00	1934.0
79.90	636.0
80.90	2206.0
81.90	470.0
86.00	54.0
87.00	1761.0
88.00	1792.0
88.80	56.0
91.00	248.0
92.10	1508.0
93.00	2213.0
94.10	5879.0
95.10	45640.0
96.10	3087.0
96.90	59.0
97.20	84.0
103.90	312.0
105.90	272.0
111.00	58.0
111.90	63.0
113.00	91.0
115.80	178.0
116.90	323.0
117.90	174.0
119.00	357.0
128.00	137.0
129.10	110.0
130.00	232.0
135.00	88.0
137.00	118.0
141.00	715.0
142.00	111.0
143.00	651.0
145.90	109.0
147.80	83.0
149.90	92.0
155.10	72.0
156.90	154.0
171.90	153.0
173.00	454.0
174.10	33536.0
175.00	2291.0
176.10	31984.0
177.00	1962.0
178.10	71.0

Instrument :
MSVOA_X
ClientSampleId :
BFB659