


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX122218\
 Data File : VX006761.D
 Acq On : 22 Dec 2018 09:53
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X121818W.M
 Title : SW846 8260
 Last Update : Wed Dec 19 15:20:58 2018

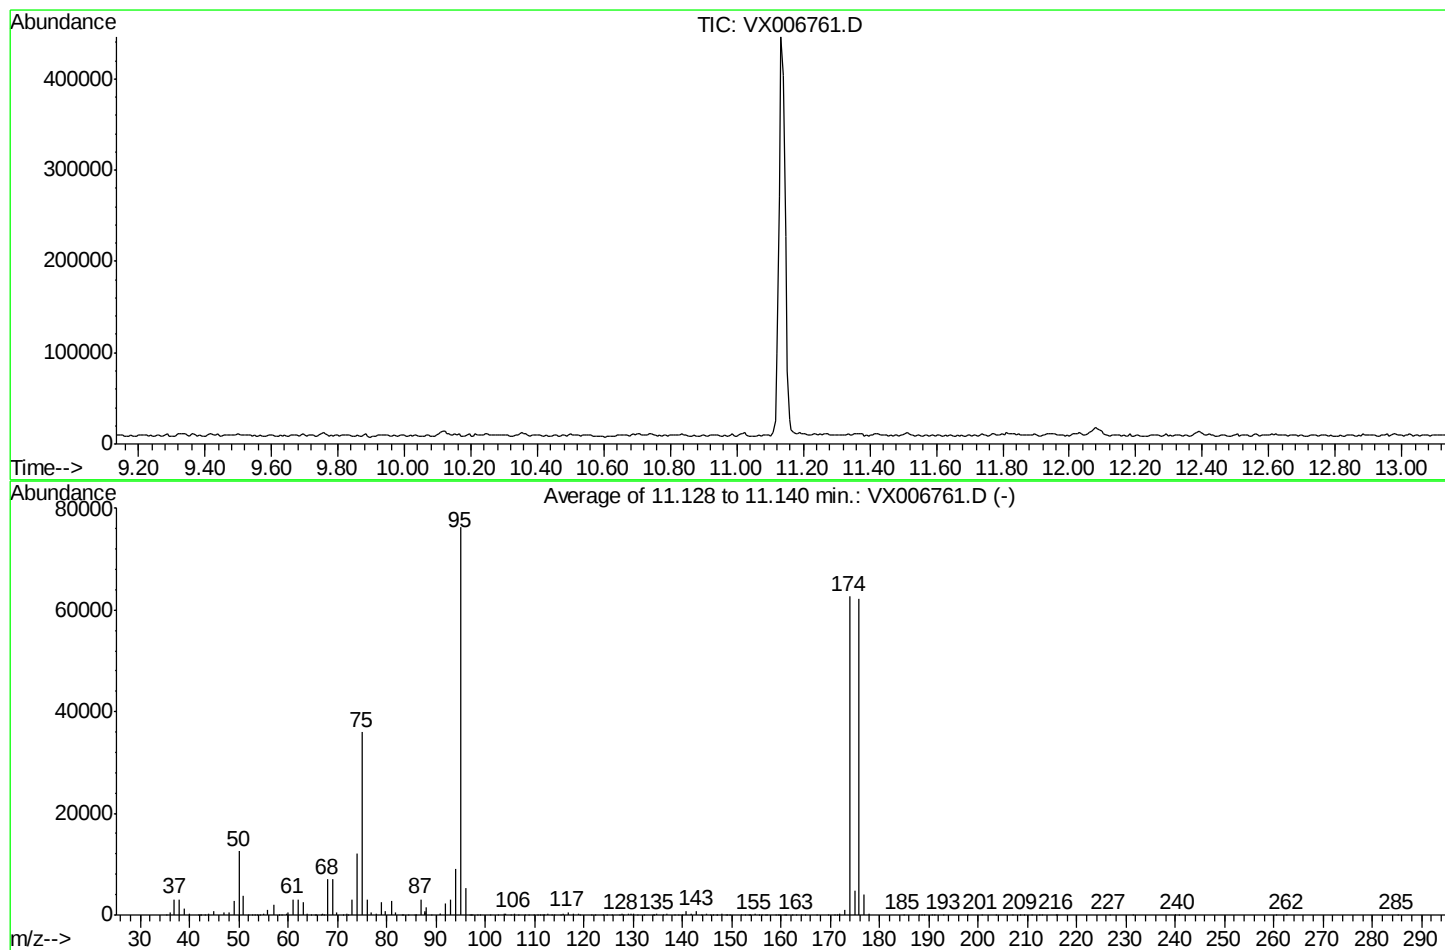

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	12566	PASS
75	95	30	60	47.1	35935	PASS
95	95	100	100	100.0	76264	PASS
96	95	5	9	6.9	5292	PASS
173	174	0.00	2	1.4	900	PASS
174	95	50	100	82.1	62618	PASS
175	174	5	9	7.7	4791	PASS
176	174	95	101	99.4	62250	PASS
177	176	5	9	6.4	3980	PASS