
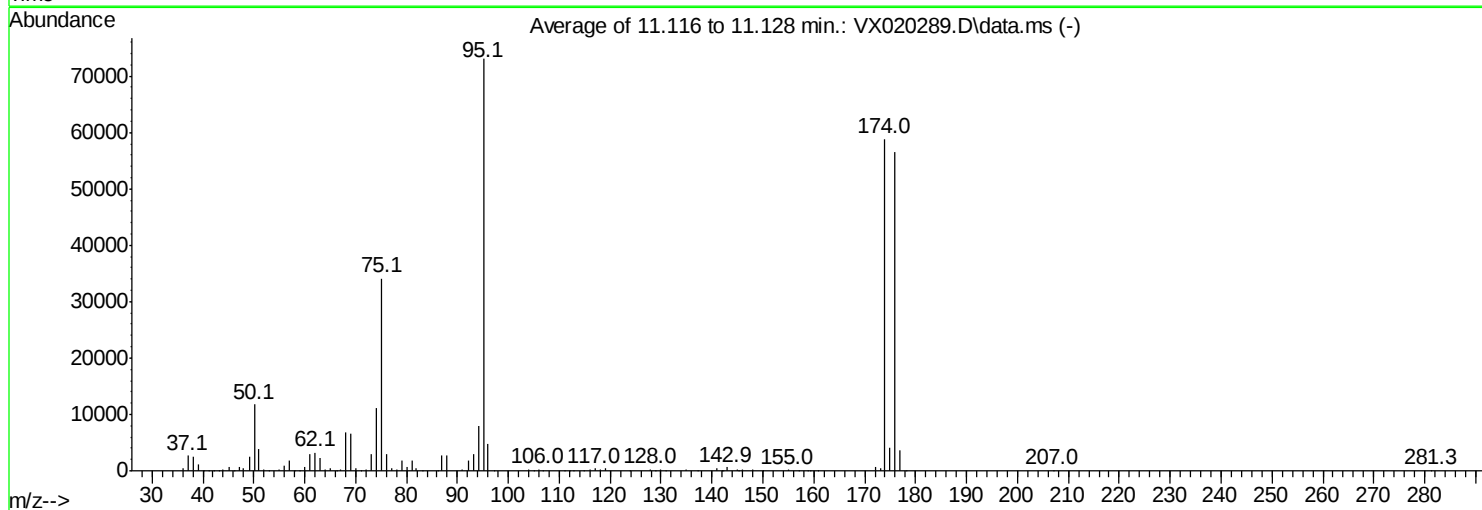


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122220\
 Data File : VX020289.D
 Acq On : 22 Dec 2020 07:57
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X121820W.M
 Title : SW846 8260
 Last Update : Fri Dec 18 13:09:49 2020

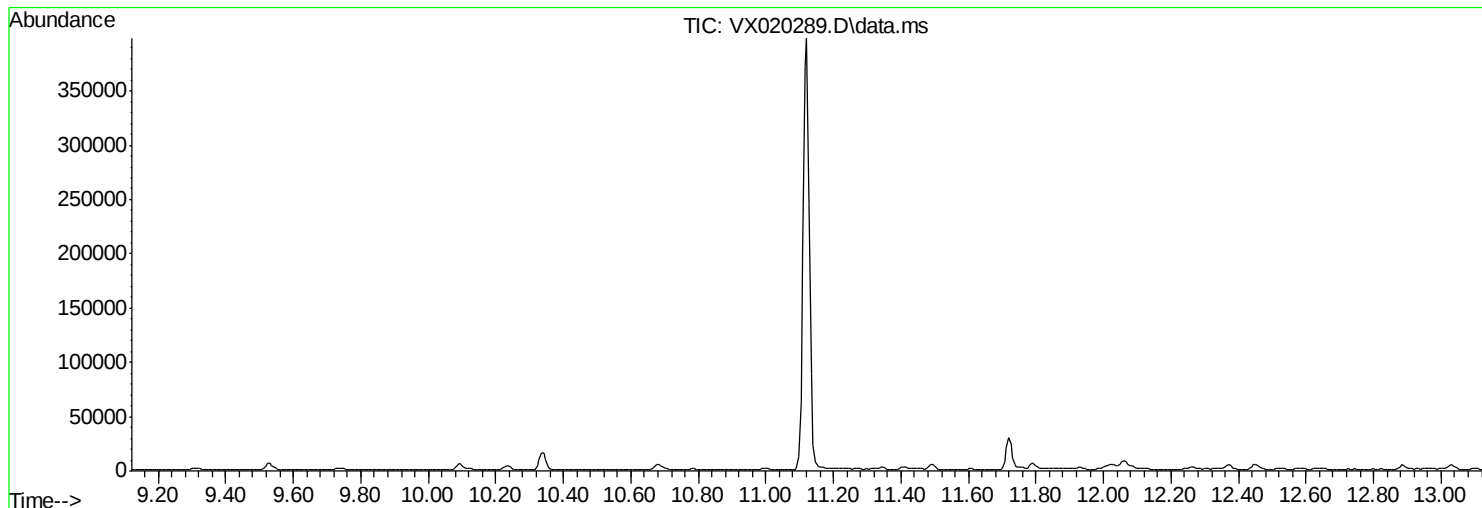

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	11807	PASS
75	95	30	60	46.7	34147	PASS
95	95	100	100	100.0	73075	PASS
96	95	5	9	6.4	4681	PASS
173	174	0.00	2	0.8	483	PASS
174	95	50	100	80.5	58813	PASS
175	174	5	9	7.0	4109	PASS
176	174	95	101	96.0	56440	PASS
177	176	5	9	6.3	3570	PASS