

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122222\
 Data File : VX033545.D
 Acq On : 22 Dec 2022 15:13
 Operator : JC/MD
 Sample : VIBLK602
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK602

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122222WMA.M
 Title : VOC Analysis

Signal : TIC: VX033545.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	27	29	31	rVB2	711	597	0.06%	0.008%
2	1.295	31	34	38	rVV3	727	1357	0.14%	0.019%
3	1.368	42	46	67	rVB	87266	115983	12.24%	1.644%
4	1.624	84	88	91	rBV3	1007	1538	0.16%	0.022%
5	1.672	91	96	116	rVB	67860	98210	10.36%	1.392%
6	1.892	129	132	136	rVB3	1271	1661	0.18%	0.024%
7	2.307	194	200	212	rBV	150791	242986	25.64%	3.443%
8	2.514	228	234	243	rBV2	3966	7224	0.76%	0.102%
9	2.624	250	252	257	rVB	152	181	0.02%	0.003%
10	2.715	263	267	270	rBV2	367	709	0.07%	0.010%
11	2.794	275	280	287	rVV3	1798	3260	0.34%	0.046%
12	3.014	312	316	317	rVB2	160	186	0.02%	0.003%
13	3.099	323	330	342	rVB4	2753	6159	0.65%	0.087%
14	3.251	353	355	358	rVB	217	196	0.02%	0.003%
15	3.349	368	371	374	rVB	178	201	0.02%	0.003%
16	3.538	399	402	406	rVB2	178	314	0.03%	0.004%
17	3.581	406	409	410	rBV	246	177	0.02%	0.003%
18	3.611	410	414	417	rVV3	497	832	0.09%	0.012%
19	3.666	422	423	425	rBV3	203	191	0.02%	0.003%
20	3.697	425	428	431	rVB	257	321	0.03%	0.005%
21	3.928	463	466	468	rBV	120	189	0.02%	0.003%
22	3.977	470	474	476	rBV2	152	243	0.03%	0.003%
23	4.465	542	554	572	rBV	57883	174319	18.40%	2.470%
24	4.910	618	627	629	rBV2	702	1459	0.15%	0.021%
25	5.056	639	651	670	rBV	123815	384630	40.59%	5.450%
26	5.202	673	675	679	rVB3	380	468	0.05%	0.007%
27	5.233	679	680	683	rBV2	240	174	0.02%	0.002%
28	5.263	683	685	690	rVB	166	245	0.03%	0.003%
29	5.312	690	693	694	rBV2	161	172	0.02%	0.002%
30	5.379	699	704	705	rBV3	847	1201	0.13%	0.017%
31	5.477	714	720	726	rVB5	1194	2995	0.32%	0.042%
32	5.562	728	734	742	rVB2	1617	3363	0.35%	0.048%
33	5.653	747	749	750	rBV	184	177	0.02%	0.003%
34	5.684	750	754	757	rBV3	663	914	0.10%	0.013%
35	5.971	789	801	820	rBV2	320176	947618	100.00%	13.428%
36	6.257	844	848	850	rVB2	157	174	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122222\
 Data File : VX033545.D
 Acq On : 22 Dec 2022 15:13
 Operator : JC/MD
 Sample : VIBLK602
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK602

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122222WMA.M
 Title : VOC Analysis

37	6.306	854	856	860	rBB2	136	177	0.02%	0.003%
38	6.428	874	876	880	rVB2	216	312	0.03%	0.004%
39	6.470	880	883	884	rBV2	336	414	0.04%	0.006%
40	6.763	922	931	945	rVV	229015	542874	57.29%	7.693%
41	7.123	982	990	999	rVV6	3270	8373	0.88%	0.119%
42	7.312	1012	1021	1030	rBV	188951	414453	43.74%	5.873%
43	7.476	1046	1048	1055	rVB3	344	663	0.07%	0.009%
44	7.617	1067	1071	1073	rBV2	102	188	0.02%	0.003%
45	7.824	1101	1105	1111	rVB4	506	1113	0.12%	0.016%
46	7.885	1111	1115	1118	rBV2	129	206	0.02%	0.003%
47	7.934	1118	1123	1128	rBV2	1674	3159	0.33%	0.045%
48	8.324	1181	1187	1199	rBV	131902	217749	22.98%	3.086%
49	8.482	1209	1213	1219	rBV2	974	1852	0.20%	0.026%
50	8.580	1225	1229	1233	rBV3	1064	1392	0.15%	0.020%
51	8.647	1234	1240	1249	rVV	510319	808623	85.33%	11.459%
52	8.720	1249	1252	1260	rVB	3169	5767	0.61%	0.082%
53	8.952	1284	1290	1304	rVV	98496	145015	15.30%	2.055%
54	9.159	1321	1324	1329	rBV4	1248	1539	0.16%	0.022%
55	9.275	1339	1343	1349	rVB2	4164	6190	0.65%	0.088%
56	9.385	1356	1361	1376	rBV	282031	394676	41.65%	5.593%
57	9.525	1381	1384	1388	rVB2	853	1145	0.12%	0.016%
58	9.616	1394	1399	1405	rBV2	965	1671	0.18%	0.024%
59	9.854	1437	1438	1442	rVB2	198	228	0.02%	0.003%
60	9.945	1452	1453	1456	rVB2	219	170	0.02%	0.002%
61	9.982	1456	1459	1461	rBV2	139	199	0.02%	0.003%
62	10.055	1465	1471	1485	rVV	446577	618779	65.30%	8.768%
63	10.153	1485	1487	1489	rVV2	232	193	0.02%	0.003%
64	10.195	1491	1494	1500	rVB	4466	5892	0.62%	0.083%
65	10.305	1507	1512	1518	rBV	4445	6421	0.68%	0.091%
66	10.653	1563	1569	1575	rBV4	5141	10389	1.10%	0.147%
67	10.750	1582	1585	1587	rBV2	175	211	0.02%	0.003%
68	10.805	1590	1594	1597	rVB2	714	980	0.10%	0.014%
69	10.909	1607	1611	1613	rBV2	143	210	0.02%	0.003%
70	10.964	1616	1620	1626	rVB2	5355	6351	0.67%	0.090%
71	11.189	1652	1657	1664	rBV	330671	446141	47.08%	6.322%
72	11.451	1696	1700	1705	rVV2	6152	7267	0.77%	0.103%
73	11.689	1735	1739	1742	rVV	2489	3113	0.33%	0.044%
74	11.756	1745	1750	1755	rBV	5904	7592	0.80%	0.108%
75	11.969	1780	1785	1789	rBV	7262	9667	1.02%	0.137%
76	12.024	1789	1794	1806	rVB	472854	599134	63.23%	8.490%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122222\
 Data File : VX033545.D
 Acq On : 22 Dec 2022 15:13
 Operator : JC/MD
 Sample : VIBLK602
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK602

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122222WMA.M
 Title : VOC Analysis

77	12.317	1837	1842	1853	rBV	541658	707065	74.61%	10.019%
78	12.811	1921	1923	1924	rBV	208	177	0.02%	0.003%
79	12.847	1927	1929	1935	rVB3	229	344	0.04%	0.005%
80	12.945	1943	1945	1949	rVB2	669	660	0.07%	0.009%
81	13.036	1957	1960	1961	rVB2	204	180	0.02%	0.003%
82	13.067	1961	1965	1966	rBV2	230	314	0.03%	0.004%
83	13.116	1968	1973	1979	rVB	10966	13810	1.46%	0.196%
84	13.585	2046	2050	2058	rVB	12674	16420	1.73%	0.233%
85	13.774	2077	2081	2090	rVB	11756	15892	1.68%	0.225%
86	13.896	2098	2101	2107	rBV2	155	346	0.04%	0.005%
87	13.963	2107	2112	2117	rVV	11920	16119	1.70%	0.228%
88	14.134	2138	2140	2143	rVB2	165	180	0.02%	0.003%
89	14.219	2151	2154	2158	rBV4	408	574	0.06%	0.008%
90	14.438	2184	2190	2193	rBV2	1077	1341	0.14%	0.019%
91	14.518	2199	2203	2204	rBV2	157	187	0.02%	0.003%
92	14.567	2209	2211	2216	rBV3	290	440	0.05%	0.006%
93	14.871	2257	2261	2262	rBV2	232	248	0.03%	0.004%
94	15.152	2305	2307	2308	rBV	274	220	0.02%	0.003%
95	15.426	2349	2352	2354	rBV2	318	371	0.04%	0.005%
96	15.444	2354	2355	2357	rBV	245	174	0.02%	0.002%
97	16.048	2452	2454	2455	rBV	235	195	0.02%	0.003%
98	16.219	2481	2482	2485	rBV2	166	198	0.02%	0.003%
99	16.542	2533	2535	2537	rVB	278	186	0.02%	0.003%
100	16.615	2546	2547	2549	rBV	315	205	0.02%	0.003%


Sum of corrected areas: 7056958

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122222\
Data File : VX033545.D
Acq On : 22 Dec 2022 15:13
Operator : JC/MD
Sample : VIBLK602
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK602

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

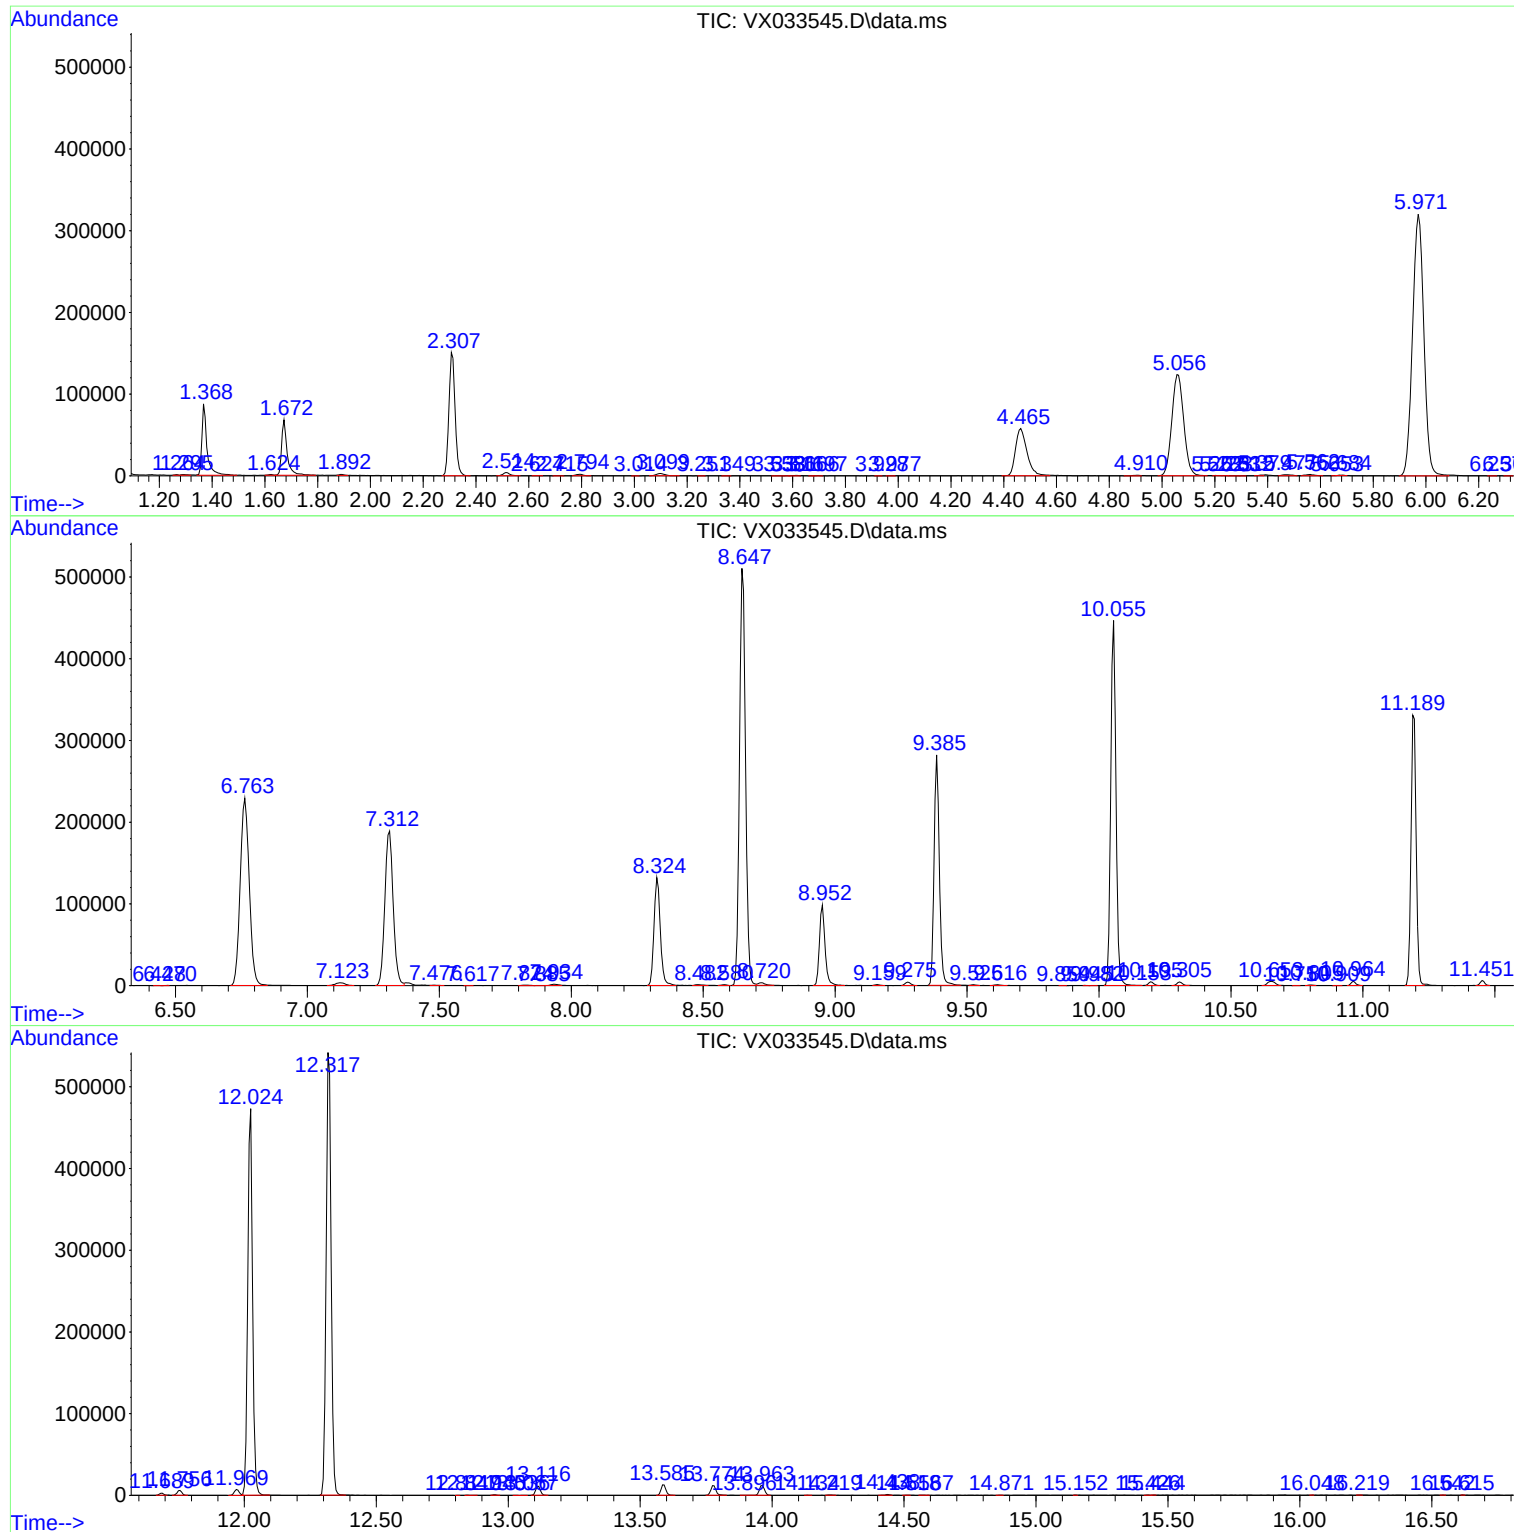

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122222\
Data File : VX033545.D
Acq On : 22 Dec 2022 15:13
Operator : JC/MD
Sample : VIBLK602
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK602

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122222\
Data File : VX033545.D
Acq On : 22 Dec 2022 15:13
Operator : JC/MD
Sample : VIBLK602
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK602

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc