

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122222\
 Data File : VX033548.D
 Acq On : 22 Dec 2022 16:34
 Operator : JC/MD
 Sample : VX1222WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK604

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122222WMA.M
 Title : VOC Analysis

Signal : TIC: VX033548.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	59	rBV	76021	98246	10.95%	1.485%
2	1.672	91	96	115	rVB	69221	99244	11.06%	1.501%
3	2.307	194	200	211	rVB	147935	231710	25.82%	3.503%
4	2.508	230	233	237	rBV2	947	1642	0.18%	0.025%
5	2.794	276	280	285	rVB3	1016	2022	0.23%	0.031%
6	3.099	327	330	334	rBV2	439	658	0.07%	0.010%
7	3.422	381	383	386	rBV	262	215	0.02%	0.003%
8	3.928	463	466	467	rBV2	299	330	0.04%	0.005%
9	4.056	485	487	489	rBV2	222	239	0.03%	0.004%
10	4.459	545	553	570	rBV	56423	163703	18.24%	2.475%
11	5.062	640	652	668	rBV	119699	367582	40.95%	5.558%
12	5.970	789	801	820	rBV2	304321	897539	100.00%	13.571%
13	6.281	849	852	853	rBV	206	183	0.02%	0.003%
14	6.300	853	855	857	rVV	182	170	0.02%	0.003%
15	6.318	857	858	861	rVB2	163	116	0.01%	0.002%
16	6.458	880	881	883	rBV	166	102	0.01%	0.002%
17	6.629	906	909	910	rBV2	122	117	0.01%	0.002%
18	6.690	918	919	921	rBV	124	103	0.01%	0.002%
19	6.763	921	931	946	rVV	233109	549837	61.26%	8.313%
20	6.964	962	964	965	rVB	245	120	0.01%	0.002%
21	7.025	970	974	976	rBV	184	276	0.03%	0.004%
22	7.123	984	990	995	rBV4	1954	4056	0.45%	0.061%
23	7.196	1000	1002	1003	rBV	115	77	0.01%	0.001%
24	7.312	1012	1021	1038	rVB	180386	393737	43.87%	5.953%
25	7.488	1043	1050	1055	rVB2	768	1397	0.16%	0.021%
26	7.525	1055	1056	1059	rBV	266	261	0.03%	0.004%
27	7.635	1073	1074	1075	rVB	226	83	0.01%	0.001%
28	7.653	1075	1077	1079	rBV2	163	179	0.02%	0.003%
29	7.738	1089	1091	1093	rBV2	194	156	0.02%	0.002%
30	7.763	1093	1095	1099	rVB2	185	221	0.02%	0.003%
31	7.885	1113	1115	1116	rBV	92	87	0.01%	0.001%
32	7.940	1118	1124	1130	rVV2	1515	3364	0.37%	0.051%
33	8.013	1134	1136	1137	rBV	176	129	0.01%	0.002%
34	8.141	1156	1157	1160	rBV2	93	116	0.01%	0.002%
35	8.263	1175	1177	1181	rBV2	226	287	0.03%	0.004%
36	8.324	1181	1187	1202	rVV	129606	209210	23.31%	3.163%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122222\
 Data File : VX033548.D
 Acq On : 22 Dec 2022 16:34
 Operator : JC/MD
 Sample : VX1222WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK604

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122222WMA.M
 Title : VOC Analysis

37	8.482	1209	1213	1214	rBV2	1040	1129	0.13%	0.017%
38	8.647	1234	1240	1252	rBV	485052	762308	84.93%	11.526%
39	8.866	1274	1276	1278	rVB	272	179	0.02%	0.003%
40	8.885	1278	1279	1281	rBV	113	109	0.01%	0.002%
41	8.952	1284	1290	1299	rBV	92319	133602	14.89%	2.020%
42	9.177	1326	1327	1328	rBV	177	88	0.01%	0.001%
43	9.275	1338	1343	1346	rBV3	835	858	0.10%	0.013%
44	9.384	1356	1361	1373	rBV	271155	375849	41.88%	5.683%
45	9.653	1404	1405	1406	rVB	180	66	0.01%	0.001%
46	9.860	1437	1439	1440	rBV	155	143	0.02%	0.002%
47	9.903	1445	1446	1448	rVB	144	95	0.01%	0.001%
48	10.055	1465	1471	1487	rBV	472431	622719	69.38%	9.415%
49	10.195	1492	1494	1499	rVV2	541	645	0.07%	0.010%
50	10.281	1503	1508	1509	rBV2	154	251	0.03%	0.004%
51	10.305	1509	1512	1516	rBV2	554	668	0.07%	0.010%
52	10.360	1518	1521	1523	rBV	152	176	0.02%	0.003%
53	10.604	1560	1561	1563	rBV	131	76	0.01%	0.001%
54	10.659	1565	1570	1575	rVV4	490	827	0.09%	0.013%
55	10.793	1591	1592	1595	rBV2	180	237	0.03%	0.004%
56	10.866	1602	1604	1605	rBV	121	82	0.01%	0.001%
57	11.049	1632	1634	1636	rVB2	131	85	0.01%	0.001%
58	11.085	1639	1640	1641	rVB	177	65	0.01%	0.001%
59	11.189	1652	1657	1664	rBV	317670	422248	47.05%	6.384%
60	11.274	1669	1671	1673	rVB	262	172	0.02%	0.003%
61	11.305	1674	1676	1677	rBV	143	85	0.01%	0.001%
62	11.378	1687	1688	1692	rBV2	130	159	0.02%	0.002%
63	11.415	1692	1694	1697	rVV2	180	205	0.02%	0.003%
64	11.451	1697	1700	1706	rVV	646	932	0.10%	0.014%
65	11.506	1708	1709	1713	rVB	195	113	0.01%	0.002%
66	11.537	1713	1714	1717	rBV2	156	133	0.01%	0.002%
67	11.683	1735	1738	1742	rVV2	2053	2547	0.28%	0.039%
68	11.719	1742	1744	1747	rVB	320	280	0.03%	0.004%
69	11.756	1747	1750	1753	rBV2	703	878	0.10%	0.013%
70	11.969	1782	1785	1788	rBV4	801	1078	0.12%	0.016%
71	12.024	1788	1794	1805	rVB	461634	590338	65.77%	8.926%
72	12.317	1837	1842	1854	rBV	498585	658232	73.34%	9.952%
73	12.463	1864	1866	1868	rBV	242	133	0.01%	0.002%
74	12.549	1878	1880	1885	rVV2	126	147	0.02%	0.002%
75	12.768	1914	1916	1918	rVB2	206	178	0.02%	0.003%
76	12.963	1946	1948	1949	rVB	171	97	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122222\
 Data File : VX033548.D
 Acq On : 22 Dec 2022 16:34
 Operator : JC/MD
 Sample : VX1222WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK604

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122222WMA.M
 Title : VOC Analysis

77	13.067	1963	1965	1966	rBV	149	92	0.01%	0.001%
78	13.085	1966	1968	1970	rVV2	176	158	0.02%	0.002%
79	13.116	1970	1973	1977	rVB3	857	1044	0.12%	0.016%
80	13.225	1990	1991	1992	rBV	200	129	0.01%	0.002%
81	13.311	2004	2005	2007	rBV	181	157	0.02%	0.002%
82	13.439	2025	2026	2029	rBV	237	176	0.02%	0.003%
83	13.554	2043	2045	2047	rBV	111	64	0.01%	0.001%
84	13.591	2047	2051	2054	rBV2	815	1059	0.12%	0.016%
85	13.658	2060	2062	2064	rBV2	112	79	0.01%	0.001%
86	13.683	2064	2066	2068	rVB2	123	80	0.01%	0.001%
87	13.780	2079	2082	2087	rVB	662	991	0.11%	0.015%
88	13.823	2087	2089	2091	rBV2	102	108	0.01%	0.002%
89	13.884	2098	2099	2100	rBV	183	75	0.01%	0.001%
90	13.963	2109	2112	2117	rBV2	898	1031	0.11%	0.016%
91	14.079	2129	2131	2132	rVB	180	117	0.01%	0.002%
92	14.298	2166	2167	2168	rVB	182	67	0.01%	0.001%
93	14.438	2183	2190	2193	rBV3	803	1215	0.14%	0.018%
94	14.481	2195	2197	2199	rVB	216	99	0.01%	0.001%
95	15.152	2304	2307	2309	rBV2	216	245	0.03%	0.004%
96	15.219	2316	2318	2320	rBV	272	205	0.02%	0.003%
97	15.725	2399	2401	2403	rBV	319	150	0.02%	0.002%
98	15.774	2405	2409	2411	rBV3	231	373	0.04%	0.006%
99	16.560	2536	2538	2539	rBV	270	161	0.02%	0.002%
100	16.773	2571	2573	2574	rBV	369	223	0.02%	0.003%




Sum of corrected areas: 6613824

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122222\
Data File : VX033548.D
Acq On : 22 Dec 2022 16:34
Operator : JC/MD
Sample : VX1222WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK604

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

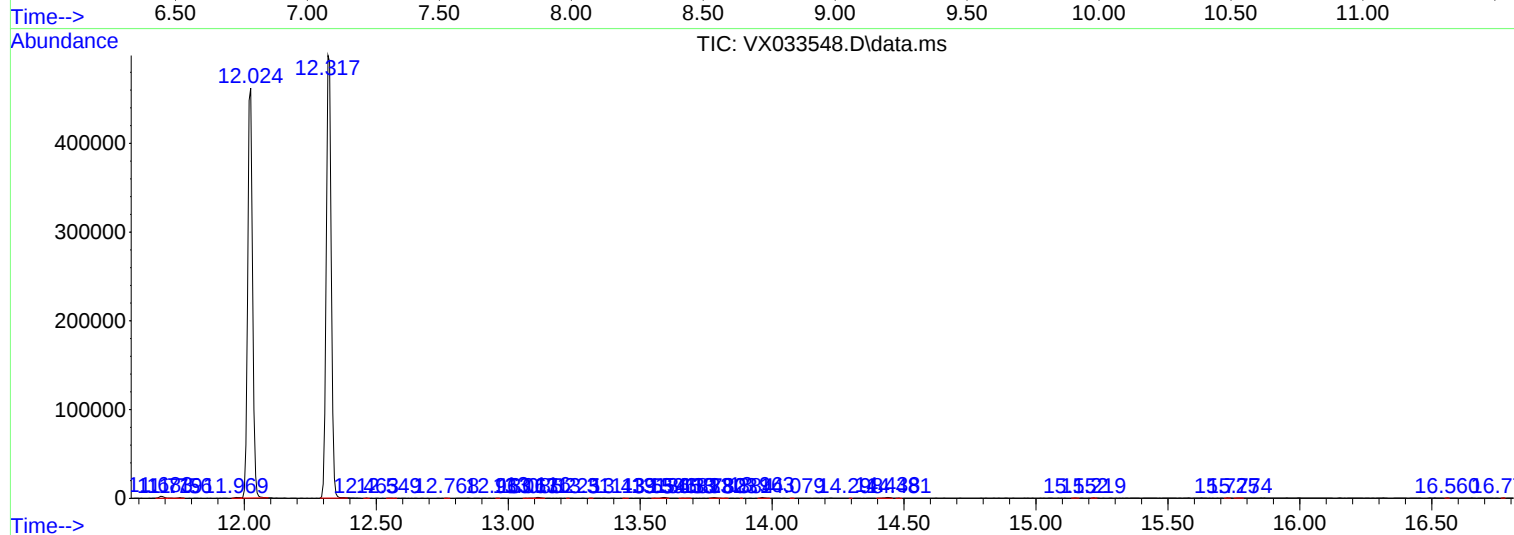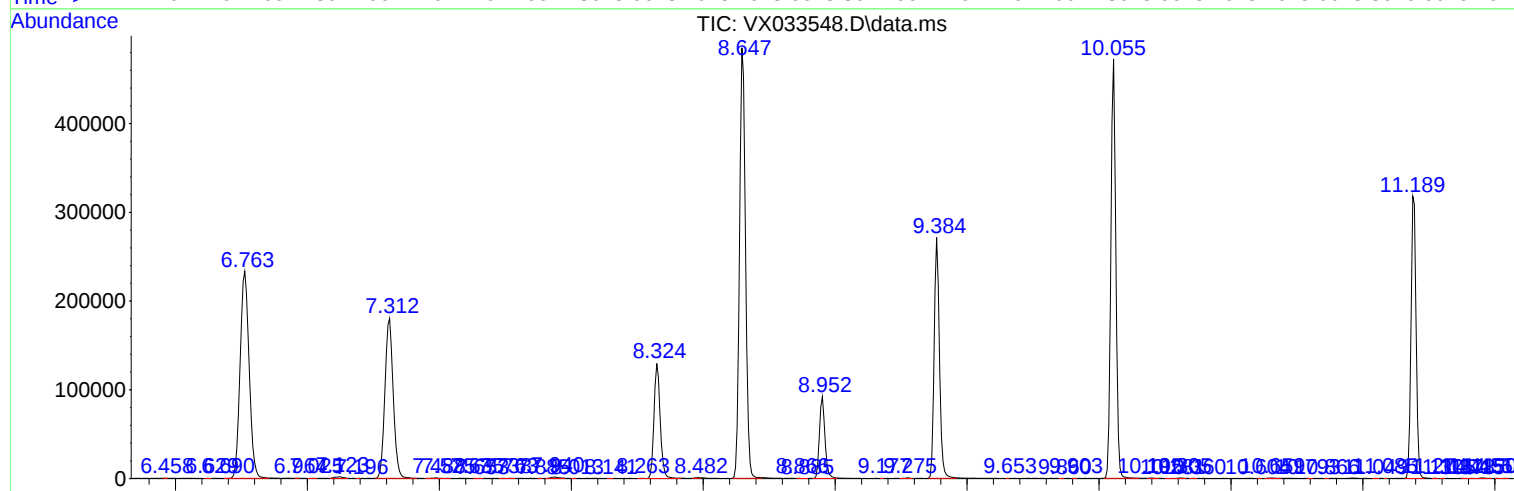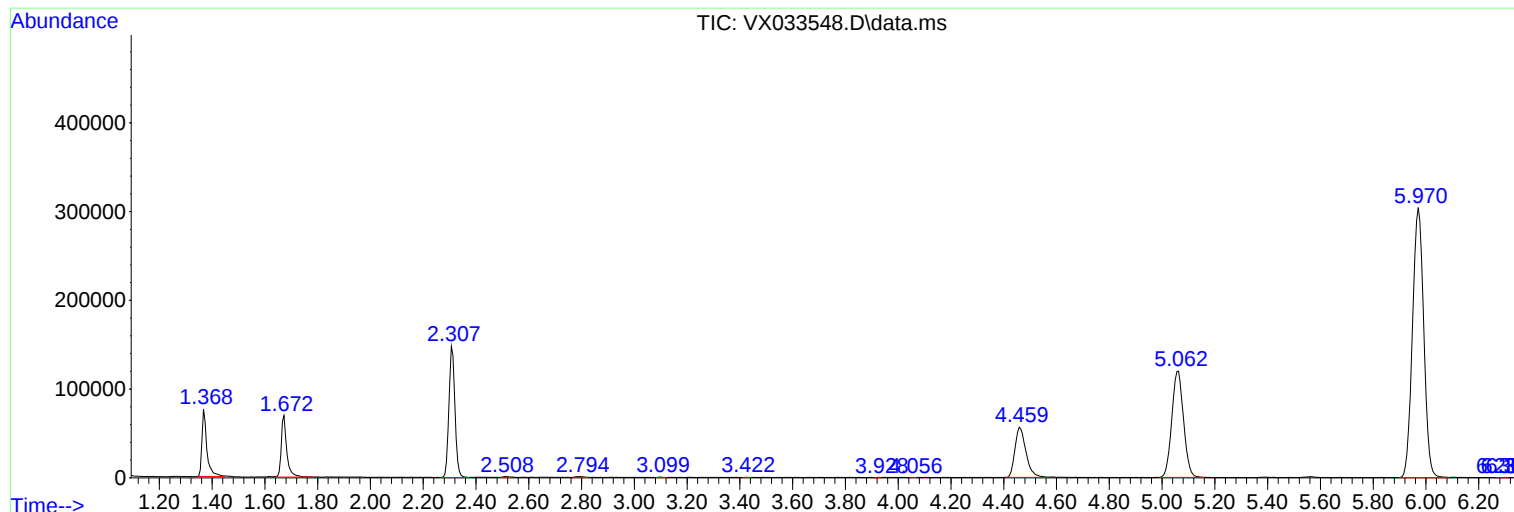

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122222\
Data File : VX033548.D
Acq On : 22 Dec 2022 16:34
Operator : JC/MD
Sample : VX1222WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK604

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122222\
Data File : VX033548.D
Acq On : 22 Dec 2022 16:34
Operator : JC/MD
Sample : VX1222WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK604

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
