


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122222\
 Data File : VX033537.D
 Acq On : 22 Dec 2022 10:00
 Operator : JC/MD
 Sample : BFB601
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB601

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122222WMA.M
 Title : VOC Analysis
 Last Update : Sat Dec 24 00:26:44 2022

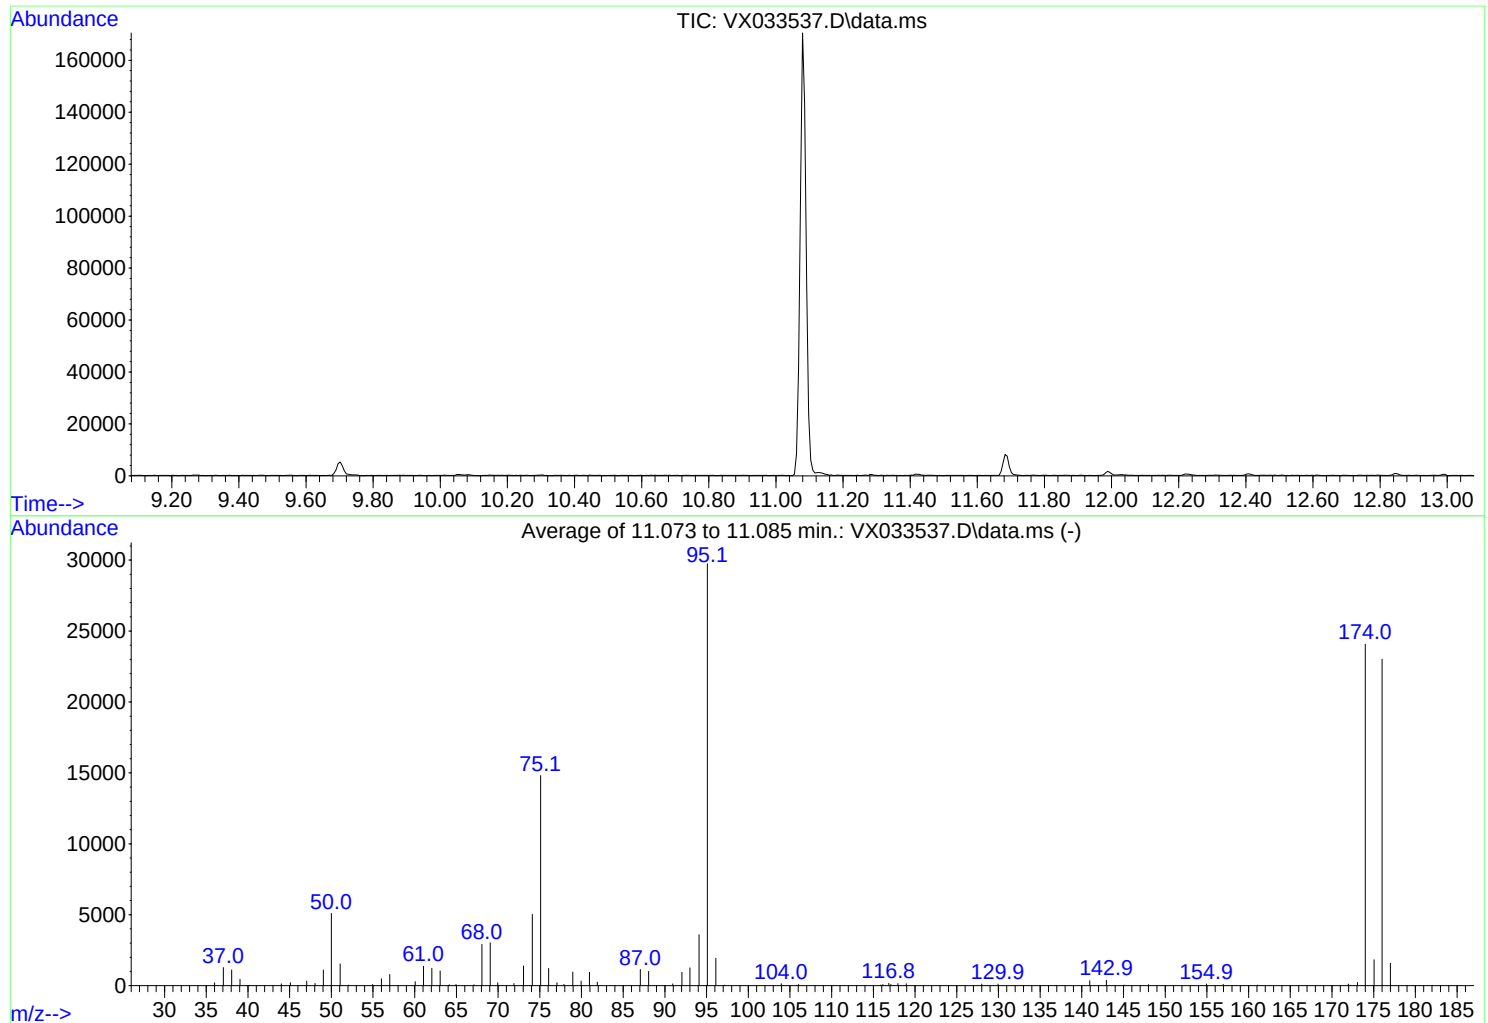

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	5082	PASS
75	95	30	80	49.8	14807	PASS
95	95	100	100	100.0	29736	PASS
96	95	5	9	6.5	1934	PASS
173	174	0.00	2	0.9	221	PASS
174	95	50	120	81.0	24075	PASS
175	174	5	9	7.6	1823	PASS
176	174	95	101	95.6	23017	PASS
177	176	5	9	6.9	1582	PASS

m/z	Abundance
39.90	75.0
43.90	76.0

Instrument :
MSVOA_X
ClientSampleId :
BFB601

m/z	Abundance
36.00	203.0
37.10	1059.0
38.10	1117.0
39.10	317.0
39.90	169.0
44.00	198.0
45.10	246.0
47.00	353.0
48.00	135.0
49.00	979.0
50.00	4320.0
51.00	1465.0
52.10	65.0
55.00	56.0
56.00	429.0
57.00	677.0
60.10	311.0
61.10	1070.0
62.00	990.0
63.00	883.0
64.20	54.0
64.90	116.0
67.10	75.0
68.00	2614.0
69.10	2723.0
69.90	173.0
71.90	125.0
73.00	1174.0
74.10	4411.0
75.10	12607.0
76.10	1037.0
77.00	200.0
77.80	105.0
78.90	816.0
79.90	327.0
80.90	766.0
81.90	225.0
87.00	993.0
88.10	862.0
91.00	108.0
92.00	732.0
93.00	1108.0
94.10	3003.0
95.10	24096.0
96.10	1600.0
97.20	56.0
104.00	103.0
105.80	94.0
116.20	102.0
116.80	187.0
117.10	166.0
117.90	111.0
118.90	104.0
127.90	72.0
130.00	67.0
136.90	63.0
141.00	259.0
143.00	331.0
155.00	79.0
156.90	78.0
172.20	98.0
173.10	228.0
174.00	16408.0
175.10	1291.0
176.00	15491.0
177.00	1138.0

Instrument :
MSVOA_X
ClientSampleId :
BFB601

m/z	Abundance
36.00	227.0
37.00	1585.0
38.10	1327.0
39.00	596.0
40.00	107.0
44.10	222.0
45.00	210.0
47.10	263.0
48.10	225.0
49.10	1358.0
50.00	6157.0
51.10	1925.0
52.10	59.0
55.00	77.0
56.00	645.0
57.00	1028.0
60.00	368.0
61.00	1635.0
62.10	1557.0
63.10	1296.0
64.10	81.0
64.90	74.0
67.10	61.0
68.10	3613.0
69.10	3530.0
70.00	258.0
71.90	176.0
73.00	1797.0
74.10	6007.0
75.10	17880.0
76.00	1482.0
77.10	166.0
77.90	81.0
78.90	1092.0
80.00	373.0
81.00	1092.0
81.90	337.0
87.00	1409.0
88.00	1251.0
90.90	136.0
92.10	1315.0
93.00	1485.0
94.10	4077.0
95.10	35888.0
96.10	2207.0
97.10	61.0
104.00	178.0
106.10	126.0
116.10	140.0
116.90	232.0
118.00	195.0
119.00	160.0
128.00	142.0
128.70	56.0
129.90	164.0
141.00	441.0
143.00	433.0
145.00	58.0
148.00	85.0
155.00	129.0
156.90	85.0
161.10	72.0
171.90	149.0
173.00	205.0
174.00	29264.0
175.10	2212.0
176.00	27216.0
177.00	1948.0

Instrument :
MSVOA_X
ClientSampleId :
BFB601

m/z	Abundance
36.00	189.0
37.10	1183.0
38.00	873.0
39.10	436.0
40.20	73.0
44.00	197.0
45.20	153.0
47.00	339.0
48.00	126.0
49.00	982.0
50.00	4768.0
51.10	1207.0
54.90	109.0
56.00	386.0
57.00	680.0
60.00	160.0
61.00	1400.0
62.10	1092.0
63.10	922.0
64.10	81.0
65.00	65.0
67.10	80.0
68.00	2514.0
69.00	2812.0
69.90	168.0
71.90	130.0
73.10	1187.0
74.10	4639.0
75.10	13933.0
76.10	1110.0
77.00	232.0
78.00	82.0
79.00	955.0
80.00	296.0
81.00	992.0
81.90	186.0
87.10	1024.0
88.00	905.0
91.00	141.0
92.00	776.0
93.00	1173.0
94.10	3694.0
95.10	29224.0
96.10	1996.0
103.80	134.0
106.00	95.0
115.90	142.0
116.80	96.0
117.10	96.0
117.90	128.0
118.90	158.0
128.10	111.0
130.00	109.0
140.90	334.0
142.90	392.0
145.10	80.0
148.00	104.0
154.90	140.0
157.00	97.0
161.10	65.0
172.00	201.0
173.00	231.0
174.00	26552.0
175.00	1967.0
176.00	26344.0
177.00	1661.0

Instrument :
MSVOA_X
ClientSampleId :
BFB601