

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122223\
 Data File : VX039433.D
 Acq On : 22 Dec 2023 12:35
 Operator : JC/MD
 Sample : VX1222WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX1222WBL01

Quant Time: Dec 23 06:22:19 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121323W.M
 Quant Title : SW846 8260
 QLast Update : Thu Dec 14 01:28:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	122653	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	261775	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	276869	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	136403	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	111321	49.544	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	99.080%
35) Dibromofluoromethane	5.385	113	86390	47.770	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	95.540%
50) Toluene-d8	8.647	98	336968	50.189	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	100.380%
62) 4-Bromofluorobenzene	11.079	95	150176	54.212	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	108.420%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122223\
Data File : VX039433.D
Acq On : 22 Dec 2023 12:35
Operator : JC/MD
Sample : VX1222WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1222WBL01

Quant Time: Dec 23 06:22:19 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121323W.M
Quant Title : SW846 8260
QLast Update : Thu Dec 14 01:28:15 2023
Response via : Initial Calibration




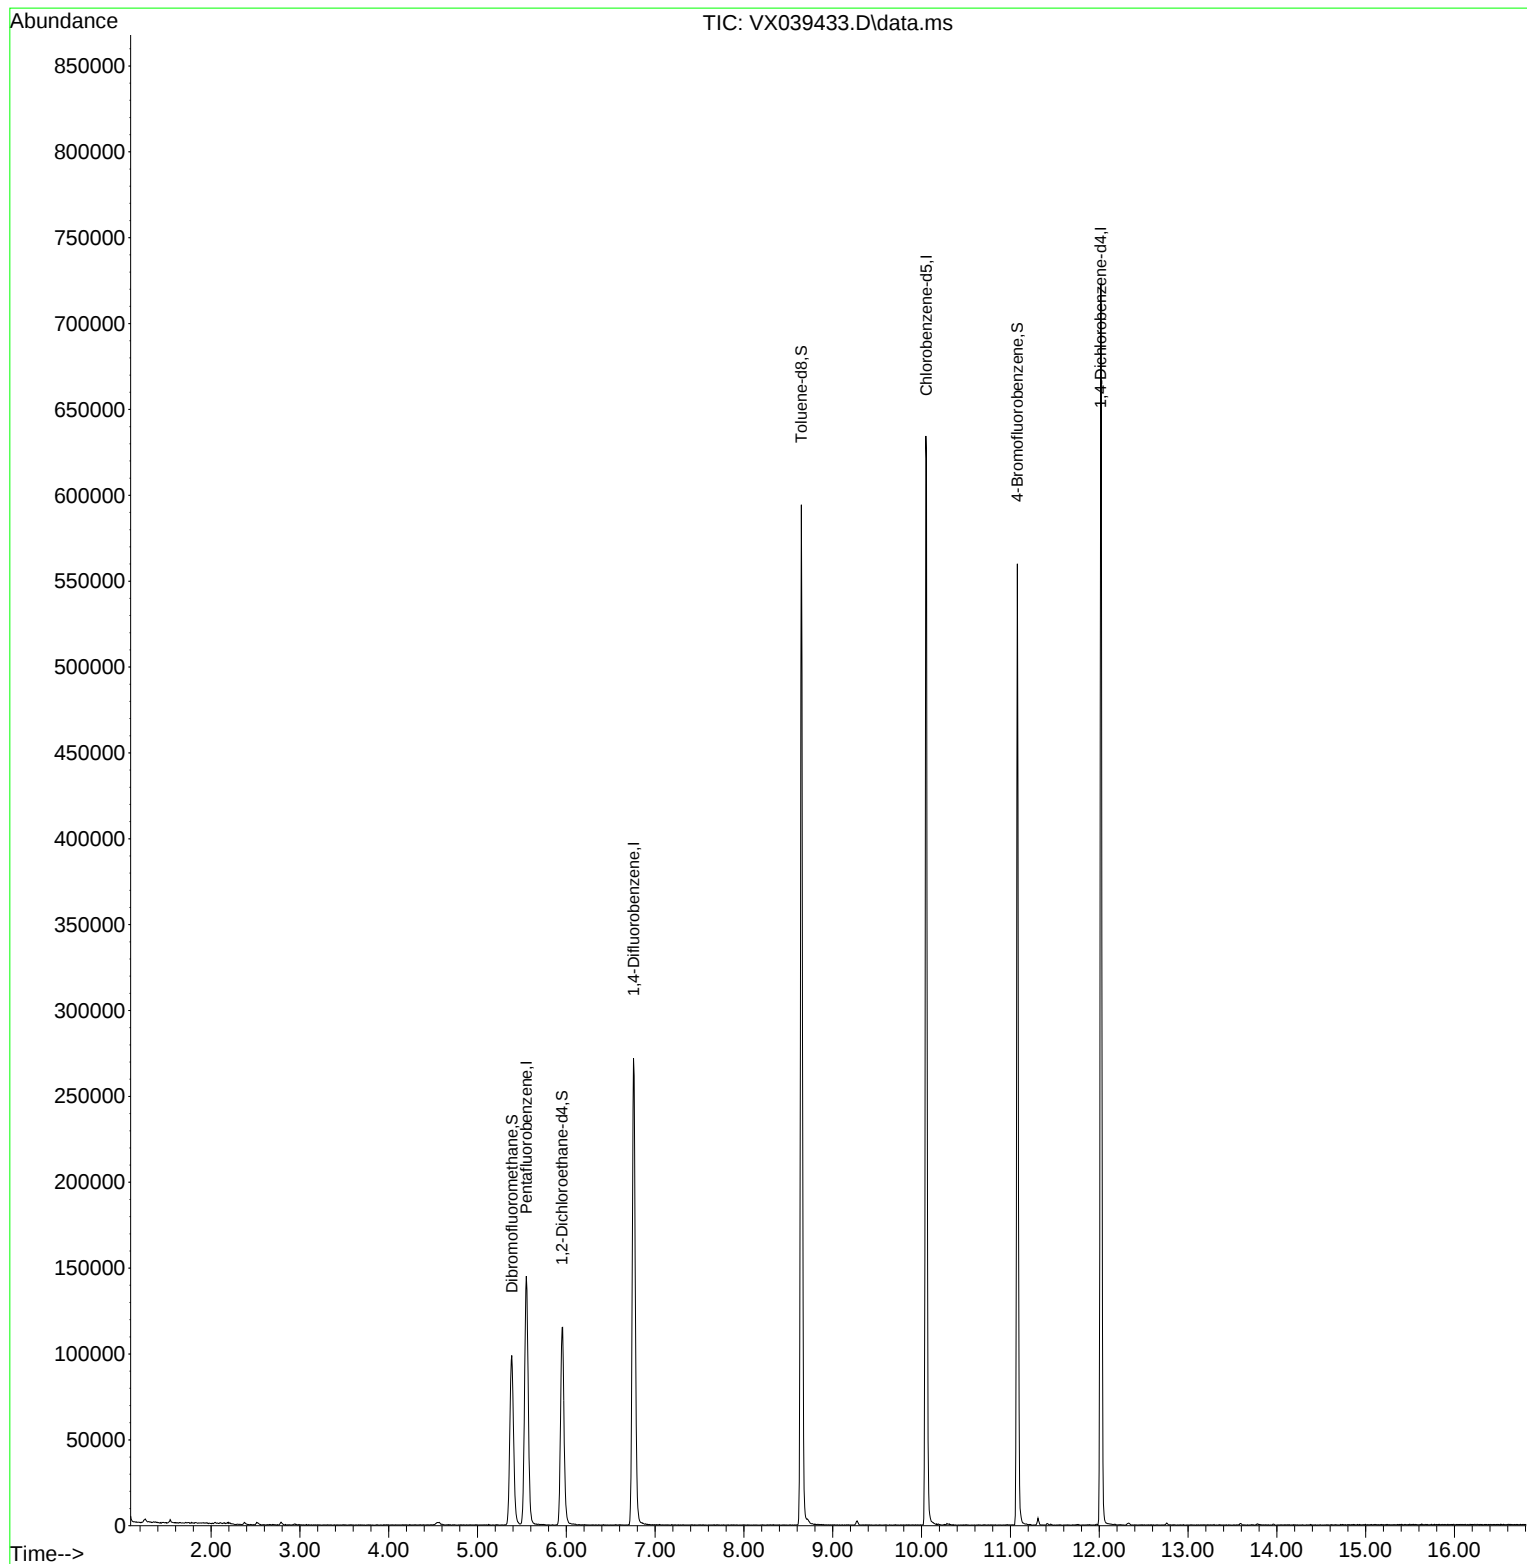


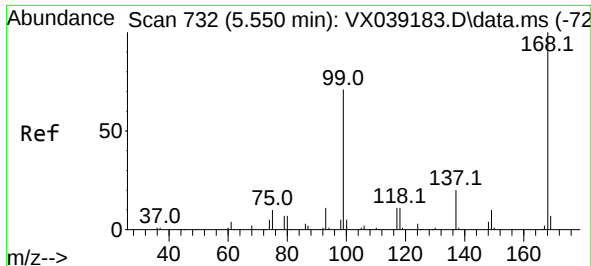

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 712
Delta R.T. -0.000 min
Lab File: VX039433.D
Acq: 22 Dec 2023 12:35




Instrument :
MSVOA_X
ClientSampleId :
VX1222WBL01


Tgt Ion:168 Resp: 122653
Ion Ratio Lower Upper
168 100
99 69.9 56.6 85.0

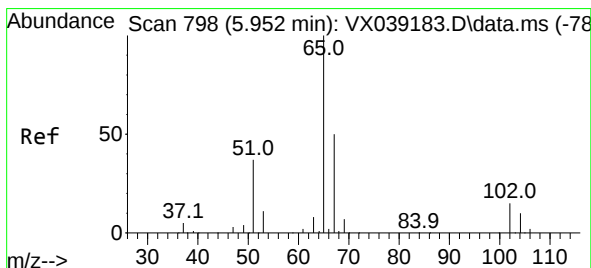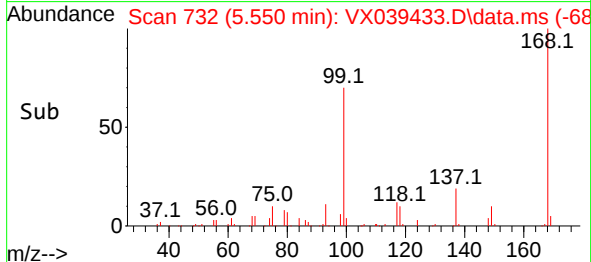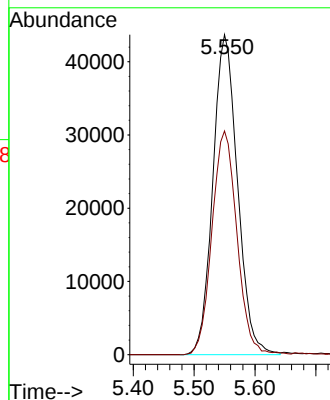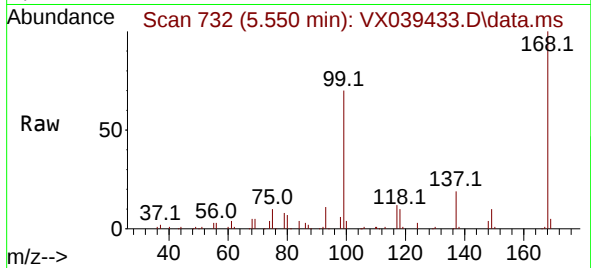

#33
1,2-Dichloroethane-d4
Concen: 49.544 ug/l
RT: 5.952 min Scan# 798
Delta R.T. 0.000 min
Lab File: VX039433.D
Acq: 22 Dec 2023 12:35

Tgt Ion: 65 Resp: 111321
Ion Ratio Lower Upper
65 100
67 52.0 0.0 100.2


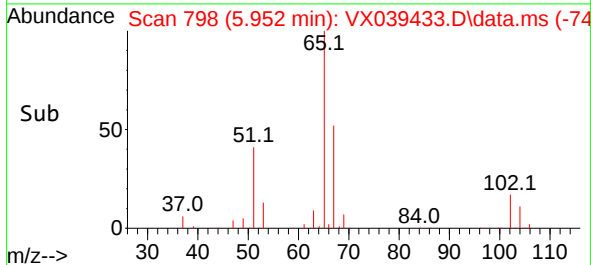
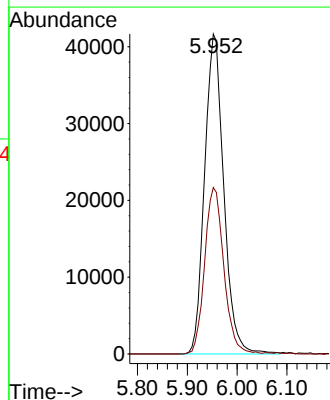
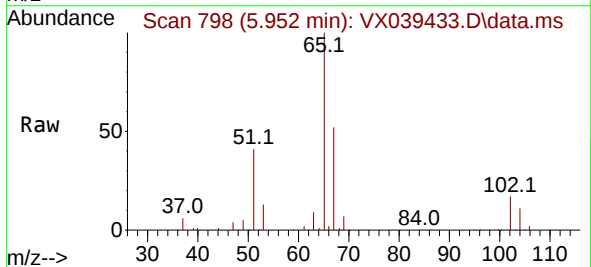


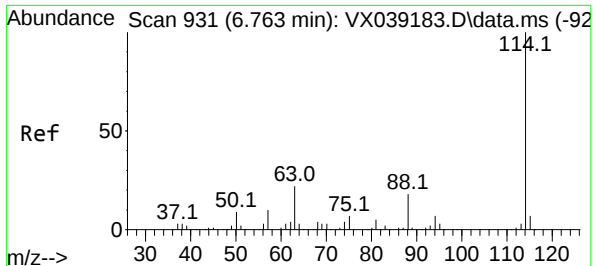

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. -0.006 min
Lab File: VX039433.D
Acq: 22 Dec 2023 12:35




Instrument :
MSVOA_X
ClientSampleId :
VX1222WBL01


Tgt Ion:114 Resp: 261775
Ion Ratio Lower Upper
114 100
63 24.2 0.0 45.0
88 17.5 0.0 36.6

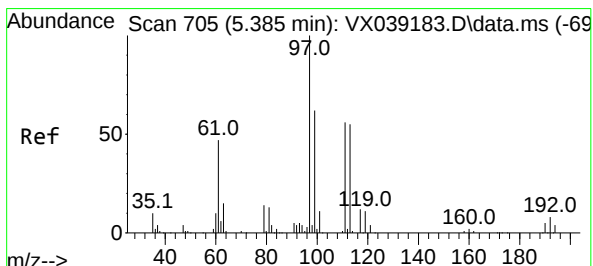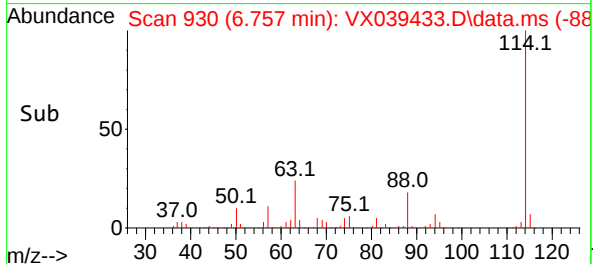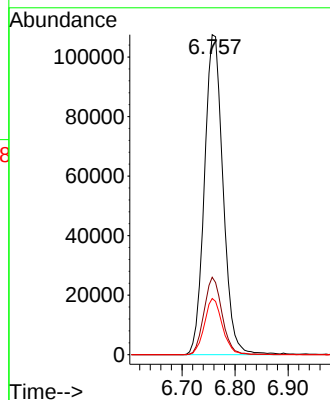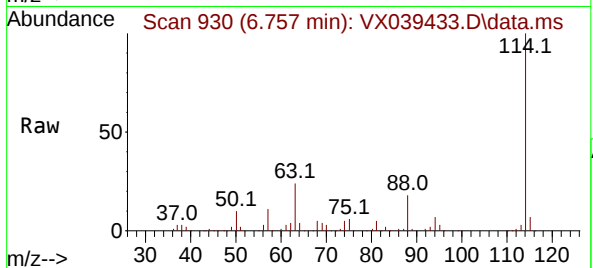

#35
Dibromofluoromethane
Concen: 47.770 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX039433.D
Acq: 22 Dec 2023 12:35

Tgt Ion:113 Resp: 86390
Ion Ratio Lower Upper
113 100
111 105.0 82.9 124.3
192 15.4 13.3 19.9

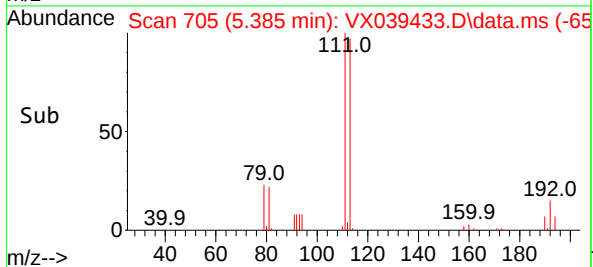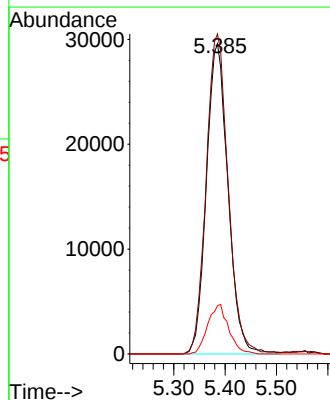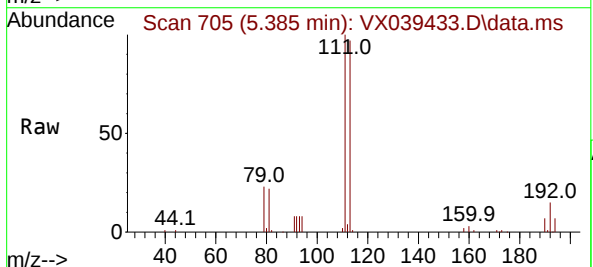

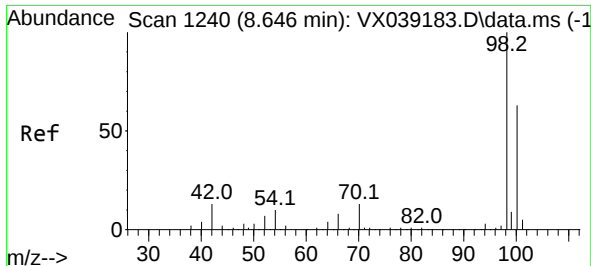

#50

Toluene-d8

Concen: 50.189 ug/l

RT: 8.647 min Scan# 11

Delta R.T. 0.000 min

Lab File: VX039433.D

Acq: 22 Dec 2023 12:35

Instrument :

MSVOA_X

ClientSampleId :





VX1222WBL01

Tgt Ion: 98 Resp: 336968

Ion Ratio Lower Upper

98 100

100 64.1 53.1 79.7

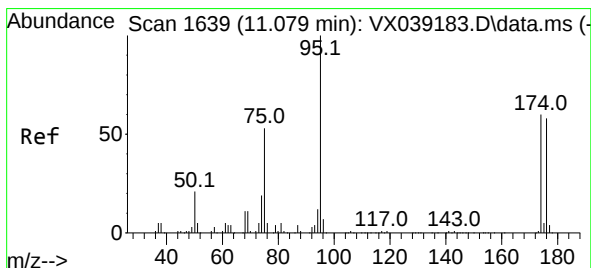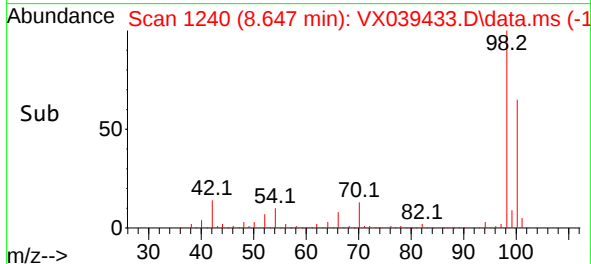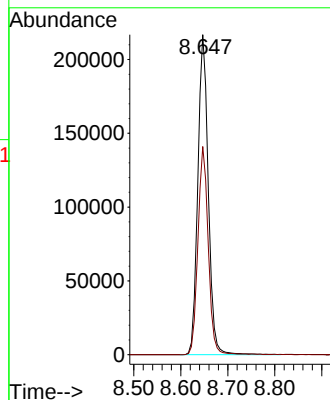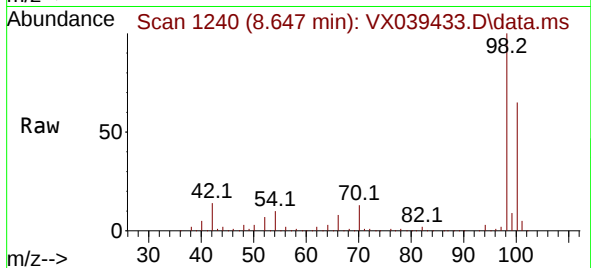

#62

4-Bromofluorobenzene

Concen: 54.212 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX039433.D

Acq: 22 Dec 2023 12:35




Tgt Ion: 95 Resp: 150176


Ion Ratio Lower Upper

95 100

174 63.8 0.0 135.6

176 61.1 0.0 131.0


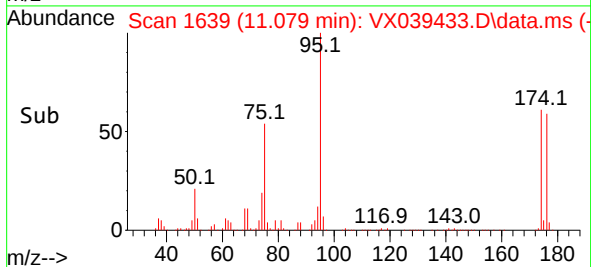
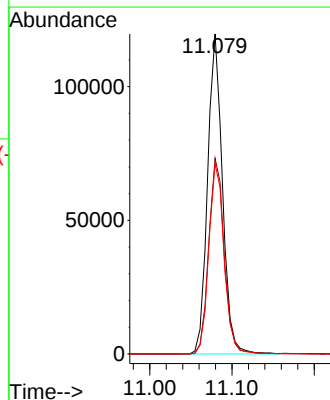
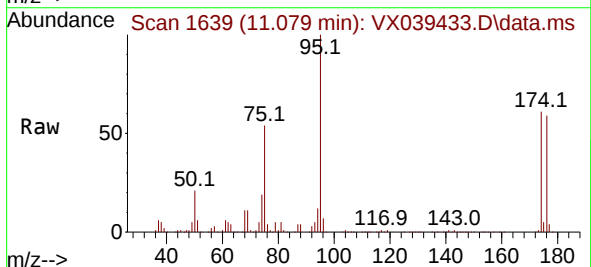


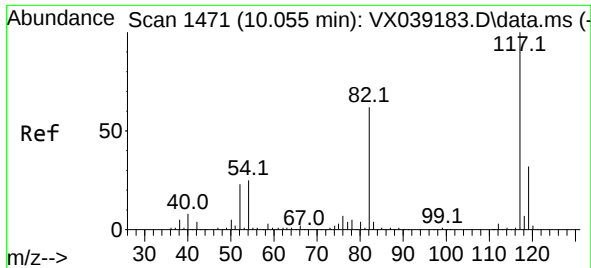

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX039433.D
Acq: 22 Dec 2023 12:35

Instrument :
MSVOA_X
ClientSampleId :
VX1222WBL01

Tgt Ion:117 Resp: 276869
Ion Ratio Lower Upper
117 100
82 59.5 46.2 69.4
119 32.5 25.5 38.3

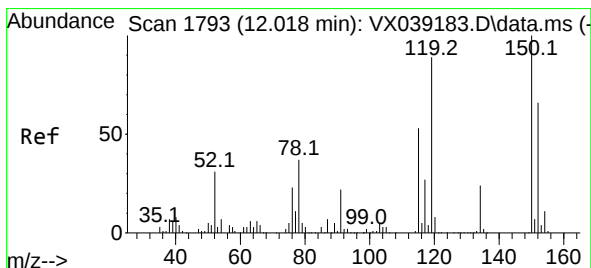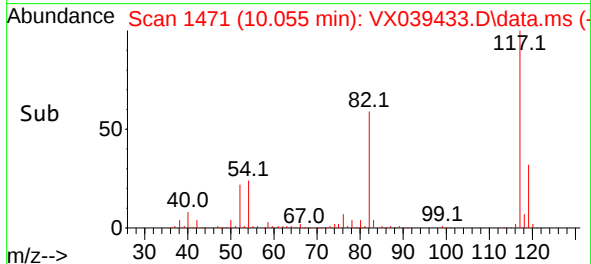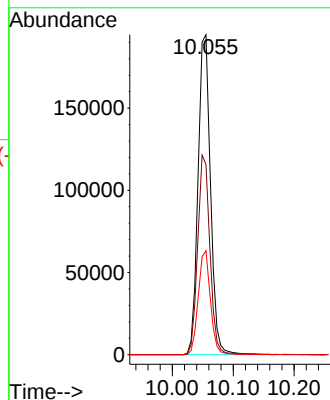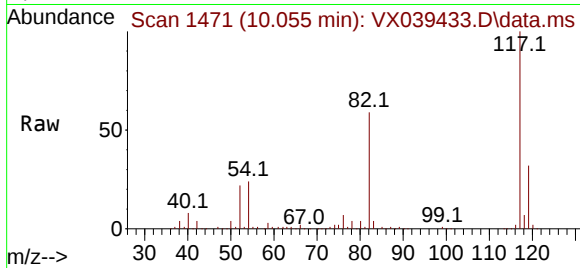

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. 0.000 min
Lab File: VX039433.D
Acq: 22 Dec 2023 12:35

Tgt Ion:152 Resp: 136403
Ion Ratio Lower Upper
152 100
115 66.2 43.3 129.9
150 155.8 0.0 345.0

