

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122223\
 Data File : VX039454.D
 Acq On : 22 Dec 2023 20:38
 Operator : JC/MD
 Sample : 05975-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RT-GWDUP01-122023

Quant Time: Dec 23 06:30:54 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121323W.M
 Quant Title : SW846 8260
 QLast Update : Thu Dec 14 01:28:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	98435	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	209731	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	220475	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	110925	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	91022	50.476	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	100.960%
35) Dibromofluoromethane	5.385	113	69260	47.801	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	95.600%
50) Toluene-d8	8.647	98	269165	50.038	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	100.080%
62) 4-Bromofluorobenzene	11.079	95	119448	53.819	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	107.640%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122223\
Data File : VX039454.D
Acq On : 22 Dec 2023 20:38
Operator : JC/MD
Sample : 05975-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RT-GWDUP01-122023

Quant Time: Dec 23 06:30:54 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121323W.M
Quant Title : SW846 8260
QLast Update : Thu Dec 14 01:28:15 2023
Response via : Initial Calibration




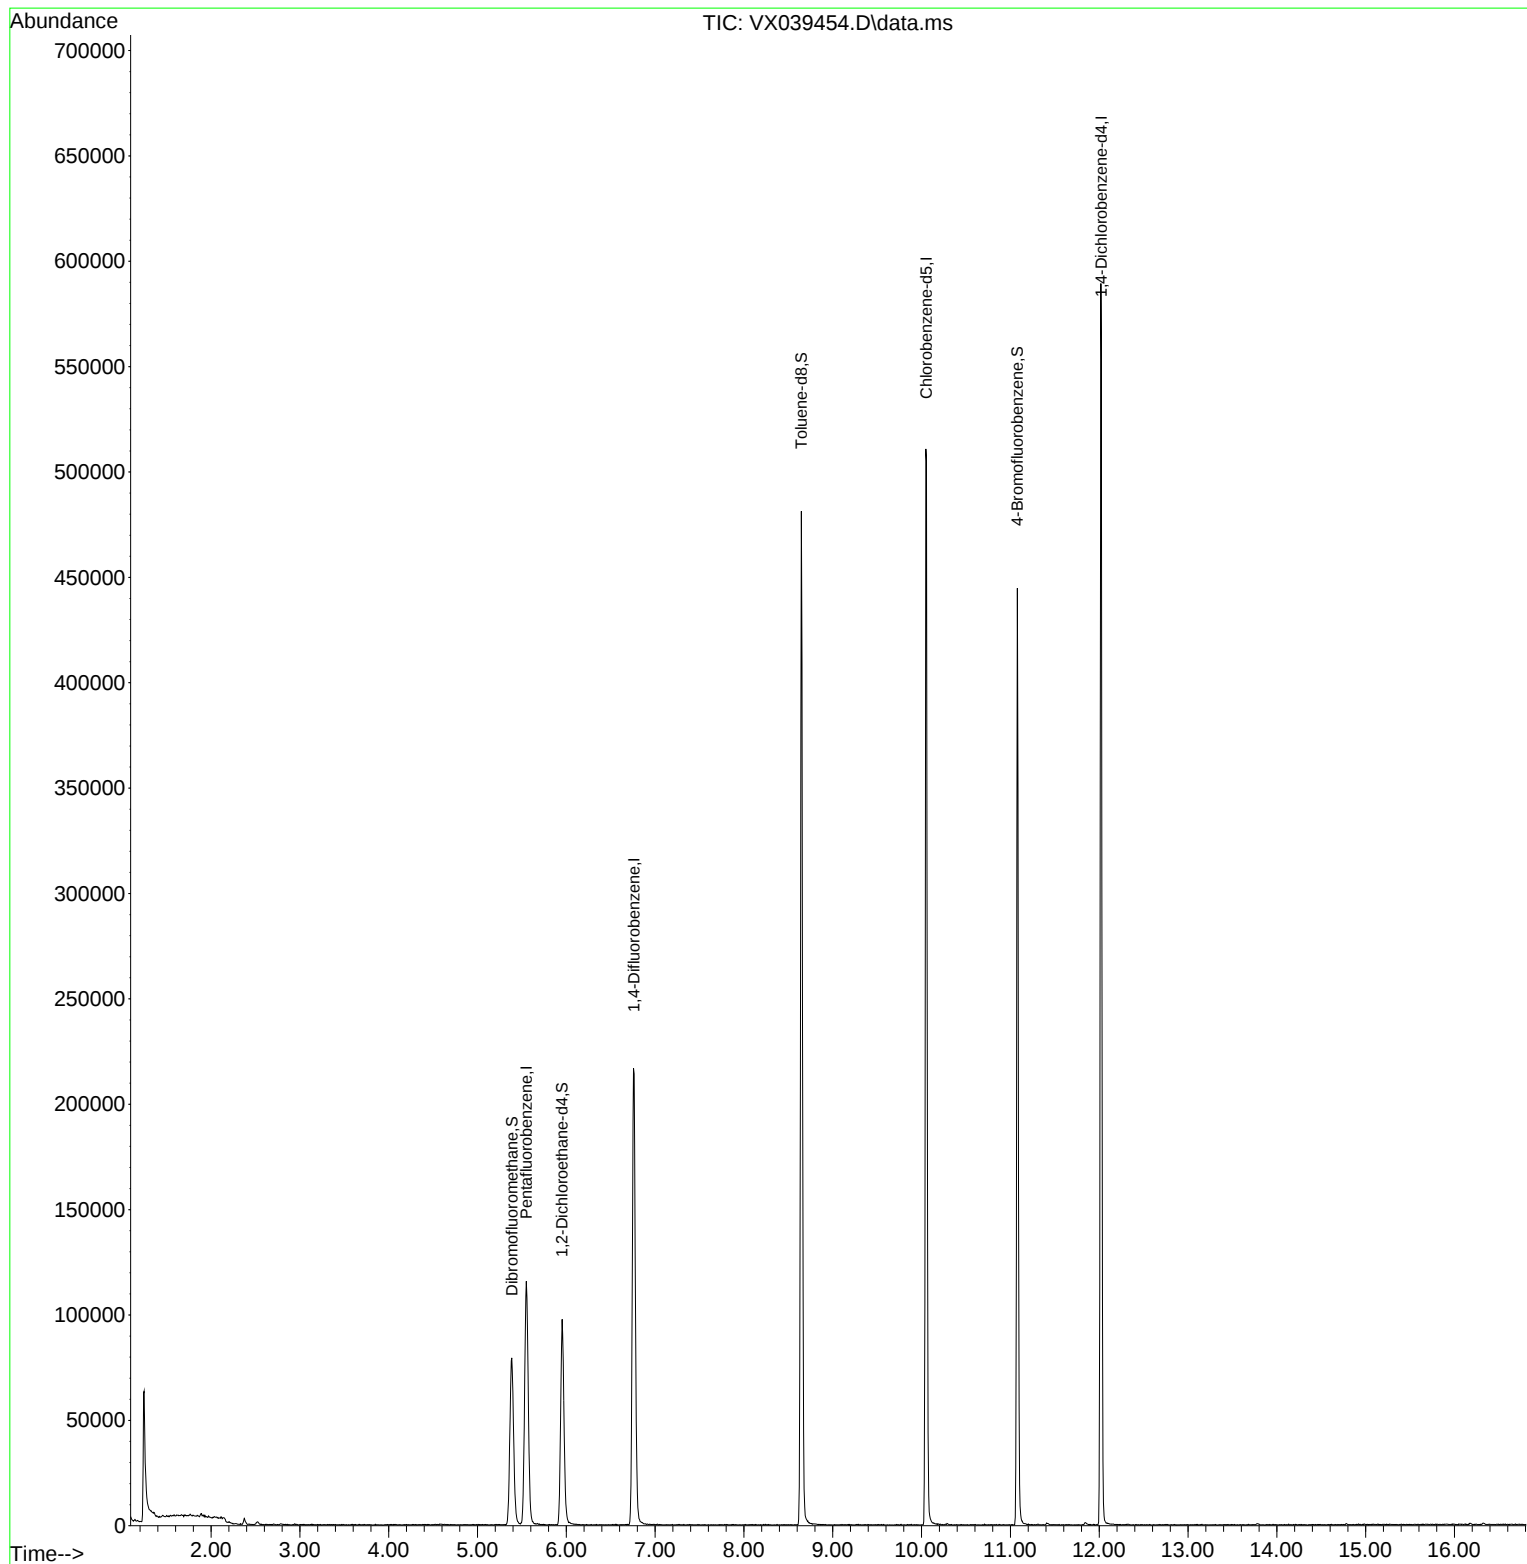


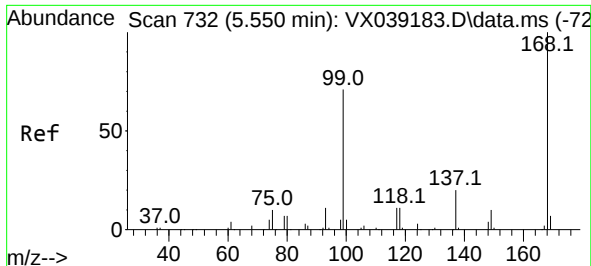

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 712
Delta R.T. -0.000 min
Lab File: VX039454.D
Acq: 22 Dec 2023 20:38




Instrument : MSVOA_X
ClientSampleId : RT-GWDUP01-122023

Tgt Ion:168 Resp: 98435
Ion Ratio Lower Upper
168 100
99 66.1 56.6 85.0

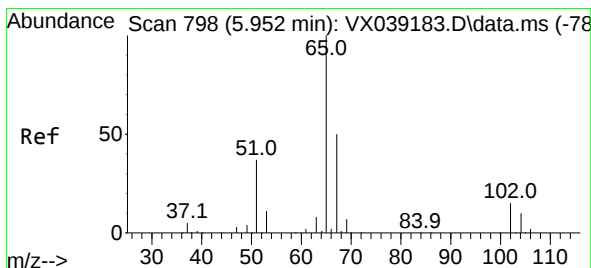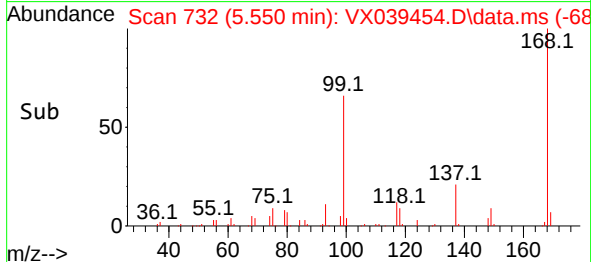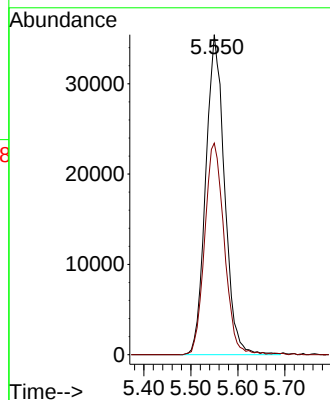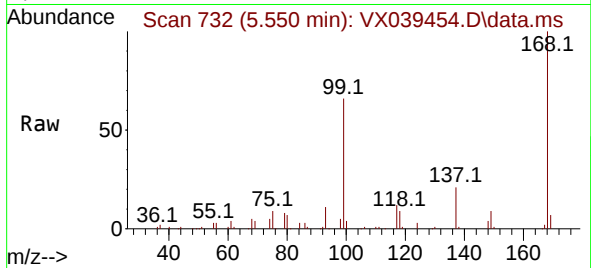

#33
1,2-Dichloroethane-d4
Concen: 50.476 ug/l
RT: 5.952 min Scan# 798
Delta R.T. 0.000 min
Lab File: VX039454.D
Acq: 22 Dec 2023 20:38

Tgt Ion: 65 Resp: 91022
Ion Ratio Lower Upper
65 100
67 51.7 0.0 100.2


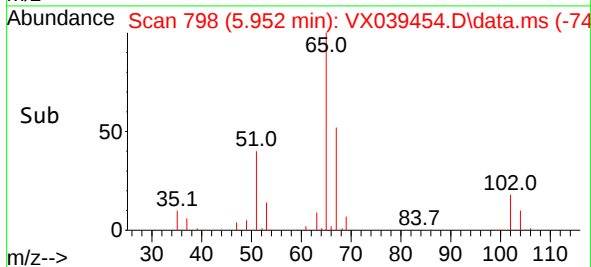
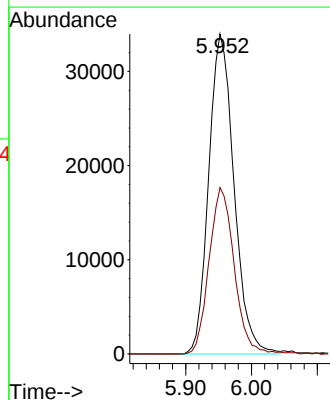
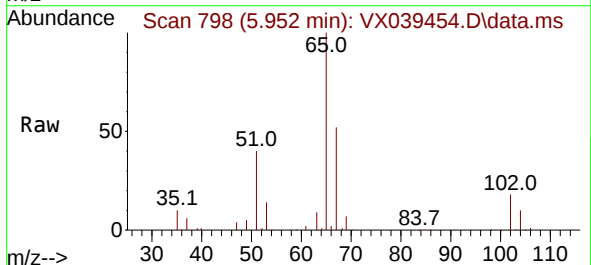




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 911
Delta R.T. 0.000 min
Lab File: VX039454.D
Acq: 22 Dec 2023 20:38




Instrument :
MSVOA_X
ClientSampleId :
RT-GWDUP01-122023

Tgt Ion:114 Resp: 209731
Ion Ratio Lower Upper
114 100
63 24.0 0.0 45.0
88 18.2 0.0 36.6

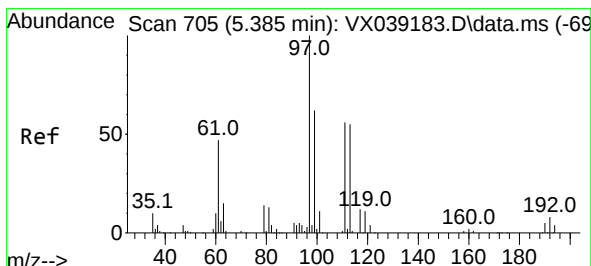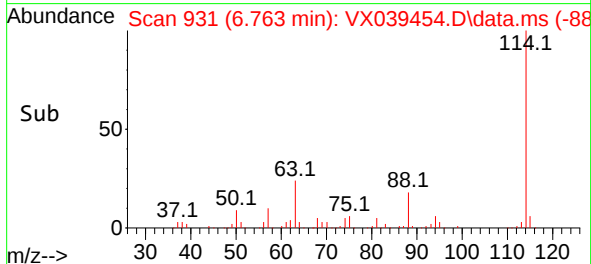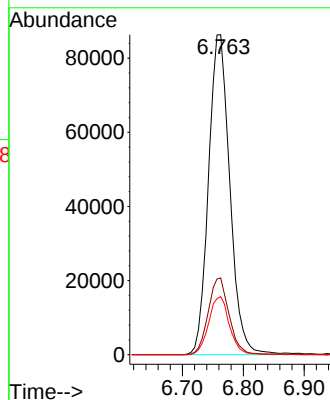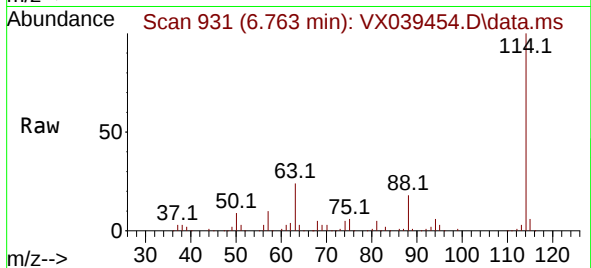

#35
Dibromofluoromethane
Concen: 47.801 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX039454.D
Acq: 22 Dec 2023 20:38

Tgt Ion:113 Resp: 69260
Ion Ratio Lower Upper
113 100
111 104.5 82.9 124.3
192 15.5 13.3 19.9

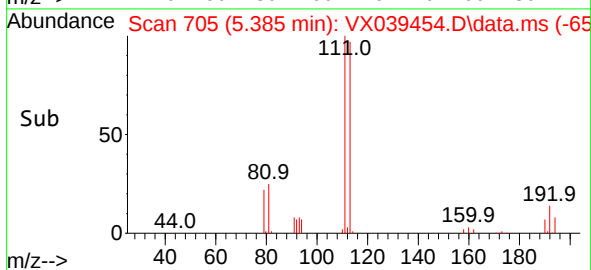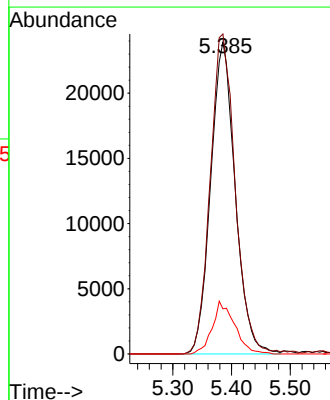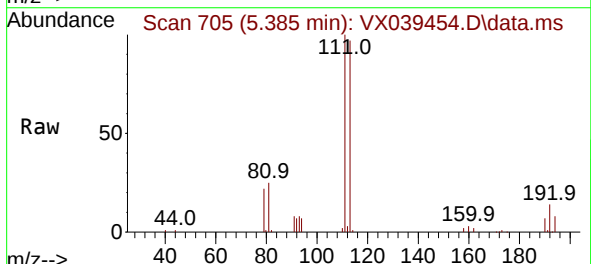



#50

Toluene-d8

Concen: 50.038 ug/l

RT: 8.647 min Scan# 11

Delta R.T. 0.000 min

Lab File: VX039454.D

Acq: 22 Dec 2023 20:38

Instrument :

MSVOA_X

ClientSampleId :





RT-GWDUP01-122023

Tgt Ion: 98 Resp: 269165

Ion Ratio Lower Upper

98 100

100 63.8 53.1 79.7

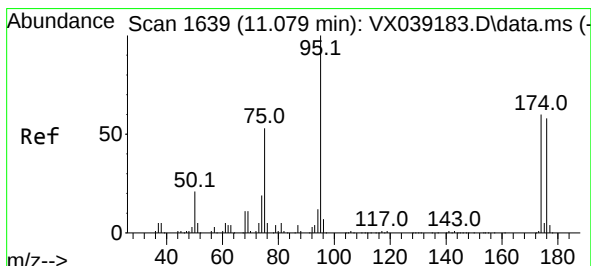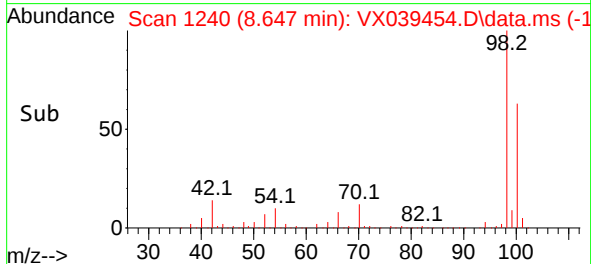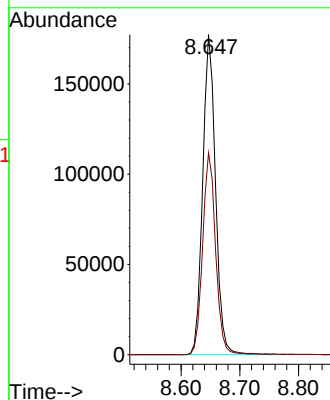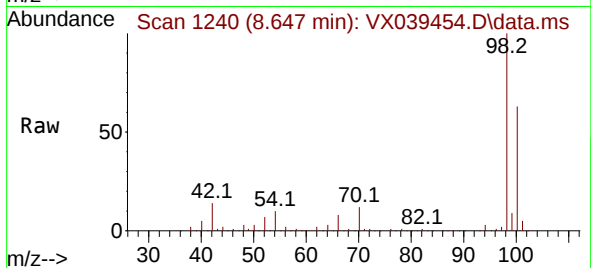

#62

4-Bromofluorobenzene

Concen: 53.819 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX039454.D

Acq: 22 Dec 2023 20:38




Tgt Ion: 95 Resp: 119448


Ion Ratio Lower Upper

95 100

174 63.6 0.0 135.6

176 60.6 0.0 131.0

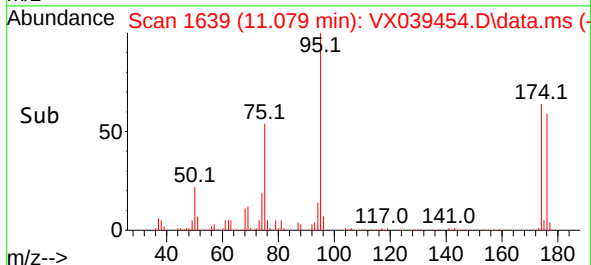
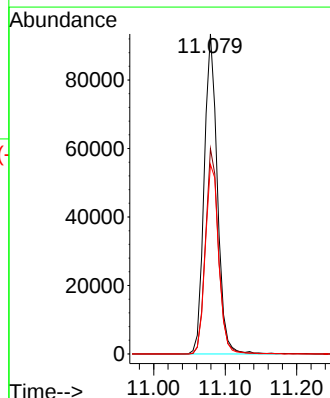
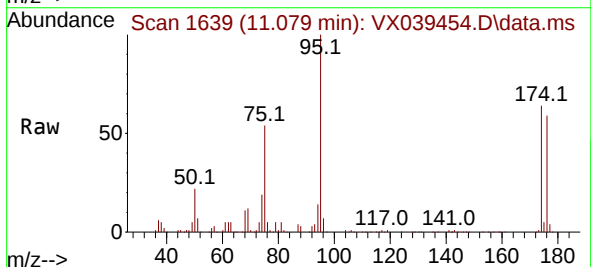


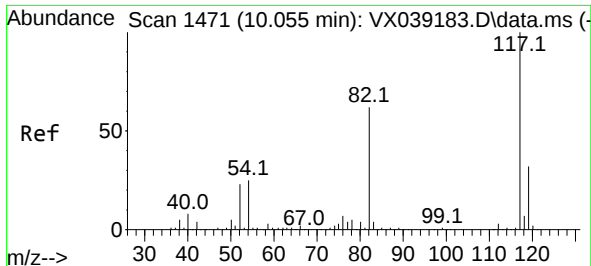

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX039454.D
Acq: 22 Dec 2023 20:38

Instrument :
MSVOA_X
ClientSampleId :
RT-GWDUP01-122023

Tgt Ion:117 Resp: 220475
Ion Ratio Lower Upper
117 100
82 60.0 46.2 69.4
119 31.4 25.5 38.3

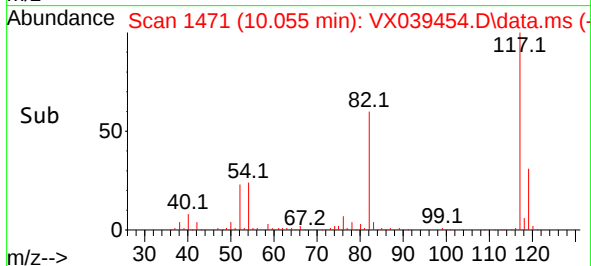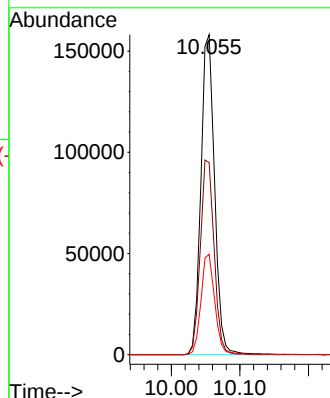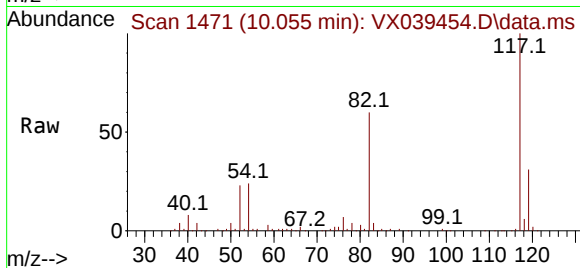

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.006 min
Lab File: VX039454.D
Acq: 22 Dec 2023 20:38

Tgt Ion:152 Resp: 110925
Ion Ratio Lower Upper
152 100
115 67.9 43.3 129.9
150 159.1 0.0 345.0

