

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX122319\
 Data File : VX014203.D
 Acq On : 23 Dec 2019 15:36
 Operator : JC/SP
 Sample : K6393-02
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MH-F

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X121319W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.070	26	30	43	rBV	1380631	1649149	61.49%	10.174%
2	1.265	59	62	70	rBV	282328	335902	12.52%	2.072%
3	1.601	111	117	119	rVB6	32778	60056	2.24%	0.370%
4	2.588	275	279	285	rVB	22266	37263	1.39%	0.230%
5	5.490	745	755	769	rBV	305099	868900	32.40%	5.360%
6	5.655	771	782	798	rVB	555258	1538817	57.37%	9.493%
7	6.057	839	848	859	rBV	331095	877270	32.71%	5.412%
8	6.850	967	978	991	rBV	840799	1967627	73.36%	12.138%
9	8.709	1275	1283	1291	rBV	1757440	2682037	100.00%	16.546%
10	10.105	1506	1512	1525	rBV	1693326	2326150	86.73%	14.350%
11	11.135	1675	1681	1688	rBV	1336810	1750146	65.25%	10.797%
12	12.074	1829	1835	1844	rBV	1746249	2116521	78.91%	13.057%


Sum of corrected areas: 16209838

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX122319\
Data File : VX014203.D
Acq On : 23 Dec 2019 15:36
Operator : JC/SP
Sample : K6393-02
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MH-F

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X121319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

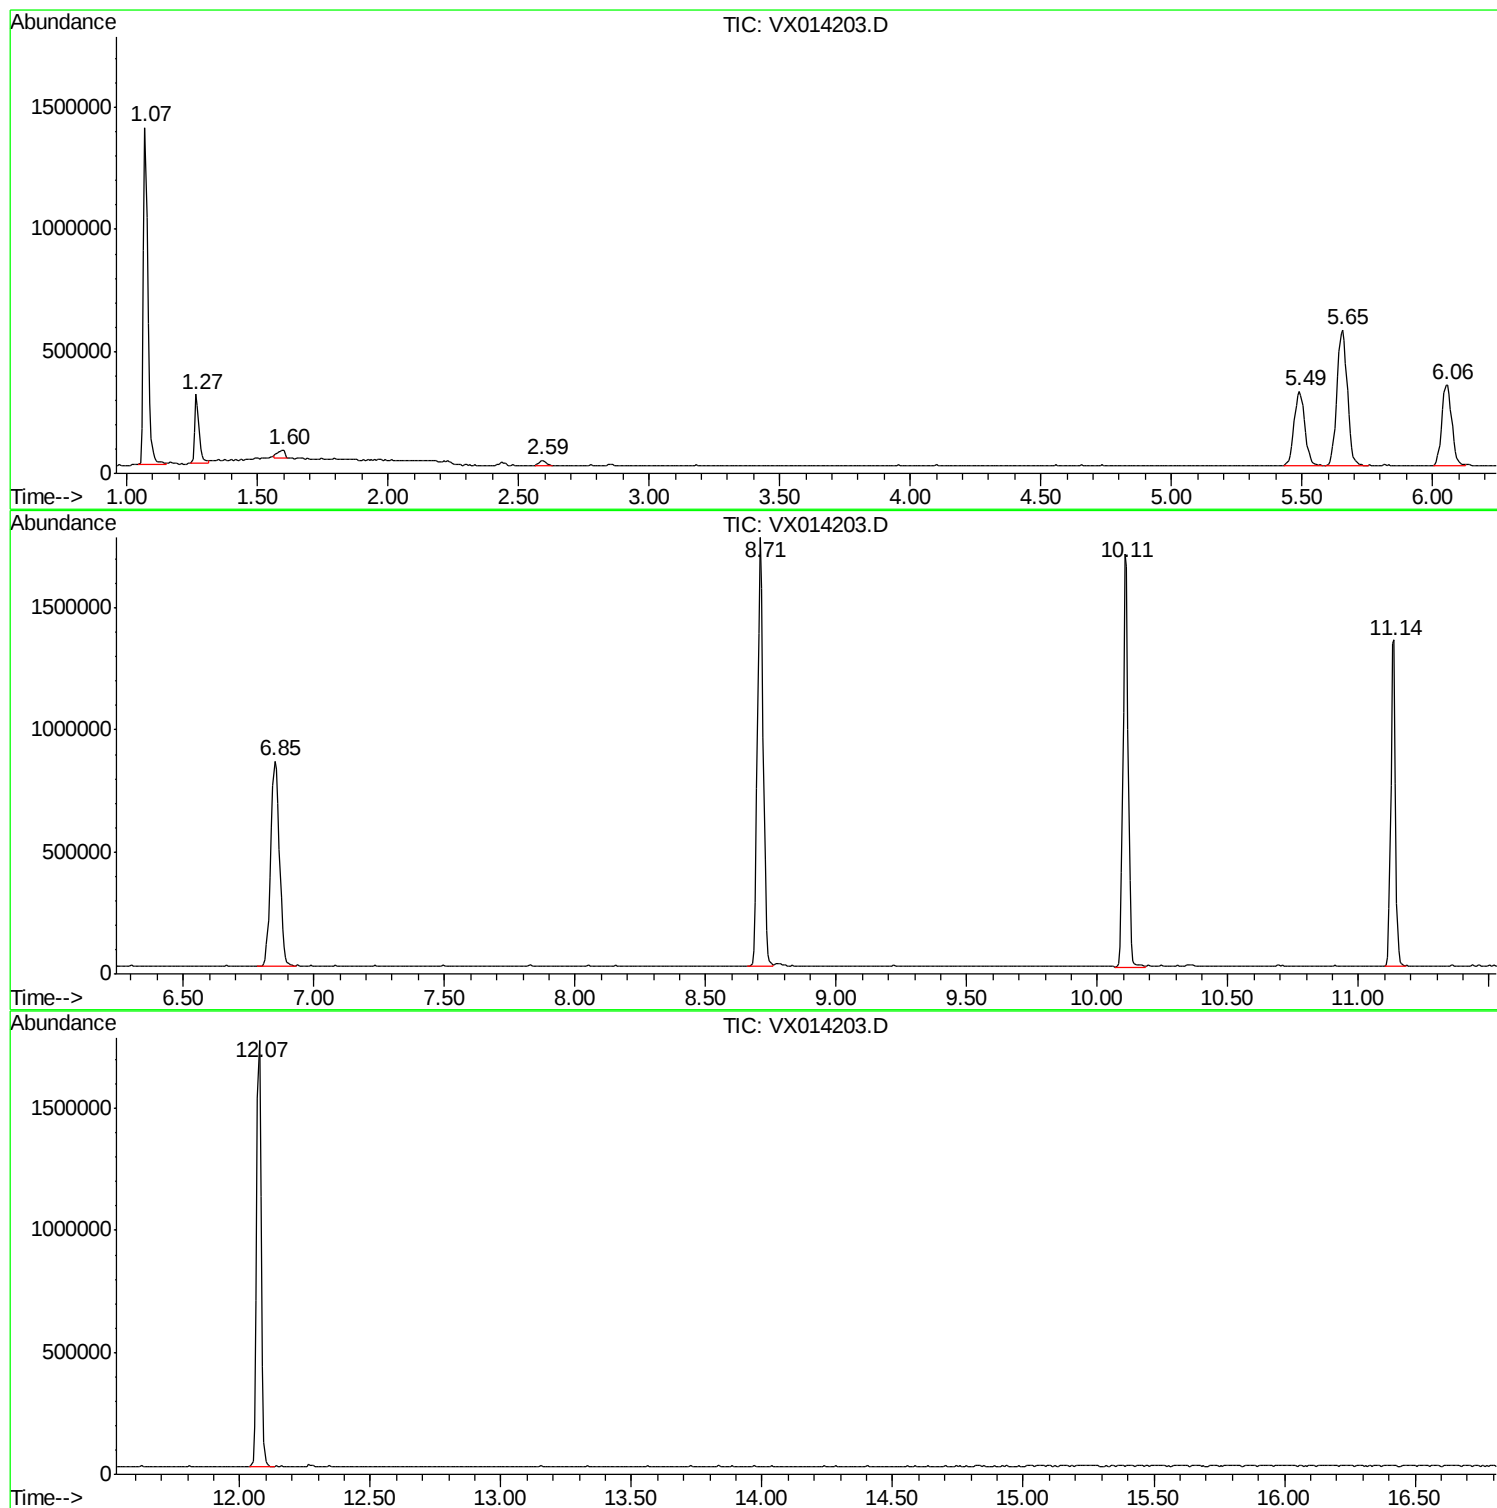

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX122319\
Data File : VX014203.D
Acq On : 23 Dec 2019 15:36
Operator : JC/SP
Sample : K6393-02
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MH-F










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X121319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Sulfur dioxide Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.27	10.91 ug/l	335902	Pentafluorobenzene	5.65

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1		Sulfur dioxide	64	O2S	007446-09-5	83
2		Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	74
3		L-Alanine, 3-sulfo-	169	C3H7NO5S	000498-40-8	9
4		Ethene, 1,1-difluoro-	64	C2H2F2	000075-38-7	4
5		Ethyl Chloride	64	C2H5Cl	000075-00-3	3

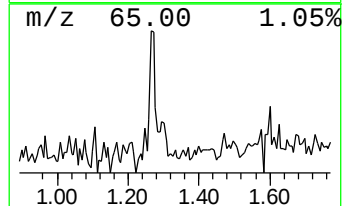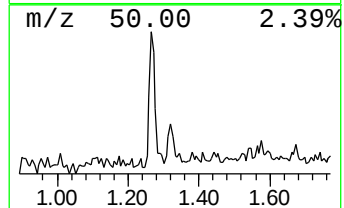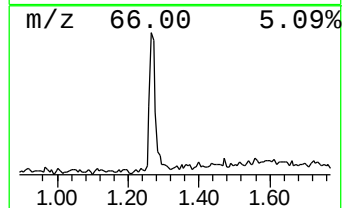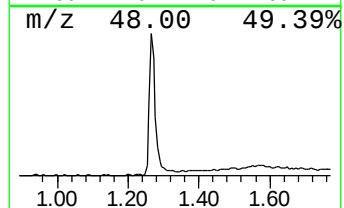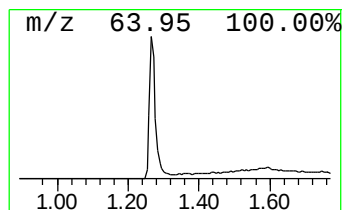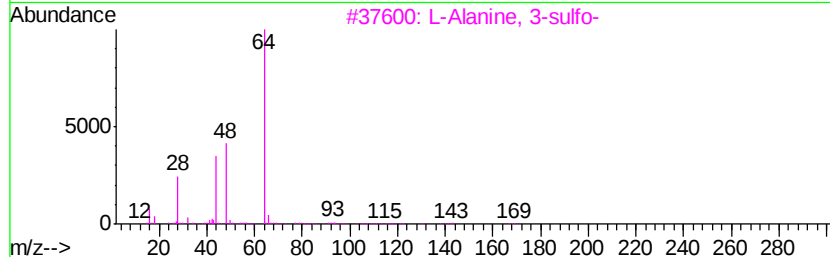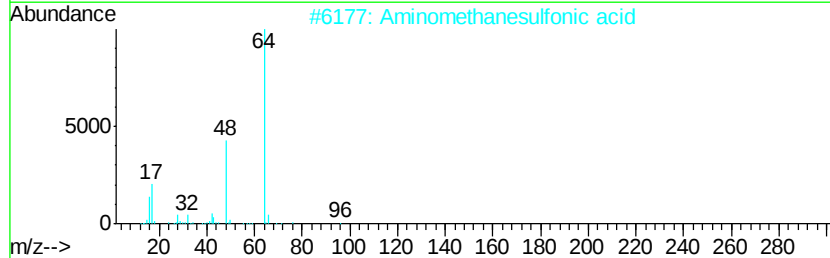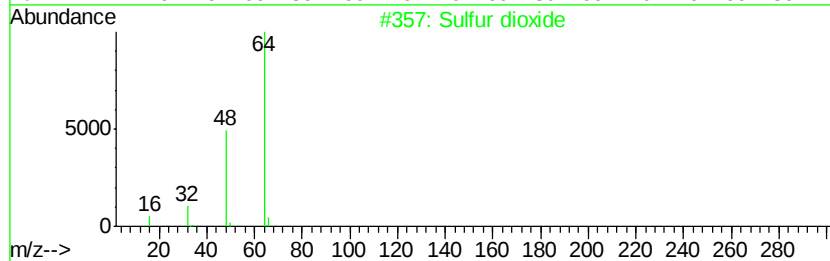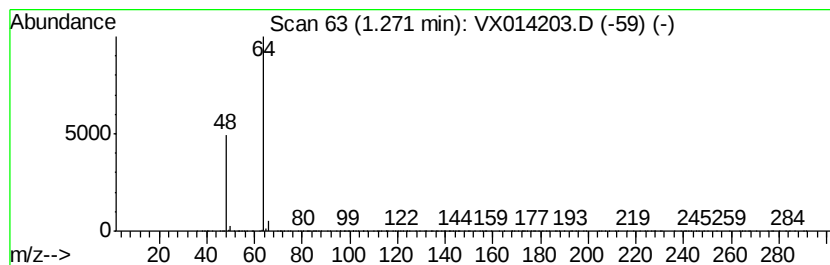

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX122319\
Data File : VX014203.D
Acq On : 23 Dec 2019 15:36
Operator : JC/SP
Sample : K6393-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MH-F

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X121319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.27	10.9	ug/l	335902	1	5.65	1538820	50.0