

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX122319\
Data File : VX014204.D
Acq On : 23 Dec 2019 15:59
Operator : JC/SP
Sample : K6393-03
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MH-20A

Integration Parameters: RTEINT.P

Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X121319W.M
Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.070	26	30	43	rBV	1673287	1993386	75.73%	12.366%
2	1.265	58	62	69	rBV	200165	243443	9.25%	1.510%
3	1.594	109	116	119	rVB7	27991	58891	2.24%	0.365%
4	2.436	249	254	260	rVB	33865	52810	2.01%	0.328%
5	2.588	275	279	285	rBV	18810	31473	1.20%	0.195%
6	5.490	743	755	766	rBV	296618	847087	32.18%	5.255%
7	5.655	771	782	796	rVV	541429	1507784	57.28%	9.353%
8	6.051	837	847	858	rBV	333685	874603	33.23%	5.426%
9	6.850	965	978	991	rBV	819369	1930132	73.33%	11.973%
10	8.709	1275	1283	1291	rBV	1696915	2632283	100.00%	16.329%
11	10.105	1507	1512	1522	rVB	1596263	2224024	84.49%	13.796%
12	11.135	1675	1681	1691	rVB	1287435	1689433	64.18%	10.480%
13	12.074	1829	1835	1842	rBV	1662562	2034858	77.30%	12.623%


Sum of corrected areas: 16120207

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX122319\
Data File : VX014204.D
Acq On : 23 Dec 2019 15:59
Operator : JC/SP
Sample : K6393-03
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MH-20A

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X121319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

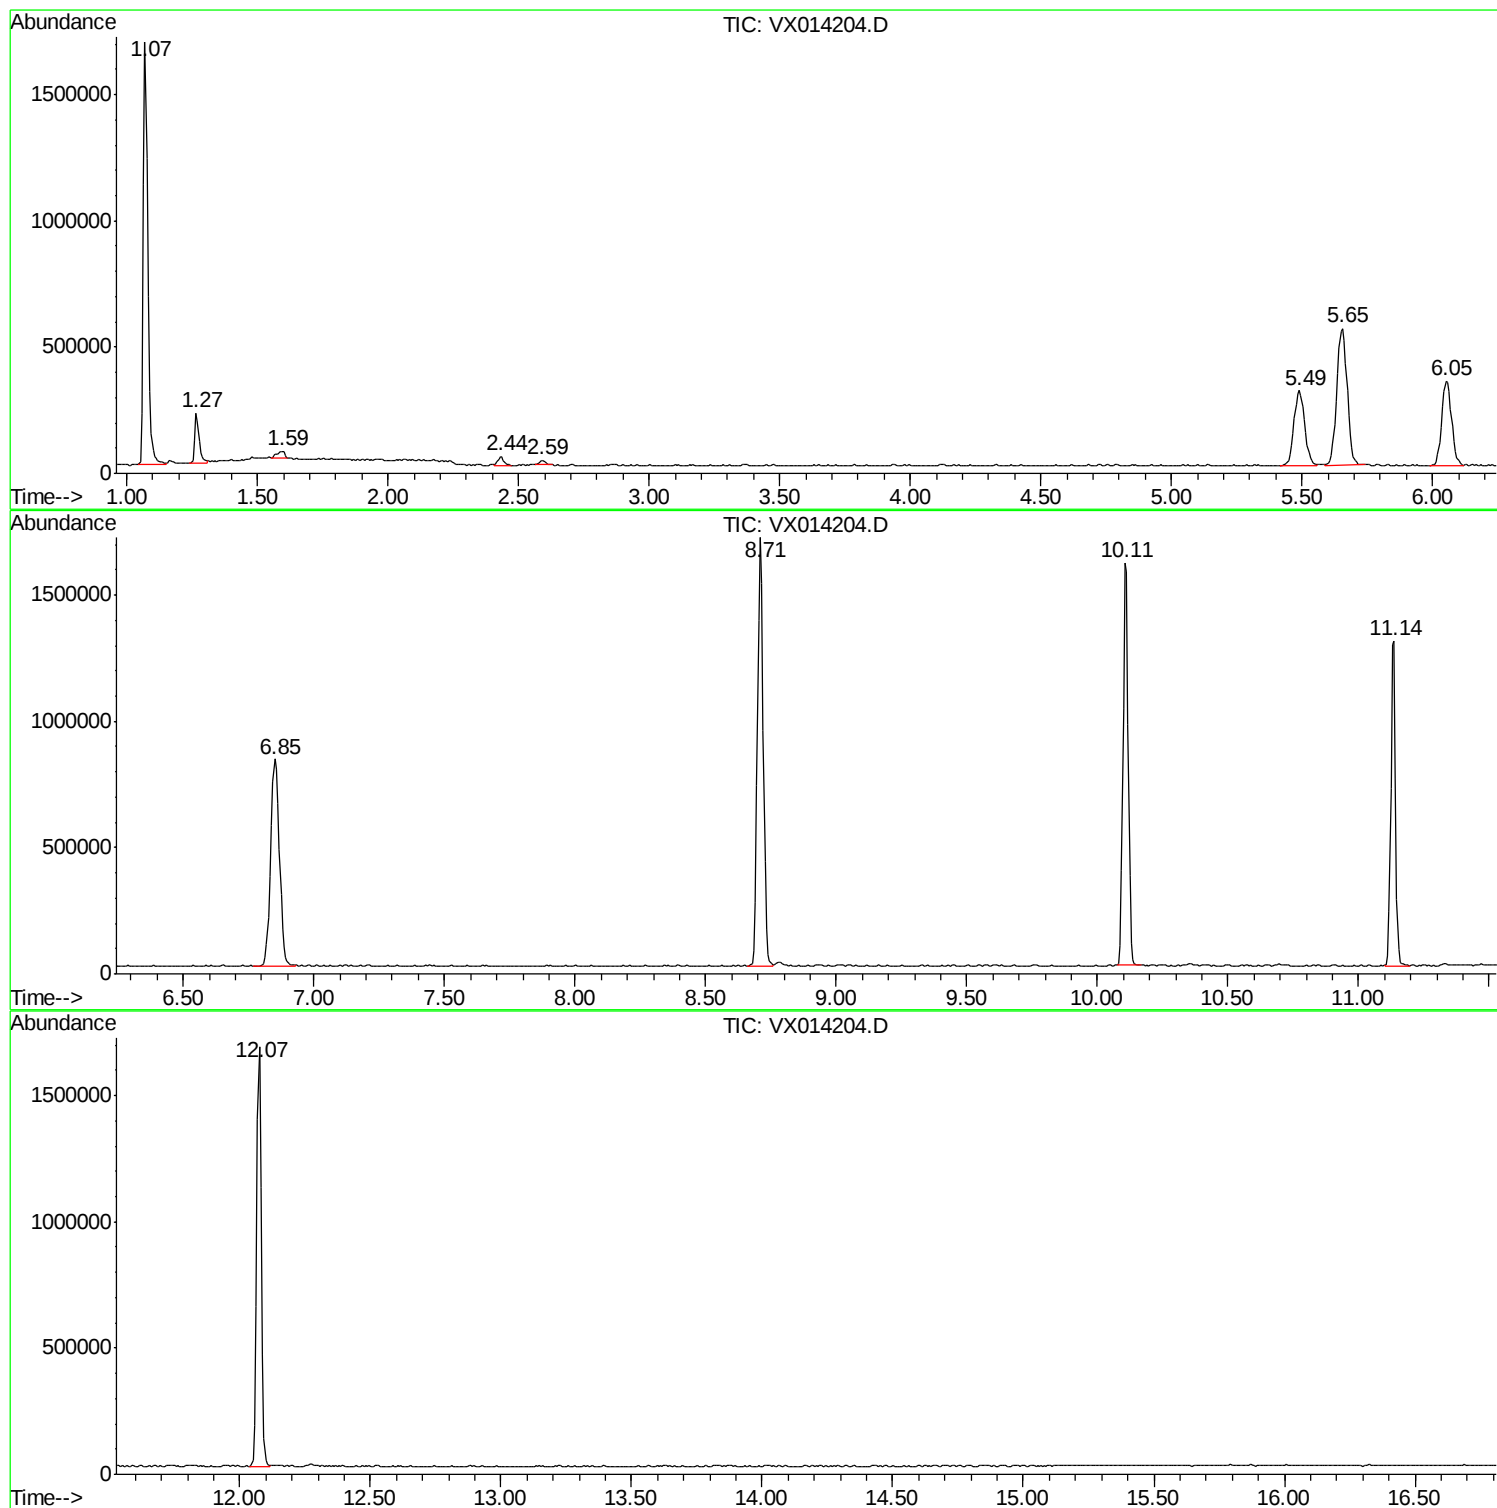

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX122319\
Data File : VX014204.D
Acq On : 23 Dec 2019 15:59
Operator : JC/SP
Sample : K6393-03
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MH-20A










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X121319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Sulfur dioxide Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.27	8.07 ug/l	243443	Pentafluorobenzene	5.65

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Sulfur dioxide	64	O2S	007446-09-5	90
2		Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	64
3		L-Alanine, 3-sulfo-	169	C3H7NO5S	000498-40-8	9
4		Ethene, 1,1-difluoro-	64	C2H2F2	000075-38-7	5
5		Ethyl Chloride	64	C2H5Cl	000075-00-3	3

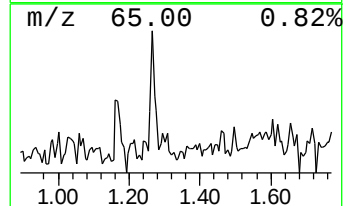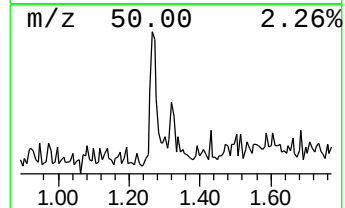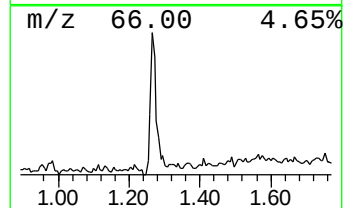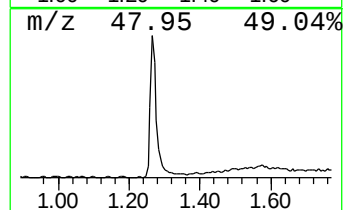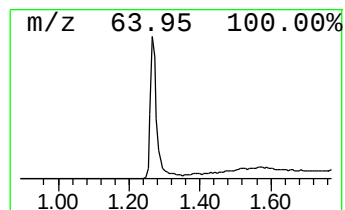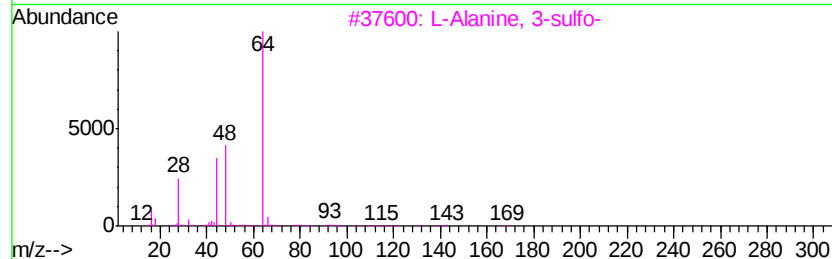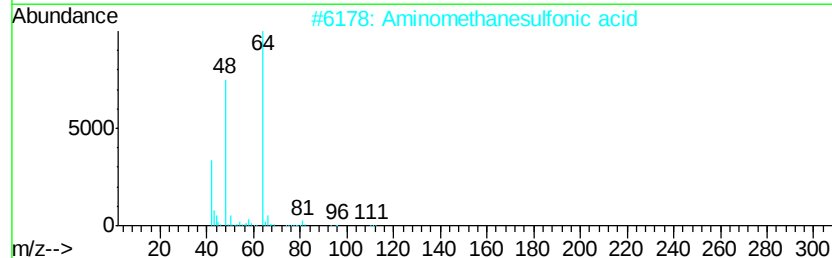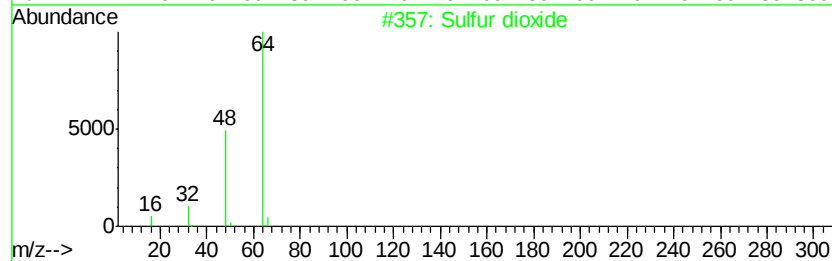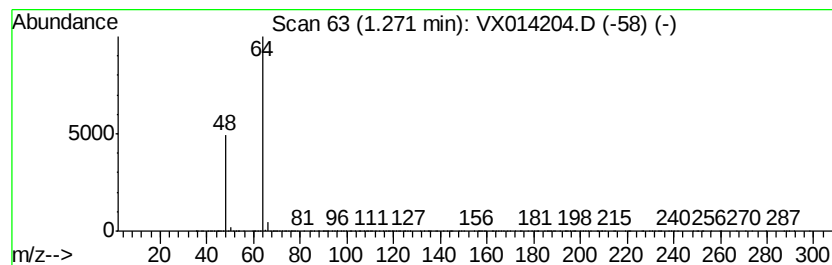

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX122319\
Data File : VX014204.D
Acq On : 23 Dec 2019 15:59
Operator : JC/SP
Sample : K6393-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MH-20A

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X121319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.27	8.1	ug/l	243443	1	5.65	1507780	50.0