


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX122319\
Data File : VX014190.D
Acq On : 23 Dec 2019 09:10
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X121319W.M
Title : SW846 8260
Last Update : Tue Dec 17 03:01:07 2019

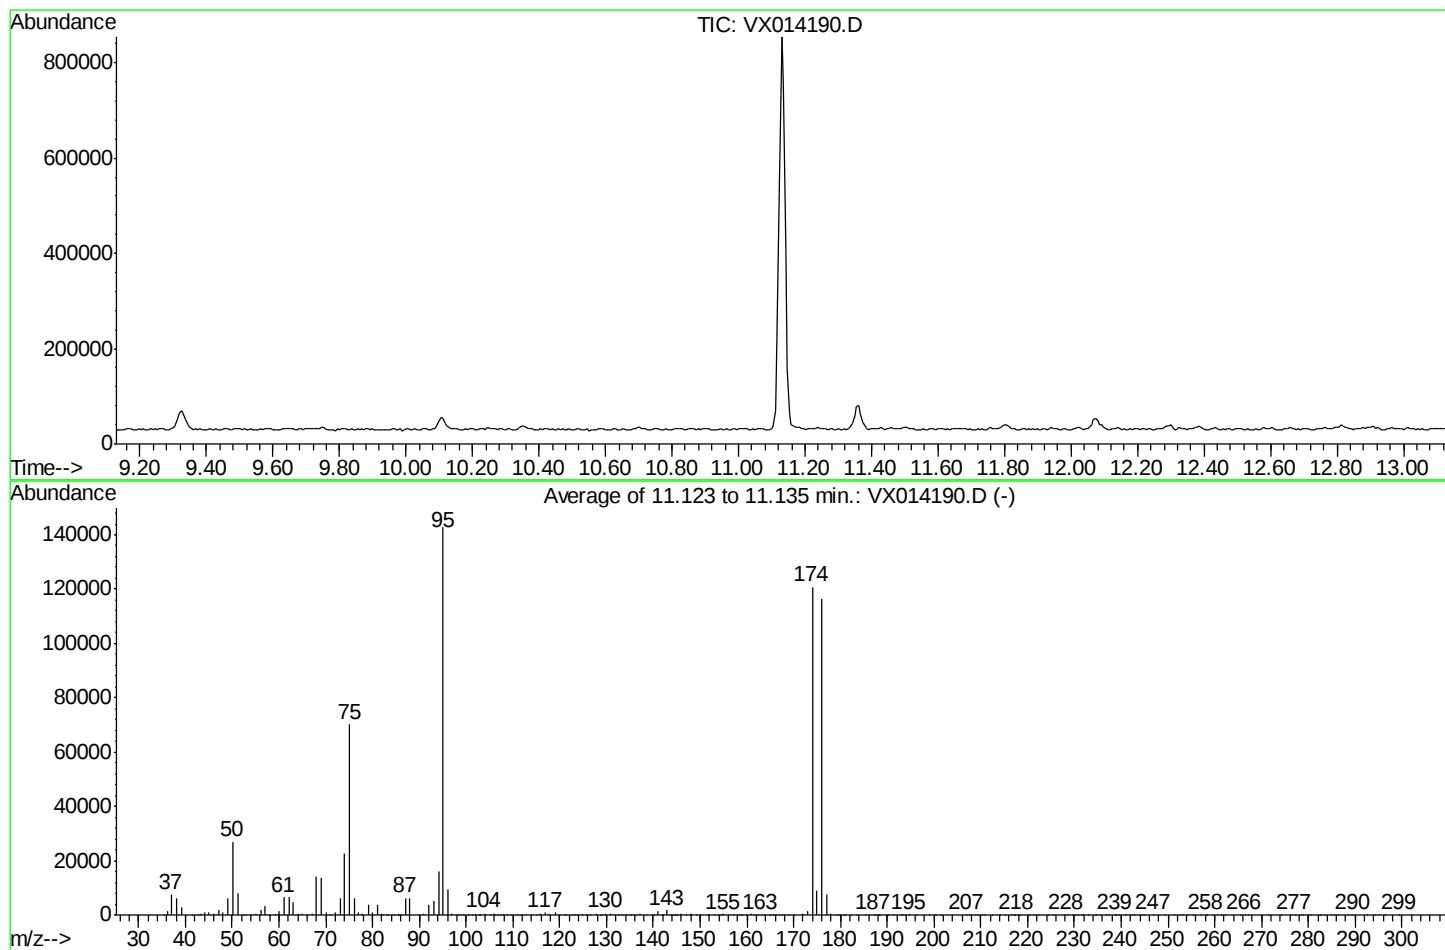

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1671

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	26907	PASS
75	95	30	60	49.2	70165	PASS
95	95	100	100	100.0	142752	PASS
96	95	5	9	6.6	9372	PASS
173	174	0.00	2	1.3	1610	PASS
174	95	50	100	84.7	120909	PASS
175	174	5	9	7.5	9023	PASS
176	174	95	101	96.3	116487	PASS
177	176	5	9	6.6	7698	PASS