


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122320\
Data File : VX020325.D
Acq On : 23 Dec 2020 08:47
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X121820W.M
Title : SW846 8260
Last Update : Fri Dec 18 13:09:49 2020

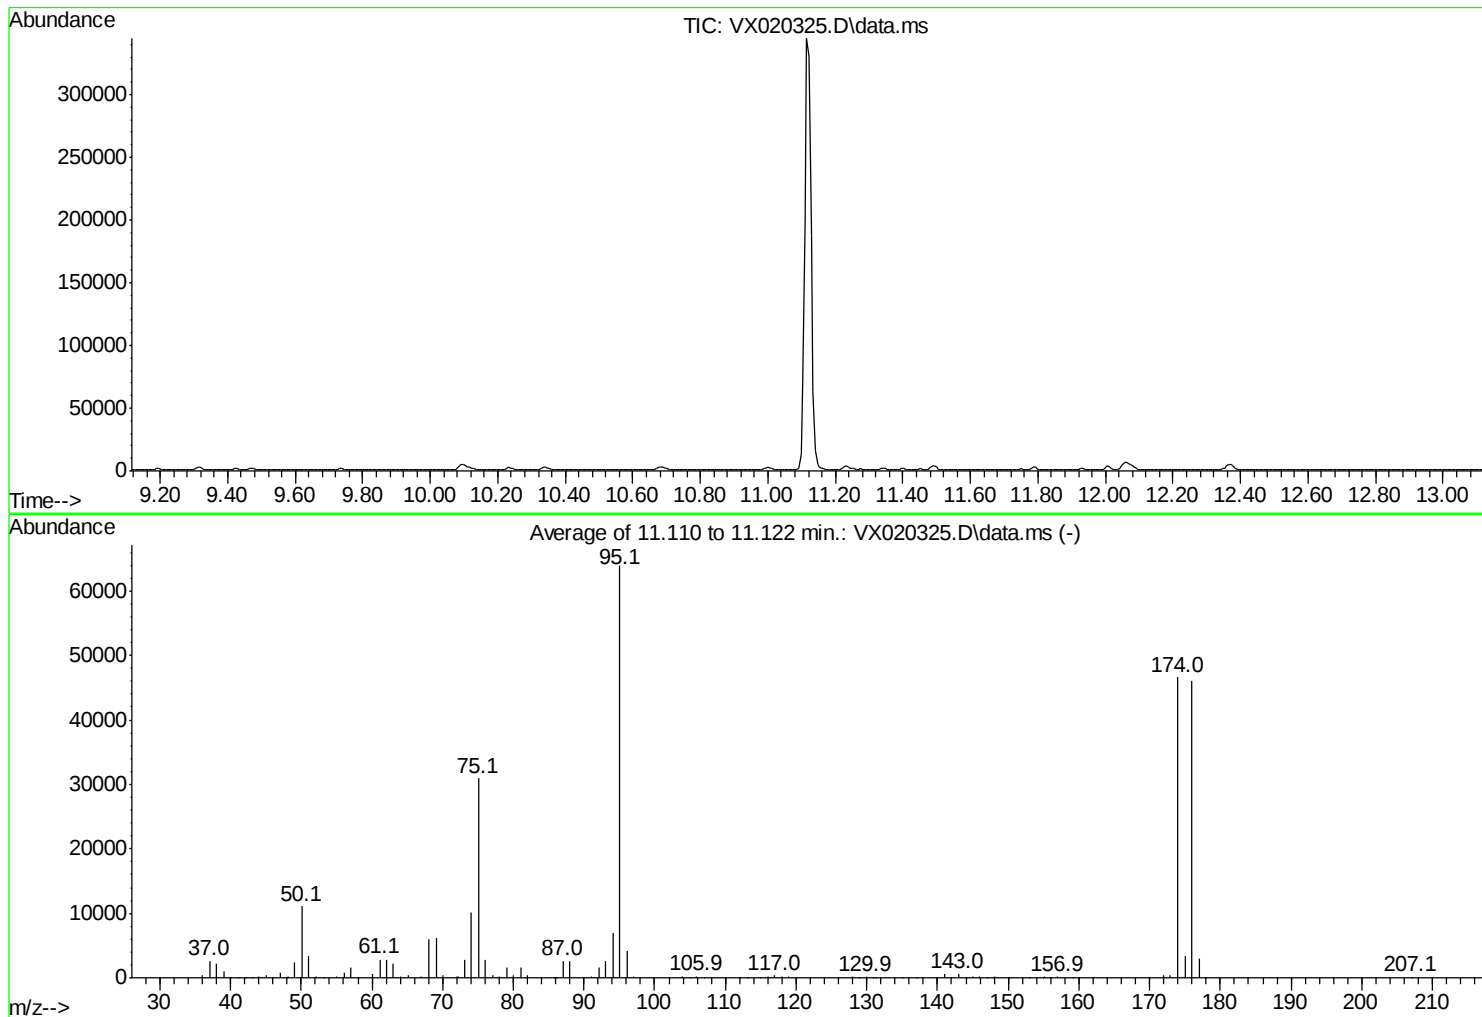

AutoFind: Scans 1644, 1645, 1646; Background Corrected with Scan 1637

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	11035	PASS
75	95	30	60	48.3	30885	PASS
95	95	100	100	100.0	63915	PASS
96	95	5	9	6.6	4235	PASS
173	174	0.00	2	0.9	402	PASS
174	95	50	100	73.0	46637	PASS
175	174	5	9	7.4	3456	PASS
176	174	95	101	98.6	45987	PASS
177	176	5	9	6.5	2982	PASS