


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122320\
Data File : VX020352.D
Acq On : 23 Dec 2020 20:57
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X121820W.M
Title : SW846 8260
Last Update : Fri Dec 18 13:09:49 2020

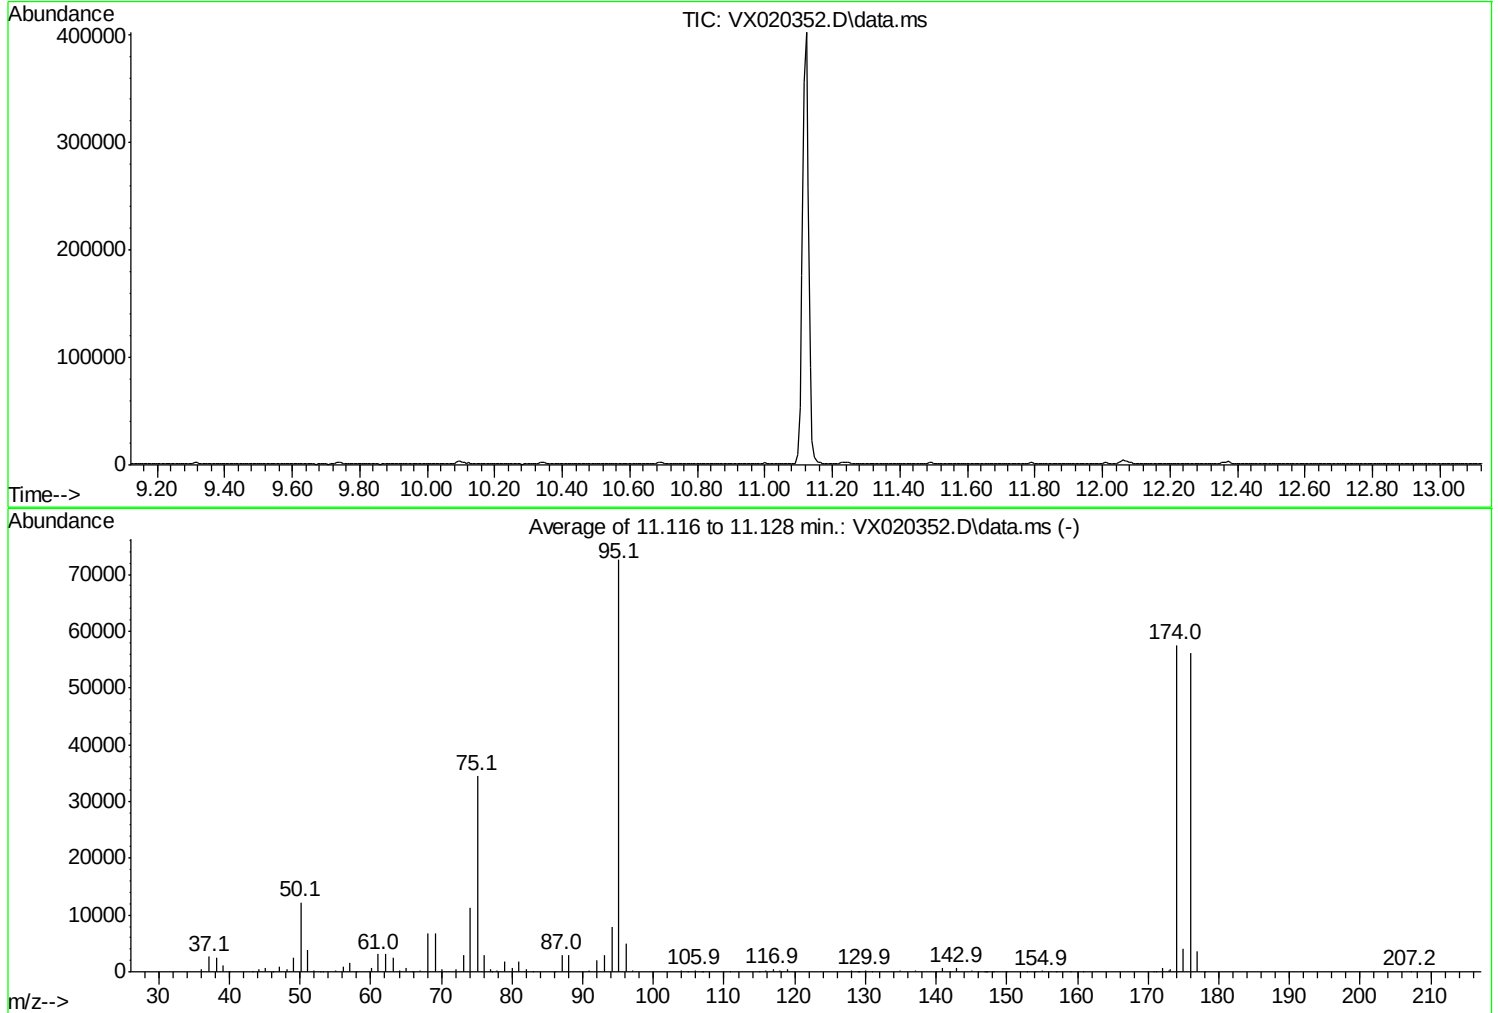

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1638

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.9	12254	PASS
75	95	30	60	47.7	34595	PASS
95	95	100	100	100.0	72597	PASS
96	95	5	9	6.7	4874	PASS
173	174	0.00	2	0.6	361	PASS
174	95	50	100	79.2	57512	PASS
175	174	5	9	7.1	4076	PASS
176	174	95	101	97.5	56099	PASS
177	176	5	9	6.5	3639	PASS