




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122321\
 Data File : VX025991.D
 Acq On : 24 Dec 2021 00:09
 Operator : JC/MD
 Sample : M5154-03ME
 Misc : 6.66g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BGL83ME

Manual IntegrationsAPPROVED

Quant Time: Dec 24 06:48:51 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Dec 23 21:00:32 2021
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/26/2021
 Supervised By :Mahesh Dadoda 12/28/2021

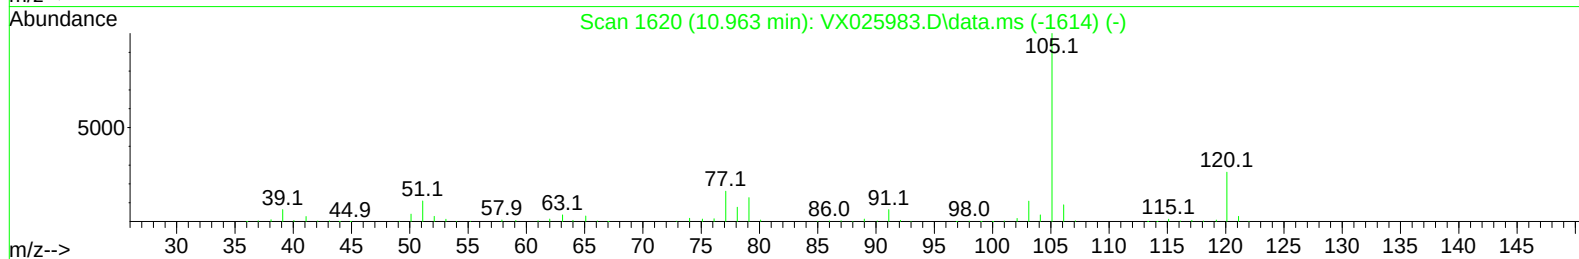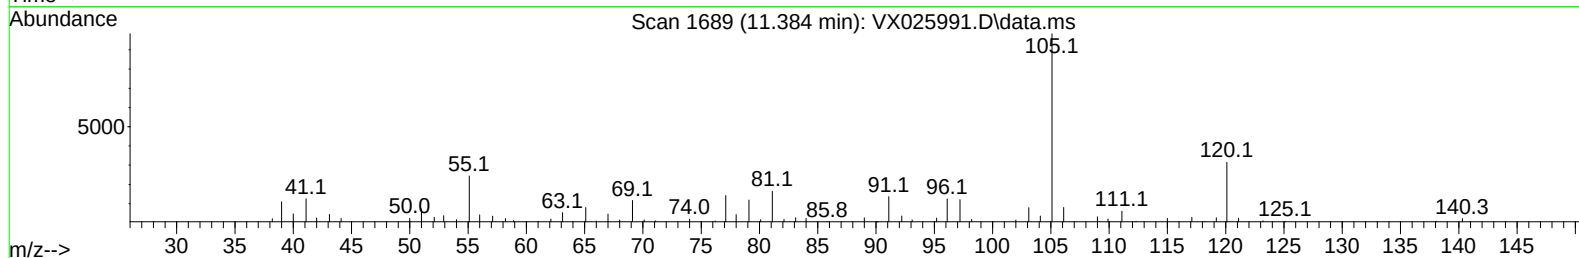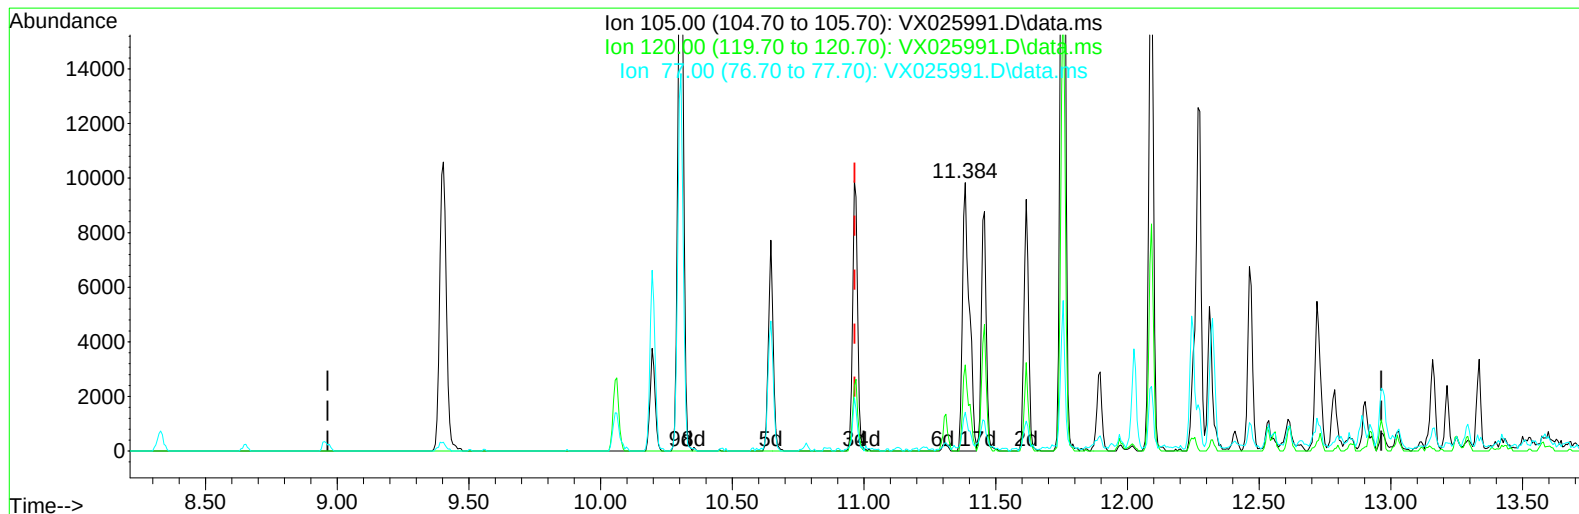

TIC: VX025991.D\data.ms

(60) Isopropylbenzene

11.384min (+ 0.421) 2.68 ug/L

response 17855

Ion	Exp%	Act%
105.00	100.00	100.00
120.00	27.90	30.59
77.00	14.40	13.28
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122321\
 Data File : VX025991.D
 Acq On : 24 Dec 2021 00:09
 Operator : JC/MD
 Sample : M5154-03ME
 Misc : 6.66g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BGL83ME

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/26/2021
 Supervised By :Mahesh Dadoda 12/28/2021

Quant Time: Dec 24 06:48:51 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Dec 23 21:00:32 2021
 Response via : Initial Calibration

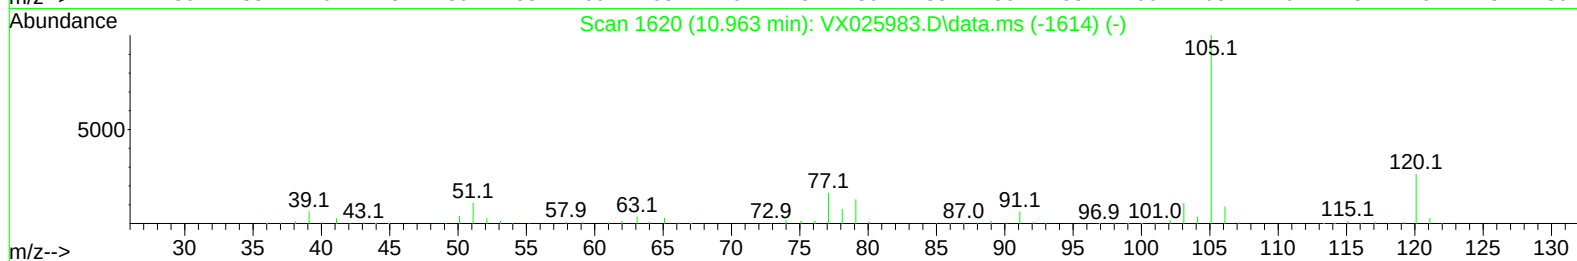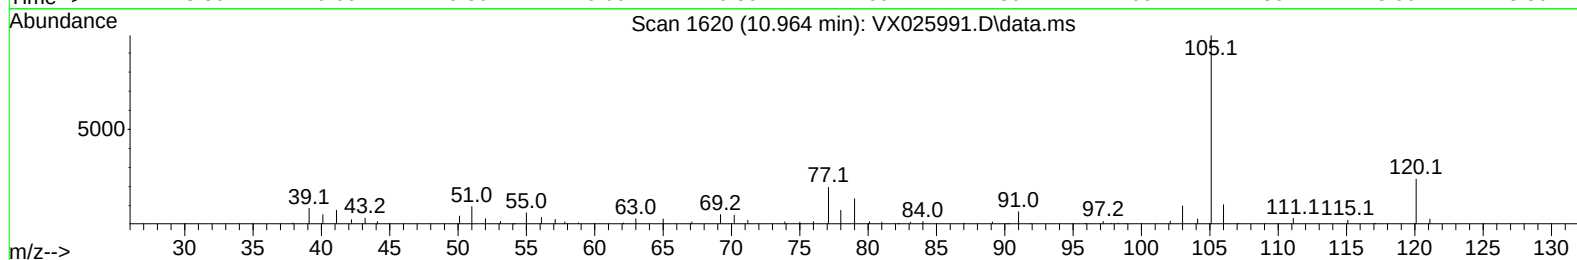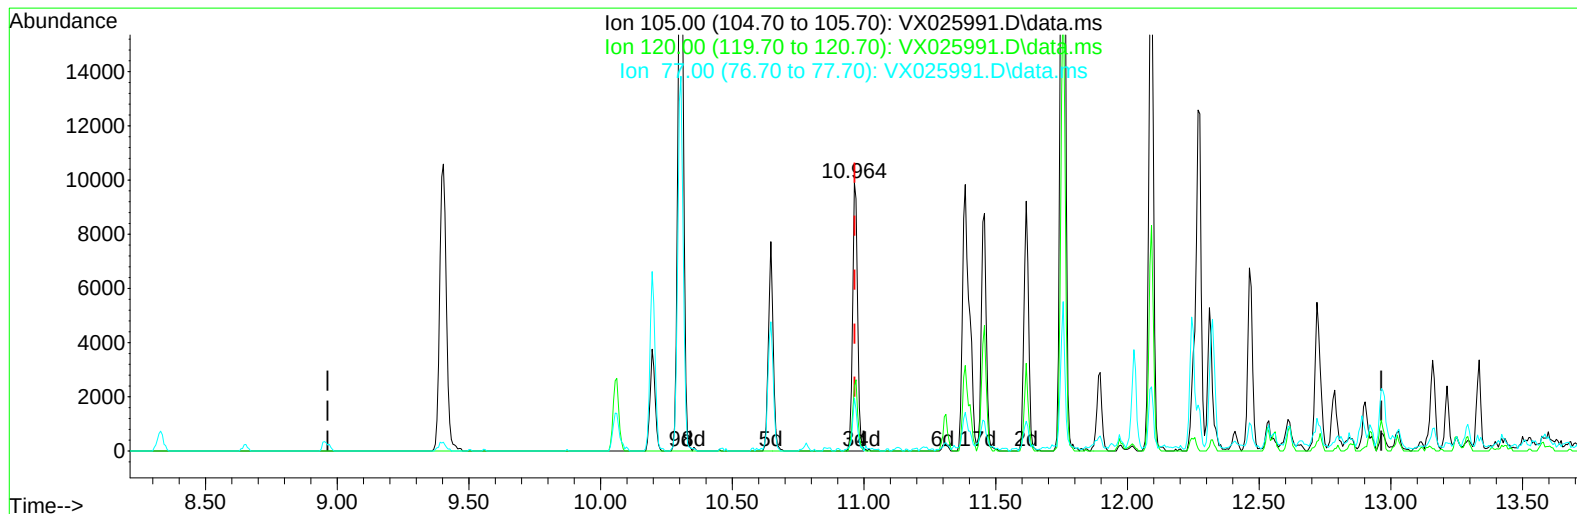

TIC: VX025991.D\data.ms

(60) Isopropylbenzene

10.964min (+ 0.000) 1.92 ug/L m

response 12782

Ion	Exp%	Act%
105.00	100.00	100.00
120.00	27.90	42.73#
77.00	14.40	18.56#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122321\
 Data File : VX025991.D
 Acq On : 24 Dec 2021 00:09
 Operator : JC/MD
 Sample : M5154-03ME
 Misc : 6.66g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BGL83ME

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/26/2021
 Supervised By :Mahesh Dadoda 12/28/2021

Quant Time: Dec 24 06:48:51 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Dec 23 21:00:32 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	210490	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	190816	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	96884	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.374	65	76722	51.399	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 102.800%			
7) Chloroethane-d5	1.648	69	32993	27.658	ug/L	-0.02
Spiked Amount 50.000	Range 70 - 130		Recovery = 55.320%#			
11) 1,1-Dichloroethene-d2	2.282	63	123355	41.703	ug/L	-0.03
Spiked Amount 50.000	Range 60 - 125		Recovery = 83.400%			
21) 2-Butanone-d5	4.489	46	106009	81.916	ug/L	0.03
Spiked Amount 100.000	Range 40 - 130		Recovery = 81.920%			
24) Chloroform-d	5.062	84	145260	48.629	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 97.260%			
26) 1,2-Dichloroethane-d4	5.958	65	105823	52.324	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 104.640%			
32) Benzene-d6	5.971	84	312843	56.960	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 113.920%			
36) 1,2-Dichloropropane-d6	7.312	67	95710	56.060	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 112.120%			
41) Toluene-d8	8.647	98	282706	55.129	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 110.260%			
43) trans-1,3-Dichloroprop...	8.952	79	28851	38.842	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 77.680%			
47) 2-Hexanone-d5	9.403	63	91273	103.588	ug/L	0.02
Spiked Amount 100.000	Range 45 - 130		Recovery = 103.590%			
56) 1,1,2,2-Tetrachloroeth...	11.195	84	130734	51.932	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 103.860%			
66) 1,2-Dichlorobenzene-d4	12.323	152	110161	60.171	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 120.340%#			
Target Compounds						
52) Ethylbenzene	10.195	91	97953	13.996	ug/L	95
53) m,p-Xylene	10.305	106	69394	25.976	ug/L	92
54) o-Xylene	10.647	106	23045	8.709	ug/L	94
60) Isopropylbenzene	10.964	105	12782m	1.920	ug/L	
62) 1,3,5-Trimethylbenzene	11.457	105	11557	2.074	ug/L	98
63) 1,2,4-Trimethylbenzene	11.756	105	46354	8.302	ug/L #	81

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122321\
Data File : VX025991.D
Acq On : 24 Dec 2021 00:09
Operator : JC/MD
Sample : M5154-03ME
Misc : 6.66g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BGL83ME

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/26/2021
Supervised By :Mahesh Dadoda 12/28/2021

Quant Time: Dec 24 06:48:51 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Dec 23 21:00:32 2021
Response via : Initial Calibration

