

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122321\
 Data File : VX025988.D
 Acq On : 23 Dec 2021 22:32
 Operator : JC/MD
 Sample : VX1223WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK656

Quant Time: Dec 24 06:48:29 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Dec 23 21:00:32 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	207153	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	192746	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	91946	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.374	65	78687	53.565	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 107.140%			
7) Chloroethane-d5	1.666	69	63330	53.945	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 107.880%			
11) 1,1-Dichloroethene-d2	2.313	63	113995	39.159	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 78.320%			
21) 2-Butanone-d5	4.459	46	134440	105.558	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 105.560%			
24) Chloroform-d	5.062	84	145259	49.412	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 98.820%			
26) 1,2-Dichloroethane-d4	5.958	65	105575	53.043	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 106.080%			
32) Benzene-d6	5.977	84	302505	54.526	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 109.060%			
36) 1,2-Dichloropropane-d6	7.312	67	96070	55.708	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 111.420%			
41) Toluene-d8	8.653	98	272138	52.536	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 105.080%			
43) trans-1,3-Dichloroprop...	8.952	79	38109	50.792	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 101.580%			
47) 2-Hexanone-d5	9.385	63	99640	111.951	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 111.950%			
56) 1,1,2,2-Tetrachloroeth...	11.195	84	130596	51.358	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 102.720%			
66) 1,2-Dichlorobenzene-d4	12.323	152	95770	55.120	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 110.240%			
Target Compounds						Qvalue
14) Carbon disulfide	2.514	76	3598	0.936	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122321\
Data File : VX025988.D
Acq On : 23 Dec 2021 22:32
Operator : JC/MD
Sample : VX1223WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK656

Quant Time: Dec 24 06:48:29 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Dec 23 21:00:32 2021
Response via : Initial Calibration

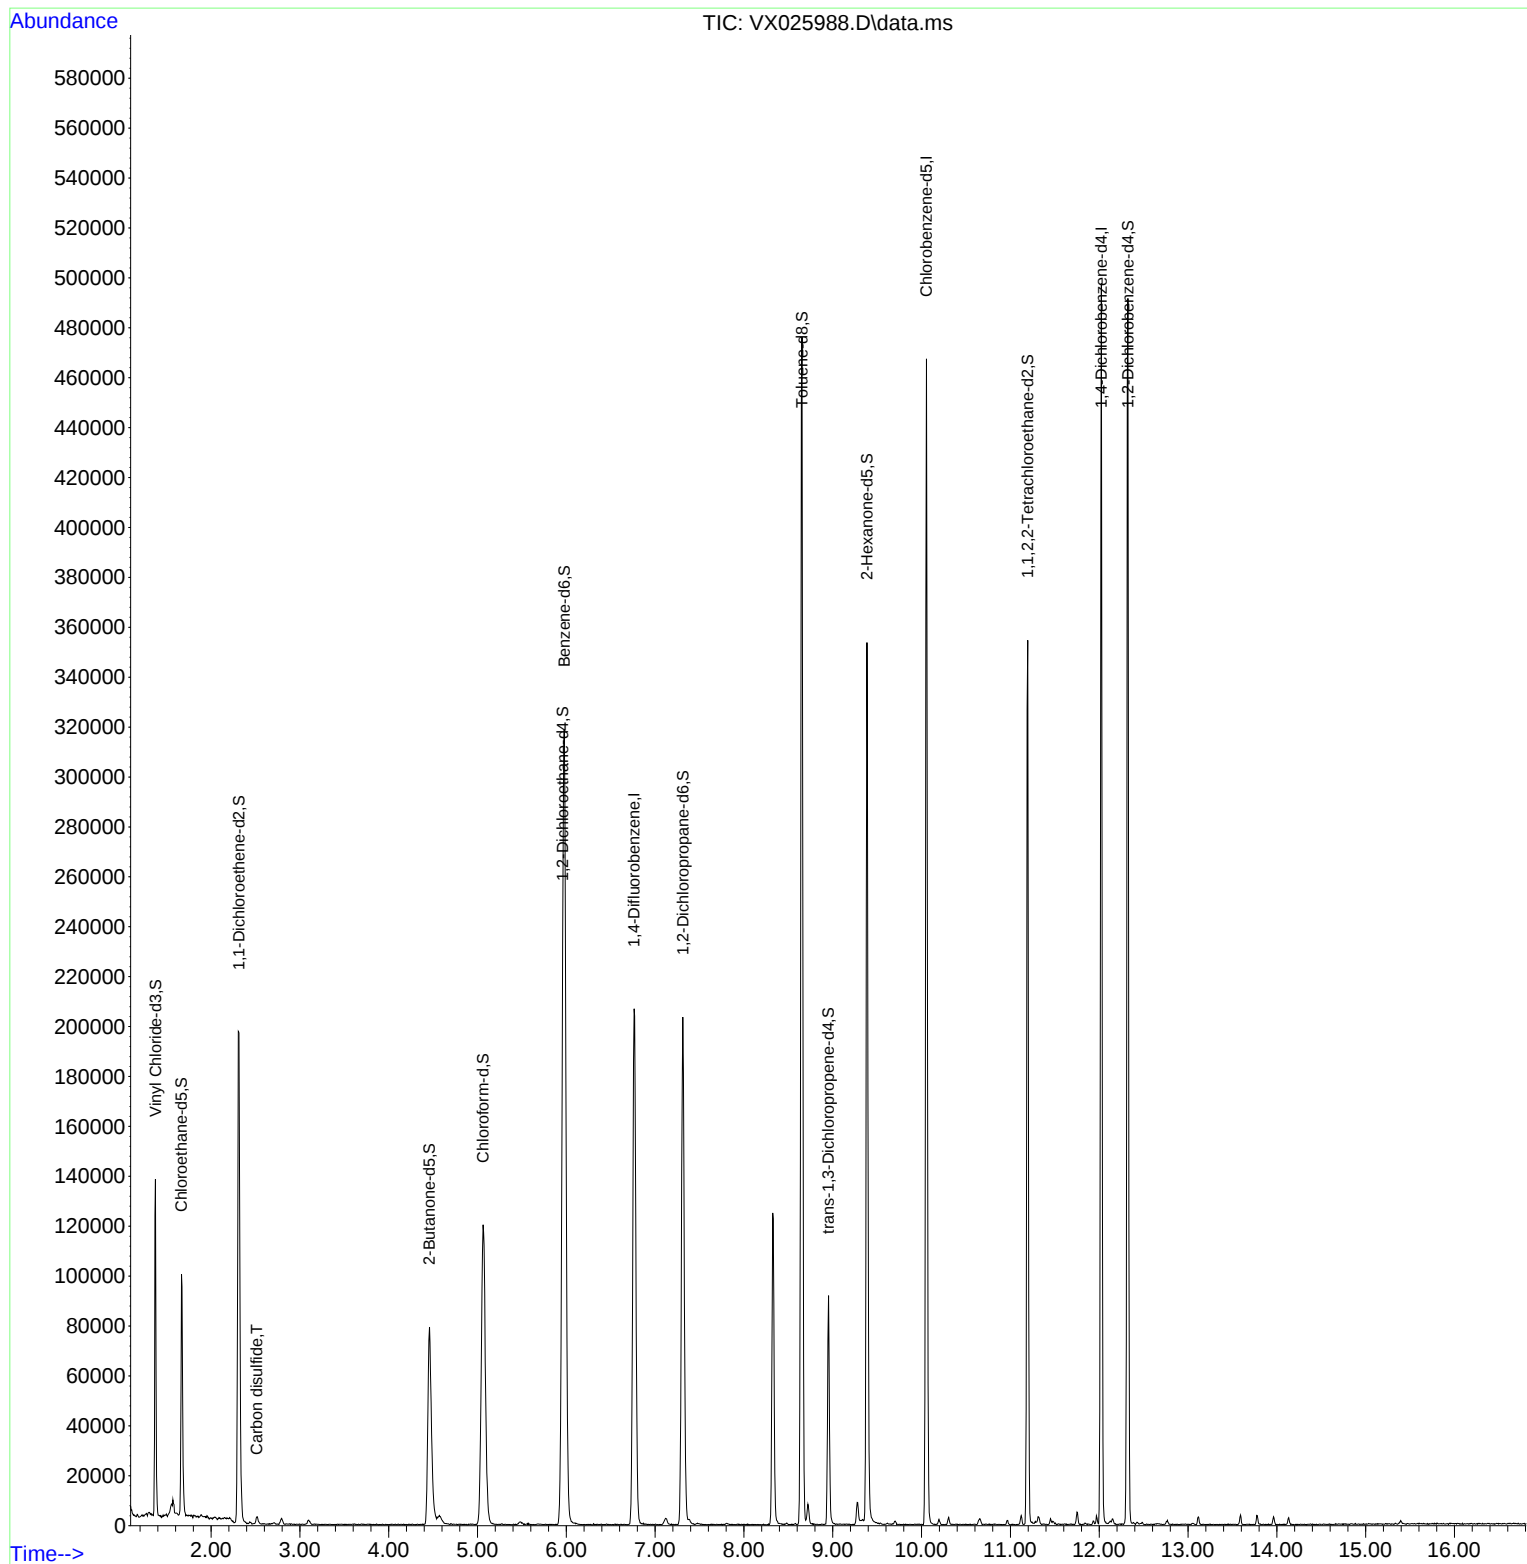

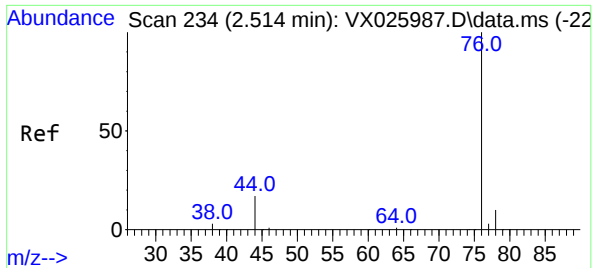

#14
Carbon disulfide
Concen: 0.936 ug/L
RT: 2.514 min Scan# 21
Delta R.T. 0.000 min
Lab File: VX025988.D
Acq: 23 Dec 2021 22:32

Instrument :
MSVOA_X
ClientSampleId :
VBLK656

Tgt Ion: 76 Resp: 3598
Ion Ratio Lower Upper
76 100
78 8.7 7.4 11.2

