

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122321\
 Data File : VX025988.D
 Acq On : 23 Dec 2021 22:32
 Operator : JC/MD
 Sample : VX1223WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK656

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
 Title : VOC Analysis

Signal : TIC: VX025988.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	58	rVB	135496	137016	14.47%	1.922%
2	1.666	91	95	103	rVB	96737	124912	13.19%	1.752%
3	2.307	194	200	211	rBV	196719	329884	34.85%	4.627%
4	2.435	219	221	225	rVB3	888	1102	0.12%	0.015%
5	2.520	230	235	243	rVB	2929	5463	0.58%	0.077%
6	2.794	275	280	287	rBV4	2402	4330	0.46%	0.061%
7	2.904	296	298	300	rBV2	317	312	0.03%	0.004%
8	2.959	305	307	312	rBV3	159	283	0.03%	0.004%
9	3.099	326	330	338	rVB4	1712	3286	0.35%	0.046%
10	3.428	381	384	385	rBV3	293	314	0.03%	0.004%
11	3.690	424	427	429	rBV	295	291	0.03%	0.004%
12	3.861	454	455	459	rVB3	350	324	0.03%	0.005%
13	3.904	459	462	464	rBV2	189	239	0.03%	0.003%
14	3.928	464	466	468	rBV2	266	265	0.03%	0.004%
15	3.965	470	472	477	rBV3	179	298	0.03%	0.004%
16	4.190	507	509	512	rBV2	191	235	0.02%	0.003%
17	4.264	519	521	523	rBV2	252	273	0.03%	0.004%
18	4.324	527	531	533	rBV	334	460	0.05%	0.006%
19	4.459	544	553	566	rBV	79002	223492	23.61%	3.135%
20	4.696	591	592	595	rBV2	345	300	0.03%	0.004%
21	5.062	640	652	669	rBV	120112	381845	40.33%	5.356%
22	5.269	684	686	689	rBV3	297	344	0.04%	0.005%
23	5.404	706	708	710	rVB2	271	190	0.02%	0.003%
24	5.483	714	721	723	rBV5	1140	2481	0.26%	0.035%
25	5.568	734	735	736	rVV	548	201	0.02%	0.003%
26	5.977	789	802	820	rBV2	318553	946695	100.00%	13.278%
27	6.306	854	856	858	rBV	480	320	0.03%	0.004%
28	6.452	878	880	882	rBV2	278	215	0.02%	0.003%
29	6.550	893	896	899	rBV2	350	449	0.05%	0.006%
30	6.763	918	931	944	rBV	206855	500949	52.92%	7.026%
31	7.117	982	989	999	rBV7	2569	6524	0.69%	0.092%
32	7.312	1012	1021	1031	rBV	203337	438276	46.30%	6.147%
33	7.635	1073	1074	1076	rBV2	264	205	0.02%	0.003%
34	7.696	1081	1084	1086	rBV2	209	238	0.03%	0.003%
35	7.745	1091	1092	1094	rVB	396	232	0.02%	0.003%
36	7.769	1094	1096	1097	rBV	368	345	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122321\
 Data File : VX025988.D
 Acq On : 23 Dec 2021 22:32
 Operator : JC/MD
 Sample : VX1223WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK656

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis

37	7.927	1119	1122	1123	rBV2	223	251	0.03%	0.004%
38	7.970	1128	1129	1132	rVB2	227	213	0.02%	0.003%
39	8.025	1136	1138	1140	rVB	248	206	0.02%	0.003%
40	8.043	1140	1141	1144	rBV	363	239	0.03%	0.003%
41	8.220	1168	1170	1172	rVB	375	270	0.03%	0.004%
42	8.324	1180	1187	1198	rBV	125015	212085	22.40%	2.975%
43	8.653	1234	1241	1248	rBV	475615	750137	79.24%	10.521%
44	8.720	1248	1252	1258	rVB2	7840	12411	1.31%	0.174%
45	8.952	1284	1290	1303	rVB	91651	130944	13.83%	1.837%
46	9.275	1338	1343	1348	rBV2	8890	15262	1.61%	0.214%
47	9.385	1356	1361	1377	rVB	352726	493880	52.17%	6.927%
48	9.702	1409	1413	1416	rVB3	1423	2070	0.22%	0.029%
49	10.055	1465	1471	1485	rBV	467122	618051	65.29%	8.669%
50	10.195	1490	1494	1499	rVB	2026	2547	0.27%	0.036%
51	10.305	1508	1512	1517	rBV	2850	3633	0.38%	0.051%
52	10.494	1542	1543	1546	rVB2	261	190	0.02%	0.003%
53	10.653	1564	1569	1574	rVB5	2437	4664	0.49%	0.065%
54	10.695	1574	1576	1577	rBV2	191	198	0.02%	0.003%
55	10.726	1579	1581	1583	rBV2	242	220	0.02%	0.003%
56	10.970	1617	1621	1624	rVB3	1660	2075	0.22%	0.029%
57	11.122	1642	1646	1651	rVV	3694	4698	0.50%	0.066%
58	11.195	1652	1658	1668	rVV	354347	460008	48.59%	6.452%
59	11.281	1670	1672	1673	rVV	1259	1121	0.12%	0.016%
60	11.317	1675	1678	1684	rVB3	3092	5117	0.54%	0.072%
61	11.451	1696	1700	1703	rBV	2282	2787	0.29%	0.039%
62	11.750	1744	1749	1754	rBV4	5061	6817	0.72%	0.096%
63	11.841	1758	1764	1768	rBV3	722	1113	0.12%	0.016%
64	11.933	1776	1779	1782	rBV2	1502	1768	0.19%	0.025%
65	11.969	1782	1785	1789	rVV	3347	3368	0.36%	0.047%
66	12.024	1789	1794	1803	rVV	496980	600939	63.48%	8.429%
67	12.152	1812	1815	1819	rVB2	2090	2809	0.30%	0.039%
68	12.256	1830	1832	1835	rBV2	400	361	0.04%	0.005%
69	12.323	1835	1843	1852	rBV	491287	640828	67.69%	8.988%
70	12.427	1857	1860	1864	rBV3	917	1379	0.15%	0.019%
71	12.536	1876	1878	1879	rBV	298	252	0.03%	0.004%
72	12.768	1912	1916	1919	rVB	1628	2021	0.21%	0.028%
73	12.823	1924	1925	1929	rBV2	264	254	0.03%	0.004%
74	12.878	1932	1934	1936	rBV2	272	247	0.03%	0.003%
75	13.055	1960	1963	1969	rVB4	606	1063	0.11%	0.015%
76	13.116	1969	1973	1980	rVB3	3172	4431	0.47%	0.062%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122321\
 Data File : VX025988.D
 Acq On : 23 Dec 2021 22:32
 Operator : JC/MD
 Sample : VX1223WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK656

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis

77	13.170	1980	1982	1987	rBV2	254	384	0.04%	0.005%
78	13.250	1992	1995	1998	rVB	255	223	0.02%	0.003%
79	13.353	2010	2012	2013	rBV	262	225	0.02%	0.003%
80	13.481	2030	2033	2035	rBV	202	207	0.02%	0.003%
81	13.591	2046	2051	2055	rBV4	3945	4932	0.52%	0.069%
82	13.774	2078	2081	2089	rBV	3758	5124	0.54%	0.072%
83	13.963	2108	2112	2116	rVB	3194	4121	0.44%	0.058%
84	14.134	2136	2140	2144	rVB	2781	3562	0.38%	0.050%
85	14.353	2173	2176	2178	rBV2	262	386	0.04%	0.005%
86	14.402	2183	2184	2186	rVV	350	232	0.02%	0.003%
87	14.524	2202	2204	2207	rBV2	255	311	0.03%	0.004%
88	14.975	2276	2278	2281	rVB2	319	272	0.03%	0.004%
89	15.005	2281	2283	2284	rBV2	305	210	0.02%	0.003%
90	15.115	2299	2301	2303	rBV2	302	201	0.02%	0.003%
91	15.225	2317	2319	2321	rBV2	357	317	0.03%	0.004%
92	15.335	2334	2337	2341	rBV2	512	592	0.06%	0.008%
93	15.396	2341	2347	2350	rBV5	1505	2371	0.25%	0.033%
94	15.469	2357	2359	2363	rBV4	376	554	0.06%	0.008%
95	15.719	2399	2400	2403	rBV2	320	336	0.04%	0.005%
96	15.950	2435	2438	2439	rBV	526	462	0.05%	0.006%
97	16.091	2459	2461	2462	rVB	497	254	0.03%	0.004%
98	16.115	2462	2465	2467	rBV3	293	376	0.04%	0.005%
99	16.274	2489	2491	2492	rBV2	395	335	0.04%	0.005%
100	16.316	2496	2498	2501	rVB2	312	213	0.02%	0.003%




Sum of corrected areas: 7129715

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122321\
Data File : VX025988.D
Acq On : 23 Dec 2021 22:32
Operator : JC/MD
Sample : VX1223WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK656

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

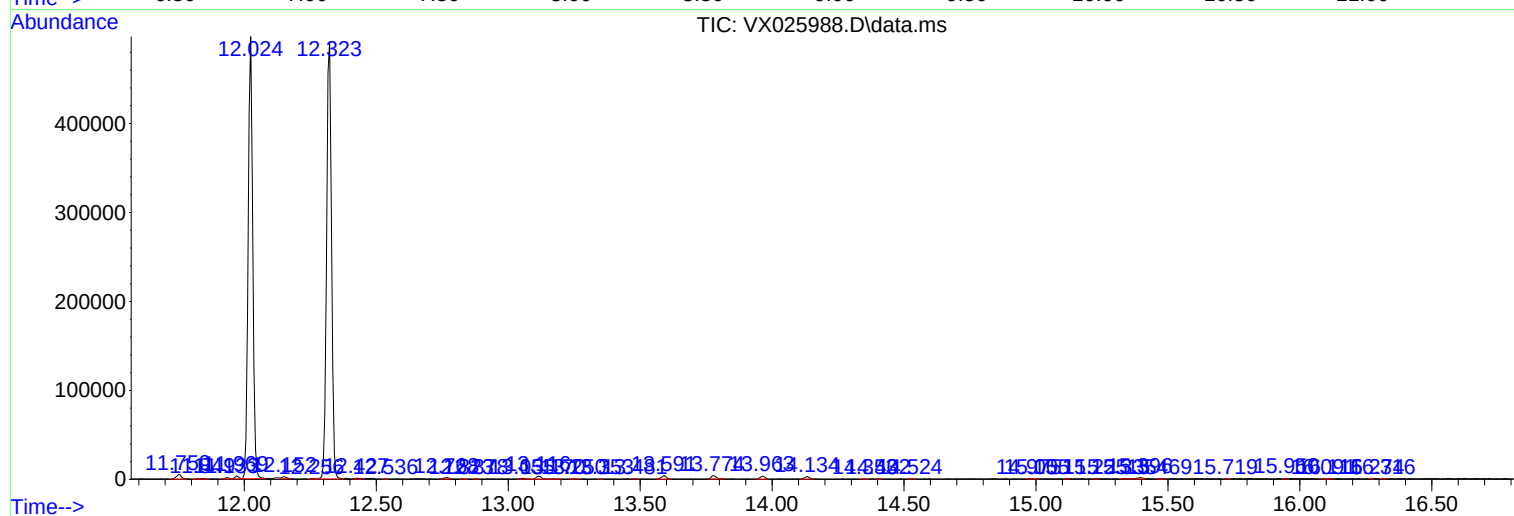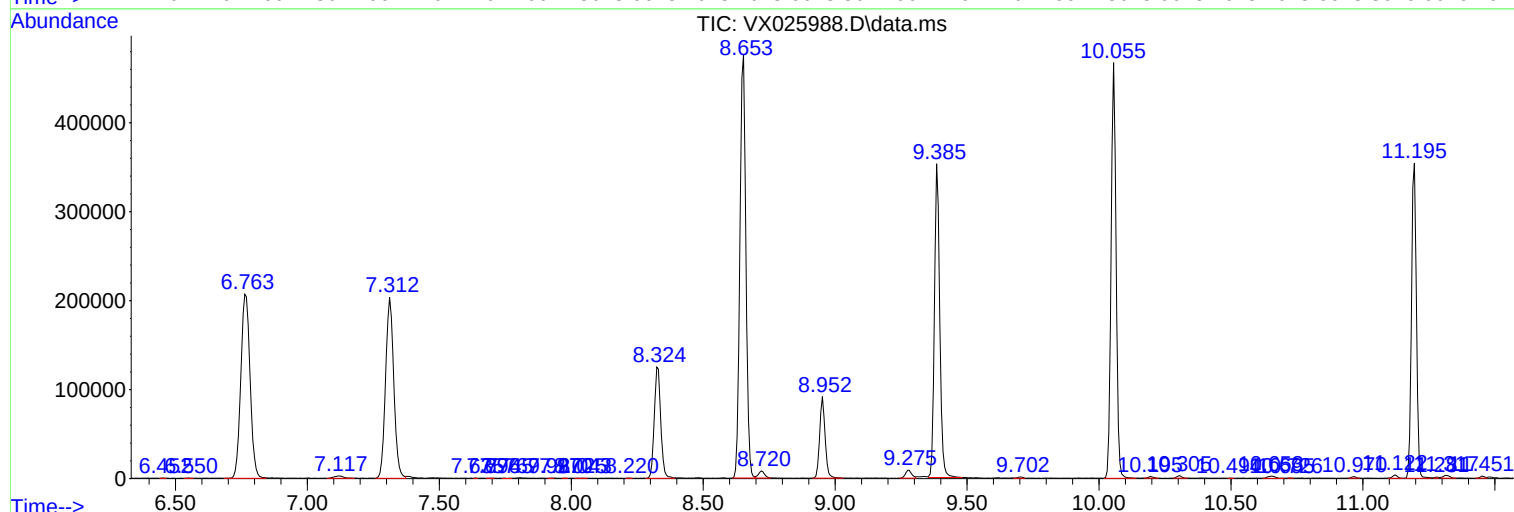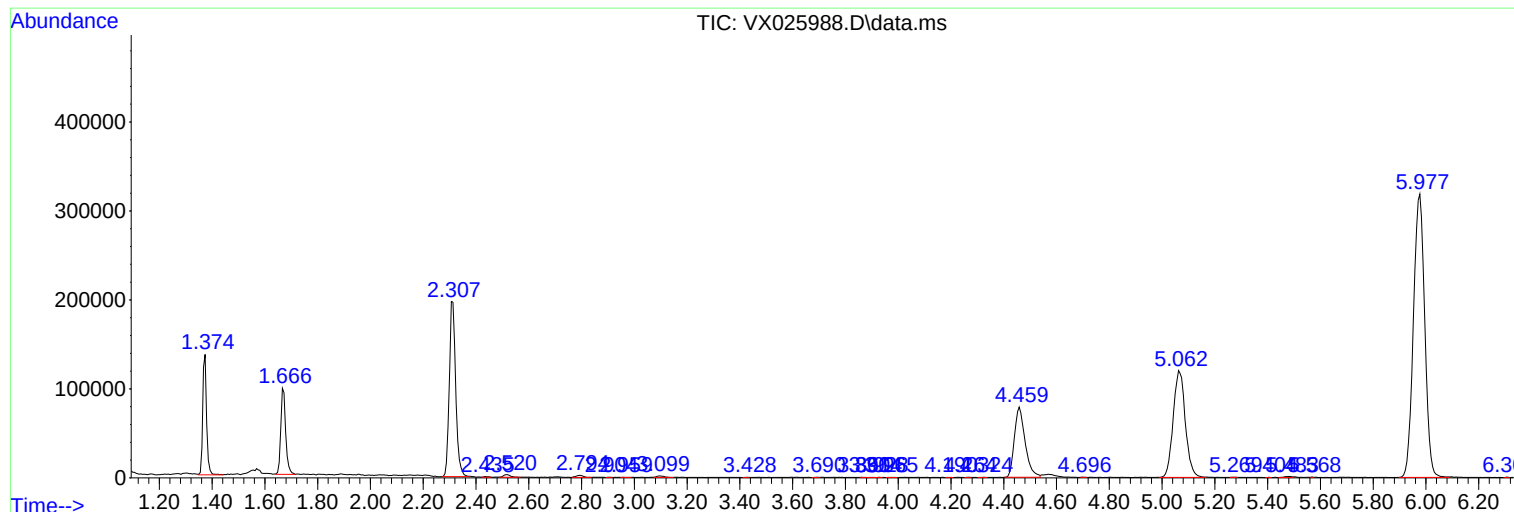

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122321\
Data File : VX025988.D
Acq On : 23 Dec 2021 22:32
Operator : JC/MD
Sample : VX1223WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK656

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122321\
Data File : VX025988.D
Acq On : 23 Dec 2021 22:32
Operator : JC/MD
Sample : VX1223WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK656

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc