

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122321\
 Data File : VX026004.D
 Acq On : 24 Dec 2021 05:17
 Operator : JC/MD
 Sample : M4975-06DL2 4000X
 Misc : 6.78g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BGKT0DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis

Signal : TIC: VX026004.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	54	rVB	146864	145787	14.40%	1.973%
2	1.672	91	96	103	rBV	103144	136291	13.46%	1.845%
3	2.313	195	201	215	rVB	226438	362897	35.84%	4.911%
4	2.654	255	257	258	rVB	311	156	0.02%	0.002%
5	2.794	275	280	286	rVB	3679	6549	0.65%	0.089%
6	2.849	286	289	290	rBV2	320	313	0.03%	0.004%
7	2.953	305	306	307	rBV	227	140	0.01%	0.002%
8	3.068	324	325	327	rBV	294	167	0.02%	0.002%
9	3.087	327	328	330	rVV	286	203	0.02%	0.003%
10	3.123	332	334	336	rBV	202	204	0.02%	0.003%
11	3.172	340	342	344	rBV	237	156	0.02%	0.002%
12	3.264	355	357	361	rVB2	277	281	0.03%	0.004%
13	3.325	365	367	369	rVV2	274	238	0.02%	0.003%
14	3.483	392	393	396	rVB	357	275	0.03%	0.004%
15	3.507	396	397	398	rBV	238	147	0.01%	0.002%
16	3.837	448	451	453	rBV2	136	154	0.02%	0.002%
17	3.867	453	456	457	rVV2	163	158	0.02%	0.002%
18	3.885	457	459	460	rVV	266	173	0.02%	0.002%
19	3.904	460	462	469	rVV2	190	376	0.04%	0.005%
20	3.965	469	472	474	rVB	293	310	0.03%	0.004%
21	3.983	474	475	477	rBV	216	174	0.02%	0.002%
22	4.007	477	479	481	rVB	302	251	0.02%	0.003%
23	4.062	486	488	489	rBV	305	192	0.02%	0.003%
24	4.080	489	491	492	rVB	223	124	0.01%	0.002%
25	4.184	506	508	511	rBV2	238	204	0.02%	0.003%
26	4.263	519	521	524	rVB2	161	133	0.01%	0.002%
27	4.318	529	530	533	rBV	371	244	0.02%	0.003%
28	4.349	533	535	537	rBV2	248	212	0.02%	0.003%
29	4.458	544	553	575	rBV	71766	221867	21.91%	3.003%
30	4.757	601	602	605	rVB2	283	259	0.03%	0.004%
31	4.836	614	615	618	rVB	358	181	0.02%	0.002%
32	4.964	634	636	638	rBV2	303	297	0.03%	0.004%
33	5.068	640	653	671	rVV	128275	396794	39.19%	5.370%
34	5.385	699	705	706	rBV2	413	752	0.07%	0.010%
35	5.531	724	729	730	rBV3	229	407	0.04%	0.006%
36	5.739	761	763	764	rVB	255	128	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122321\
 Data File : VX026004.D
 Acq On : 24 Dec 2021 05:17
 Operator : JC/MD
 Sample : M4975-06DL2 4000X
 Misc : 6.78g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BGKT0DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis

37	5.824	775	777	780	rVB2	185	122	0.01%	0.002%
38	5.879	784	786	788	rBV	143	121	0.01%	0.002%
39	5.976	788	802	816	rBV2	341170	1012580	100.00%	13.704%
40	6.135	826	828	834	rVB2	369	517	0.05%	0.007%
41	6.184	834	836	837	rVB	185	122	0.01%	0.002%
42	6.379	866	868	870	rBV	326	193	0.02%	0.003%
43	6.440	876	878	879	rVB2	194	138	0.01%	0.002%
44	6.458	879	881	883	rBV	304	296	0.03%	0.004%
45	6.671	914	916	918	rBV	354	260	0.03%	0.004%
46	6.702	920	921	922	rBV	282	176	0.02%	0.002%
47	6.763	922	931	944	rVV	218933	520434	51.40%	7.044%
48	7.013	970	972	974	rVB	342	252	0.02%	0.003%
49	7.037	974	976	977	rBV	254	154	0.02%	0.002%
50	7.056	977	979	982	rVB2	165	143	0.01%	0.002%
51	7.117	982	989	997	rVB5	2153	5139	0.51%	0.070%
52	7.184	997	1000	1001	rBV	214	170	0.02%	0.002%
53	7.196	1001	1002	1003	rBV	318	168	0.02%	0.002%
54	7.312	1012	1021	1034	rBV2	213007	461495	45.58%	6.246%
55	7.482	1045	1049	1051	rBV3	693	919	0.09%	0.012%
56	7.562	1061	1062	1067	rBV2	206	356	0.04%	0.005%
57	7.671	1077	1080	1082	rBV2	364	328	0.03%	0.004%
58	7.726	1085	1089	1090	rVB2	251	308	0.03%	0.004%
59	7.793	1097	1100	1101	rBV2	486	489	0.05%	0.007%
60	7.866	1110	1112	1115	rBV2	159	149	0.01%	0.002%
61	7.891	1115	1116	1118	rBV	224	117	0.01%	0.002%
62	7.921	1119	1121	1122	rBV	237	162	0.02%	0.002%
63	7.982	1130	1131	1133	rVB	341	208	0.02%	0.003%
64	8.001	1133	1134	1135	rVB	314	115	0.01%	0.002%
65	8.019	1135	1137	1140	rBV2	309	462	0.05%	0.006%
66	8.116	1151	1153	1155	rVV2	201	204	0.02%	0.003%
67	8.153	1157	1159	1160	rVB	252	144	0.01%	0.002%
68	8.275	1178	1179	1180	rBV	305	168	0.02%	0.002%
69	8.324	1181	1187	1196	rVV	98870	165936	16.39%	2.246%
70	8.653	1234	1241	1248	rBV	513766	806114	79.61%	10.910%
71	8.720	1248	1252	1257	rVB	7785	12255	1.21%	0.166%
72	8.885	1277	1279	1283	rBV	270	277	0.03%	0.004%
73	8.952	1284	1290	1297	rBV	70525	100569	9.93%	1.361%
74	9.275	1338	1343	1350	rBV2	29446	45557	4.50%	0.617%
75	9.384	1356	1361	1377	rVB	356888	512696	50.63%	6.939%
76	9.762	1421	1423	1425	rBV	311	201	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122321\
 Data File : VX026004.D
 Acq On : 24 Dec 2021 05:17
 Operator : JC/MD
 Sample : M4975-06DL2 4000X
 Misc : 6.78g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BGKT0DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
 Title : VOC Analysis

77	9.787	1425	1427	1428	rVB	251	112	0.01%	0.002%
78	9.921	1448	1449	1450	rBV	203	141	0.01%	0.002%
79	10.055	1465	1471	1481	rBV	480610	641815	63.38%	8.686%
80	10.195	1490	1494	1499	rVB3	2418	3317	0.33%	0.045%
81	10.305	1507	1512	1517	rBV	7463	10529	1.04%	0.142%
82	10.372	1522	1523	1524	rBV	238	114	0.01%	0.002%
83	10.646	1564	1568	1572	rVB3	1754	2430	0.24%	0.033%
84	10.707	1577	1578	1580	rVB	333	178	0.02%	0.002%
85	10.726	1580	1581	1584	rBV	389	301	0.03%	0.004%
86	10.963	1617	1620	1625	rVB	1881	2065	0.20%	0.028%
87	11.122	1643	1646	1652	rVB4	1255	1841	0.18%	0.025%
88	11.195	1652	1658	1665	rBV	372058	466837	46.10%	6.318%
89	11.317	1673	1678	1683	rVB3	3249	5282	0.52%	0.071%
90	11.378	1686	1688	1695	rVB4	2119	3989	0.39%	0.054%
91	11.457	1695	1701	1703	rBV3	1662	2956	0.29%	0.040%
92	11.652	1731	1733	1735	rBV2	296	182	0.02%	0.002%
93	11.683	1735	1738	1740	rBV2	428	429	0.04%	0.006%
94	11.750	1746	1749	1756	rBV4	4338	5757	0.57%	0.078%
95	11.829	1760	1762	1765	rBV2	316	449	0.04%	0.006%
96	11.939	1777	1780	1783	rVB3	742	806	0.08%	0.011%
97	12.024	1788	1794	1800	rBV	494594	617126	60.95%	8.352%
98	12.244	1828	1830	1835	rBV6	677	1133	0.11%	0.015%
99	12.323	1837	1843	1850	rVB	524655	674755	66.64%	9.132%
100	13.780	2078	2082	2087	rVB	12793	18827	1.86%	0.255%


Sum of corrected areas: 7388779

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122321\
Data File : VX026004.D
Acq On : 24 Dec 2021 05:17
Operator : JC/MD
Sample : M4975-06DL2 4000X
Misc : 6.78g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BGKT0DL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

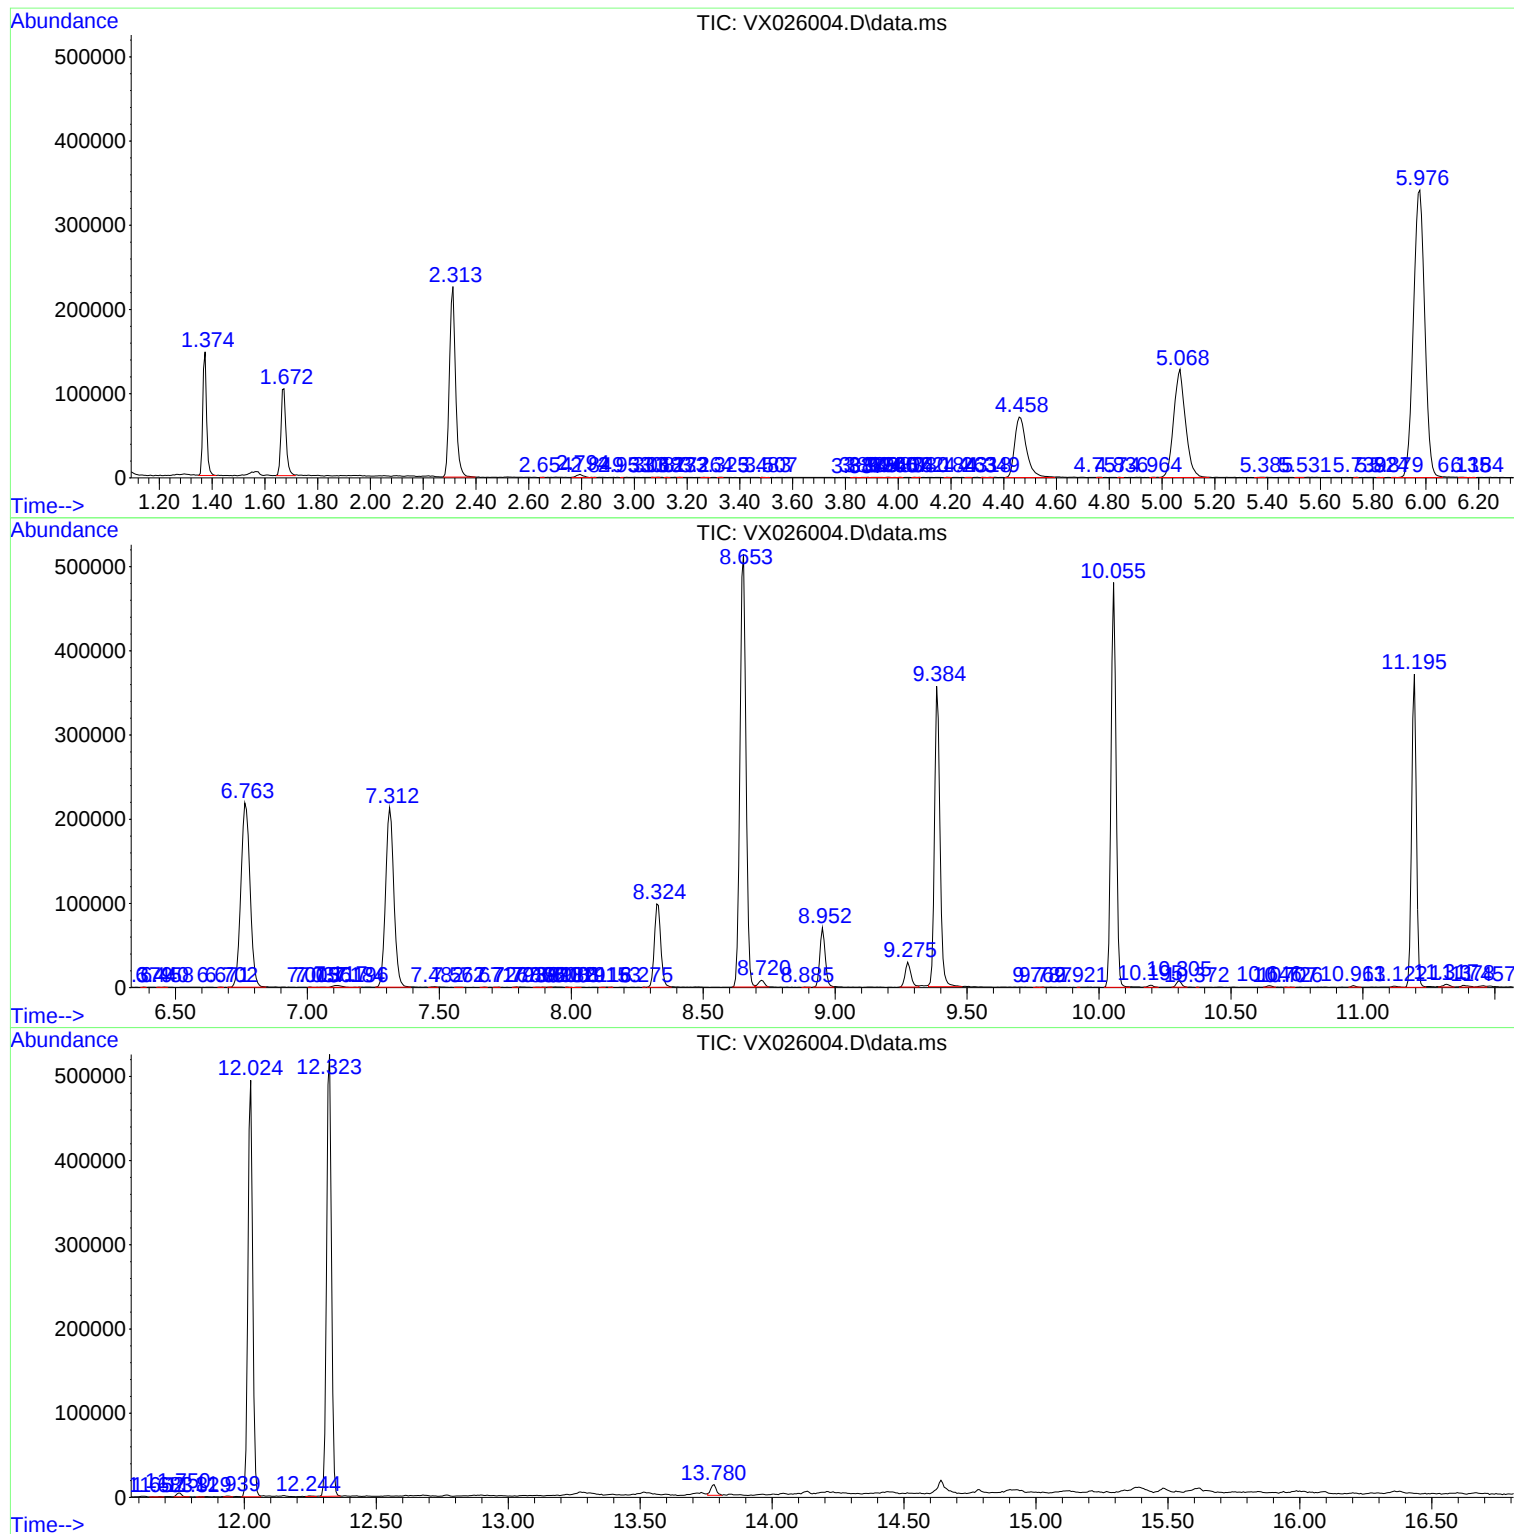

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122321\
Data File : VX026004.D
Acq On : 24 Dec 2021 05:17
Operator : JC/MD
Sample : M4975-06DL2 4000X
Misc : 6.78g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BGKT0DL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122321\
Data File : VX026004.D
Acq On : 24 Dec 2021 05:17
Operator : JC/MD
Sample : M4975-06DL2 4000X
Misc : 6.78g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BGKT0DL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc