
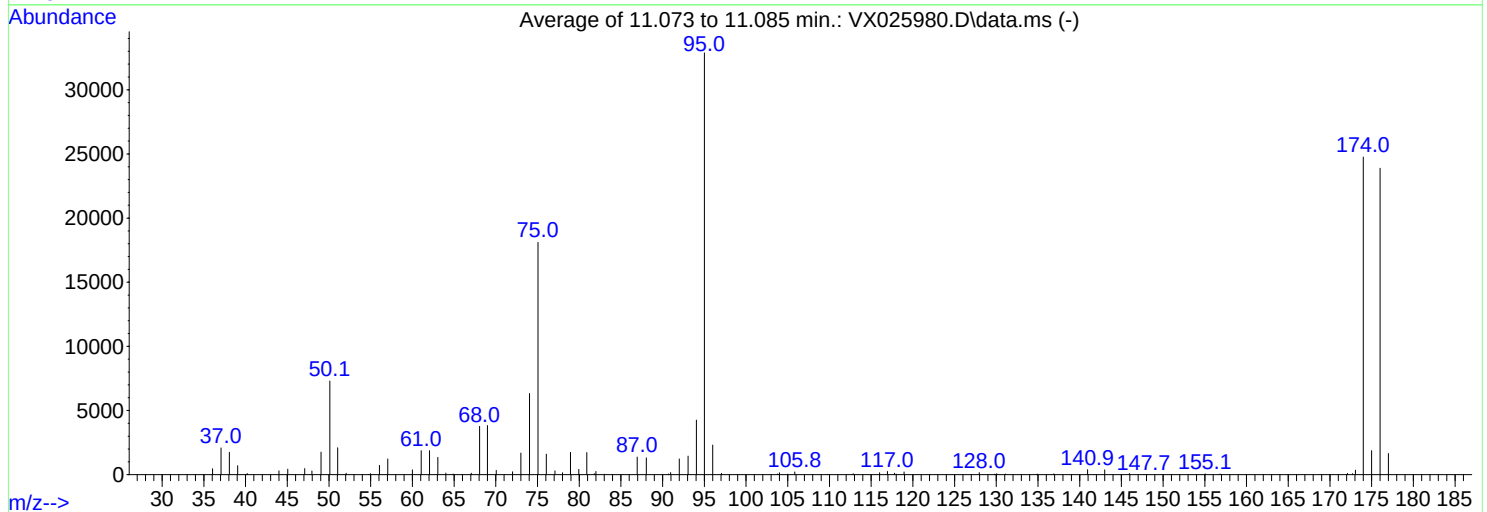


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122321\
 Data File : VX025980.D
 Acq On : 23 Dec 2021 17:50
 Operator : JC/MD
 Sample : BFB628
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB628

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis
 Last Update : Thu Dec 23 21:00:32 2021

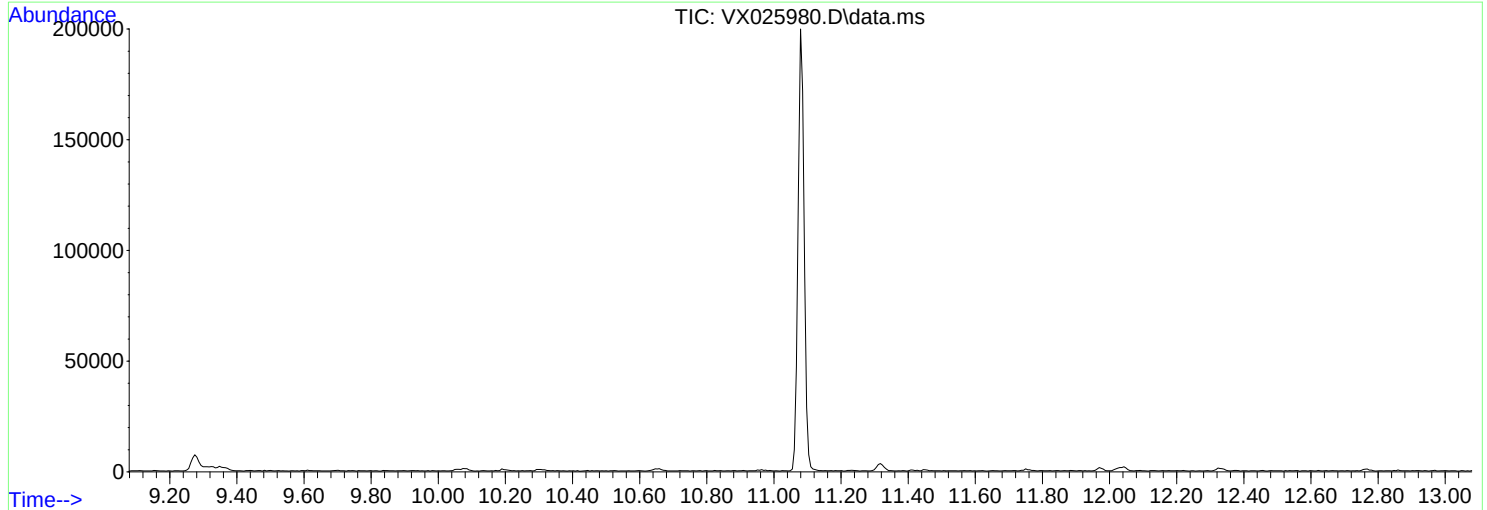

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.2	7292	PASS
75	95	30	80	55.1	18112	PASS
95	95	100	100	100.0	32880	PASS
96	95	5	9	7.0	2303	PASS
173	174	0.00	2	1.4	355	PASS
174	95	50	120	75.3	24758	PASS
175	174	5	9	7.6	1871	PASS
176	174	95	101	96.5	23890	PASS
177	176	5	9	6.9	1645	PASS

m/z	Abundance
40.00	253.0
44.10	164.0

Instrument :
MSVOA_X
ClientSampleId :
BFB628

m/z	Abundance
36.10	395.0
37.10	1953.0
38.10	1456.0
39.10	609.0
40.20	248.0
44.00	453.0
45.00	413.0
47.00	562.0
48.00	254.0
49.10	1399.0
50.10	6976.0
51.00	2132.0
52.10	112.0
55.00	119.0
56.10	677.0
57.00	1247.0
60.00	313.0
61.10	1719.0
62.00	1687.0
63.10	1291.0
64.10	156.0
67.10	72.0
68.10	3802.0
69.00	3627.0
70.00	373.0
72.00	312.0
73.00	1531.0
74.10	6287.0
75.10	17032.0
76.10	1405.0
77.10	231.0
78.00	154.0
79.00	1762.0
80.00	464.0
80.90	1693.0
82.00	331.0
87.00	1481.0
88.00	1341.0
91.00	255.0
92.00	1311.0
93.10	1545.0
94.10	4189.0
95.00	32736.0
96.00	2258.0
97.00	85.0
104.00	177.0
105.00	65.0
105.80	213.0
112.90	93.0
115.90	110.0
117.00	262.0
118.00	136.0
119.00	227.0
128.00	167.0
130.10	113.0
131.10	71.0
134.90	67.0
136.90	101.0
141.00	354.0
143.00	355.0
146.00	132.0
148.10	54.0
155.10	102.0
156.80	58.0
172.10	140.0
173.10	508.0
174.00	28880.0
175.00	2226.0
176.00	27152.0
177.00	1772.0

Instrument :
MSVOA_X
ClientSampleId :
BFB628

m/z	Abundance
36.10	555.0
37.00	2436.0
38.10	2136.0
39.10	858.0
39.90	354.0
44.00	455.0
45.00	450.0
46.00	90.0
47.10	548.0
48.00	369.0
49.00	2239.0
50.10	8972.0
51.10	2270.0
52.00	140.0
55.00	106.0
56.00	856.0
57.10	1359.0
60.00	495.0
61.00	2157.0
62.10	2189.0
63.10	1754.0
64.00	163.0
64.90	75.0
67.00	165.0
68.00	4508.0
69.00	4814.0
70.10	341.0
72.00	207.0
73.00	2017.0
74.10	7413.0
75.10	22752.0
76.10	1961.0
77.10	408.0
78.00	149.0
78.90	2121.0
79.90	402.0
80.90	2060.0
82.00	404.0
83.00	58.0
86.90	1603.0
88.10	1506.0
90.90	245.0
92.00	1229.0
93.00	1770.0
94.00	4974.0
95.00	39016.0
96.00	2725.0
97.10	127.0
104.00	282.0
105.00	56.0
105.90	223.0
109.80	69.0
112.90	82.0
116.00	184.0
117.00	291.0
117.80	197.0
119.00	235.0
127.90	191.0
130.00	104.0
134.90	85.0
136.90	92.0
140.90	478.0
141.70	56.0
143.00	389.0
145.90	60.0
147.70	58.0
155.00	77.0
156.80	102.0
169.90	63.0
172.10	97.0
172.70	236.0
173.00	385.0
174.00	29368.0
175.00	2210.0
176.00	28424.0
177.00	1914.0

Instrument :
MSVOA_X
ClientSampleId :
BFB628

m/z	Abundance
36.00	427.0
37.10	1870.0
38.00	1663.0
39.00	638.0
40.00	330.0
44.00	468.0
45.10	399.0
47.20	333.0
47.90	222.0
49.00	1636.0
50.10	5929.0
51.00	1908.0
52.00	93.0
54.80	94.0
56.00	635.0
57.00	1055.0
60.00	306.0
61.00	1746.0
62.10	1729.0
63.00	988.0
63.90	68.0
64.90	63.0
67.10	99.0
68.00	2980.0
69.00	3048.0
70.00	282.0
72.00	164.0
73.00	1498.0
74.00	5264.0
75.00	14553.0
76.00	1429.0
77.10	270.0
78.00	142.0
78.90	1310.0
79.90	356.0
80.90	1394.0
81.80	241.0
83.00	73.0
87.00	1051.0
88.00	1073.0
90.70	159.0
92.00	1131.0
93.00	1025.0
94.00	3584.0
95.00	26888.0
96.00	1926.0
97.10	72.0
103.80	140.0
105.90	221.0
112.80	59.0
116.00	149.0
116.90	190.0
117.80	127.0
118.90	188.0
128.00	124.0
129.80	101.0
131.10	68.0
140.90	325.0
143.00	385.0
145.90	74.0
172.10	66.0
173.00	172.0
174.00	16025.0
175.00	1177.0
176.00	16095.0
177.00	1249.0

Instrument :
MSVOA_X
ClientSampleId :
BFB628