

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122322\
 Data File : VX033554.D
 Acq On : 23 Dec 2022 10:52
 Operator : JC/MD
 Sample : VX1223MBL01
 Misc : 5.00g/5.0mL/100ul/5.0mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK605

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122222WMA.M
 Title : VOC Analysis

Signal : TIC: VX033554.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	64	rVB	62054	82082	10.76%	1.502%
2	1.672	91	96	109	rVB	53802	74586	9.77%	1.365%
3	2.136	168	172	174	rBV2	218	316	0.04%	0.006%
4	2.307	194	200	211	rBV	164067	258465	33.87%	4.730%
5	2.428	218	220	222	rBV	167	150	0.02%	0.003%
6	2.514	230	234	239	rVB3	709	1281	0.17%	0.023%
7	2.788	275	279	285	rVB3	1248	2391	0.31%	0.044%
8	2.947	302	305	308	rBV	178	268	0.04%	0.005%
9	3.087	326	328	330	rBV2	199	235	0.03%	0.004%
10	3.197	344	346	352	rBV2	166	272	0.04%	0.005%
11	3.264	352	357	358	rBV	141	177	0.02%	0.003%
12	3.282	358	360	363	rBV2	172	177	0.02%	0.003%
13	3.434	381	385	387	rBV2	150	199	0.03%	0.004%
14	3.703	427	429	432	rVB	140	138	0.02%	0.003%
15	3.757	436	438	440	rVB	183	153	0.02%	0.003%
16	3.965	470	472	475	rBV	130	142	0.02%	0.003%
17	4.001	475	478	481	rVV	124	169	0.02%	0.003%
18	4.068	487	489	492	rVB2	173	170	0.02%	0.003%
19	4.105	492	495	498	rBV2	202	293	0.04%	0.005%
20	4.166	500	505	506	rVV	125	166	0.02%	0.003%
21	4.361	535	537	539	rVB2	194	172	0.02%	0.003%
22	4.459	542	553	573	rBV	46638	138195	18.11%	2.529%
23	5.056	639	651	668	rBV	105634	317058	41.55%	5.802%
24	5.172	668	670	671	rVB	325	188	0.02%	0.003%
25	5.190	671	673	675	rBV	158	154	0.02%	0.003%
26	5.385	700	705	714	rVV	803	2076	0.27%	0.038%
27	5.556	725	733	742	rBV3	1920	5117	0.67%	0.094%
28	5.745	762	764	766	rBV2	110	129	0.02%	0.002%
29	5.873	782	785	788	rVB2	180	215	0.03%	0.004%
30	5.964	788	800	817	rBV2	250970	763100	100.00%	13.964%
31	6.275	848	851	852	rBV2	129	156	0.02%	0.003%
32	6.525	889	892	893	rBV	161	174	0.02%	0.003%
33	6.623	906	908	911	rBV2	121	131	0.02%	0.002%
34	6.757	921	930	944	rBV	207965	497368	65.18%	9.102%
35	6.909	953	955	960	rVB	221	362	0.05%	0.007%
36	7.111	983	988	995	rVB3	1606	3492	0.46%	0.064%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122322\
 Data File : VX033554.D
 Acq On : 23 Dec 2022 10:52
 Operator : JC/MD
 Sample : VX1223MBL01
 Misc : 5.00g/5.0mL/100ul/5.0mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK605

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122222WMA.M
 Title : VOC Analysis

37	7.165	995	997	1002	rVB2	123	172	0.02%	0.003%
38	7.306	1012	1020	1032	rBV	155804	339219	44.45%	6.208%
39	7.489	1043	1050	1052	rBV2	361	662	0.09%	0.012%
40	7.592	1063	1067	1069	rBV2	118	182	0.02%	0.003%
41	7.690	1081	1083	1087	rBV2	156	229	0.03%	0.004%
42	7.830	1104	1106	1108	rVB	245	142	0.02%	0.003%
43	7.934	1119	1123	1132	rVB2	1367	2352	0.31%	0.043%
44	8.147	1157	1158	1161	rVB2	162	131	0.02%	0.002%
45	8.324	1181	1187	1198	rBV	106796	171201	22.43%	3.133%
46	8.476	1209	1212	1220	rBV4	824	1693	0.22%	0.031%
47	8.647	1234	1240	1249	rBV	408351	634798	83.19%	11.616%
48	8.830	1268	1270	1272	rBV2	189	177	0.02%	0.003%
49	8.952	1284	1290	1302	rBV	73989	111049	14.55%	2.032%
50	9.104	1313	1315	1319	rBV2	126	144	0.02%	0.003%
51	9.269	1340	1342	1345	rBV2	477	571	0.07%	0.010%
52	9.385	1355	1361	1374	rBV	228214	317203	41.57%	5.805%
53	9.793	1425	1428	1431	rBV2	128	162	0.02%	0.003%
54	9.854	1437	1438	1441	rBV2	122	159	0.02%	0.003%
55	9.927	1447	1450	1455	rVB	159	286	0.04%	0.005%
56	9.994	1455	1461	1465	rBV2	172	445	0.06%	0.008%
57	10.055	1465	1471	1490	rVV	416487	567313	74.34%	10.382%
58	10.195	1492	1494	1501	rVB4	662	840	0.11%	0.015%
59	10.311	1508	1513	1519	rBV3	525	1158	0.15%	0.021%
60	10.646	1565	1568	1570	rBV	640	767	0.10%	0.014%
61	10.726	1576	1581	1583	rBV	182	240	0.03%	0.004%
62	10.823	1596	1597	1601	rBV2	141	204	0.03%	0.004%
63	10.964	1618	1620	1626	rVB2	545	768	0.10%	0.014%
64	11.012	1626	1628	1631	rBV2	119	161	0.02%	0.003%
65	11.092	1637	1641	1644	rBV3	349	399	0.05%	0.007%
66	11.189	1652	1657	1672	rVB	269574	353402	46.31%	6.467%
67	11.311	1675	1677	1682	rVB3	260	348	0.05%	0.006%
68	11.360	1682	1685	1686	rBV2	136	185	0.02%	0.003%
69	11.457	1697	1701	1704	rVB	569	752	0.10%	0.014%
70	11.549	1715	1716	1719	rBB	207	205	0.03%	0.004%
71	11.585	1719	1722	1725	rBV2	164	286	0.04%	0.005%
72	11.628	1727	1729	1731	rVB	189	172	0.02%	0.003%
73	11.689	1735	1739	1742	rVV2	790	954	0.13%	0.017%
74	11.762	1742	1751	1753	rVB4	417	836	0.11%	0.015%
75	11.793	1753	1756	1757	rBV2	129	127	0.02%	0.002%
76	11.976	1782	1786	1788	rBV2	739	878	0.12%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122322\
 Data File : VX033554.D
 Acq On : 23 Dec 2022 10:52
 Operator : JC/MD
 Sample : VX1223MBL01
 Misc : 5.00g/5.0mL/100ul/5.0mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK605

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122222WMA.M
 Title : VOC Analysis

77	12.024	1788	1794	1803	rBV	305112	384386	50.37%	7.034%
78	12.134	1811	1812	1815	rVB	192	143	0.02%	0.003%
79	12.189	1819	1821	1823	rVB	235	161	0.02%	0.003%
80	12.232	1826	1828	1829	rBV	174	148	0.02%	0.003%
81	12.323	1837	1843	1850	rBV	310105	408765	53.57%	7.480%
82	12.408	1855	1857	1859	rVV	283	189	0.02%	0.003%
83	12.457	1862	1865	1868	rBB	183	225	0.03%	0.004%
84	12.488	1868	1870	1871	rBV	171	146	0.02%	0.003%
85	12.719	1907	1908	1911	rBV	163	182	0.02%	0.003%
86	12.768	1913	1916	1920	rVV3	271	380	0.05%	0.007%
87	12.847	1927	1929	1931	rBV3	140	146	0.02%	0.003%
88	13.030	1955	1959	1960	rBV	120	156	0.02%	0.003%
89	13.116	1970	1973	1977	rBV2	818	991	0.13%	0.018%
90	13.183	1982	1984	1987	rVB	141	134	0.02%	0.002%
91	13.396	2017	2019	2022	rVB	145	131	0.02%	0.002%
92	13.591	2048	2051	2054	rBV2	1259	1498	0.20%	0.027%
93	13.780	2078	2082	2087	rBV	1870	2553	0.33%	0.047%
94	13.920	2102	2105	2106	rBV2	180	200	0.03%	0.004%
95	13.963	2108	2112	2119	rVV2	1847	2152	0.28%	0.039%
96	14.219	2152	2154	2158	rVB2	300	268	0.04%	0.005%
97	14.365	2176	2178	2182	rBV	189	196	0.03%	0.004%
98	14.804	2248	2250	2251	rBV	296	229	0.03%	0.004%
99	15.133	2302	2304	2307	rBV2	192	195	0.03%	0.004%
100	16.706	2560	2562	2564	rBV2	224	187	0.02%	0.003%

Sum of corrected areas: 5464650




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122322\
Data File : VX033554.D
Acq On : 23 Dec 2022 10:52
Operator : JC/MD
Sample : VX1223MBL01
Misc : 5.00g/5.0mL/100ul/5.0mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK605

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

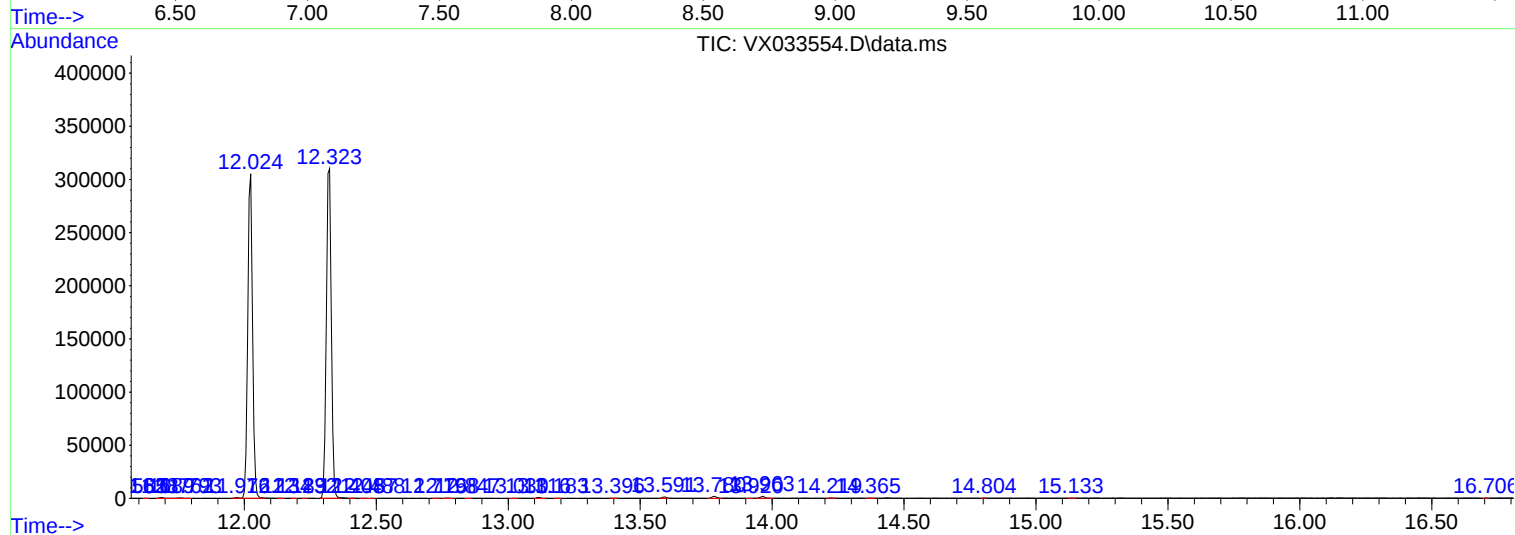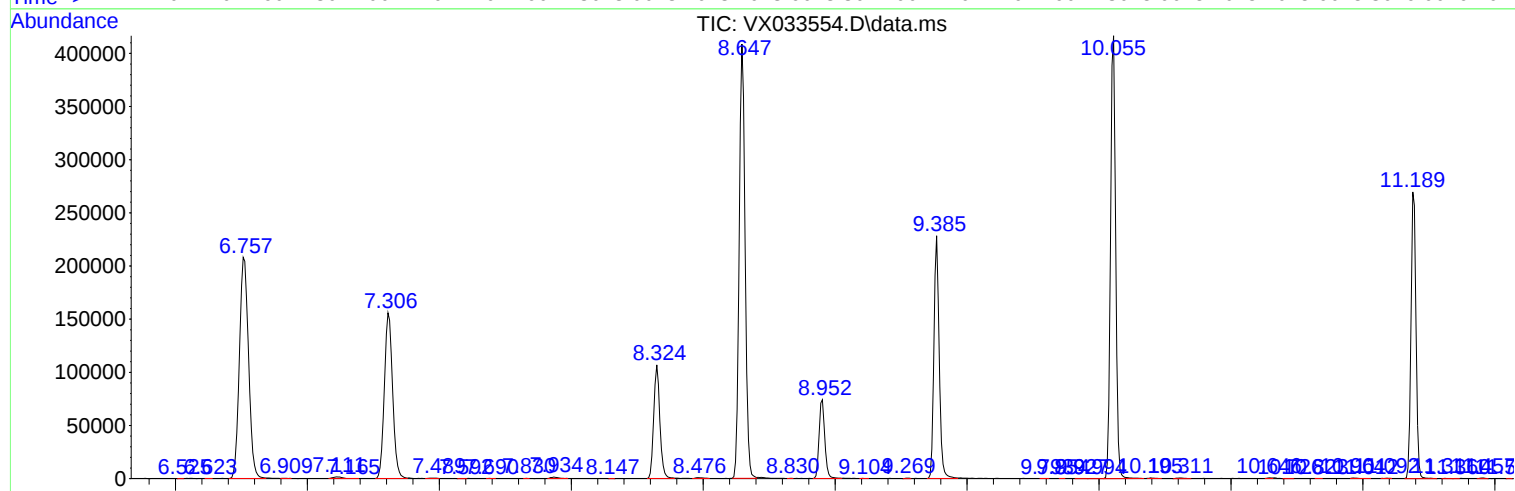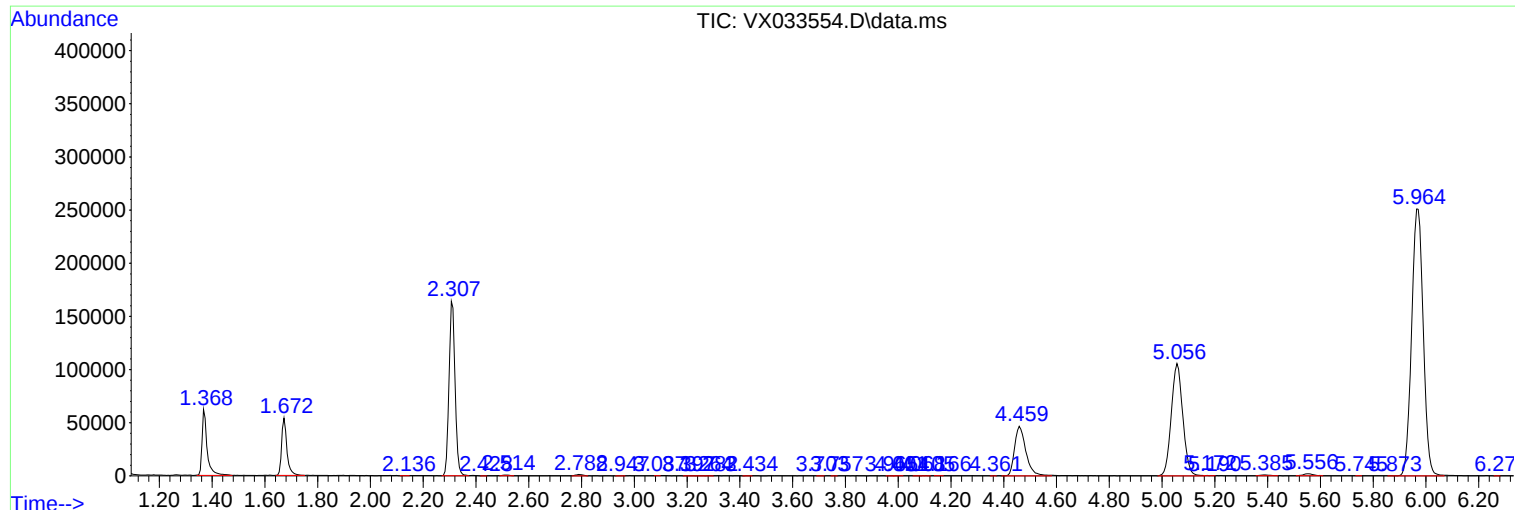

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122322\
Data File : VX033554.D
Acq On : 23 Dec 2022 10:52
Operator : JC/MD
Sample : VX1223MBL01
Misc : 5.00g/5.0mL/100ul/5.0mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK605

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122322\
Data File : VX033554.D
Acq On : 23 Dec 2022 10:52
Operator : JC/MD
Sample : VX1223MBL01
Misc : 5.00g/5.0mL/100ul/5.0mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK605

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc