
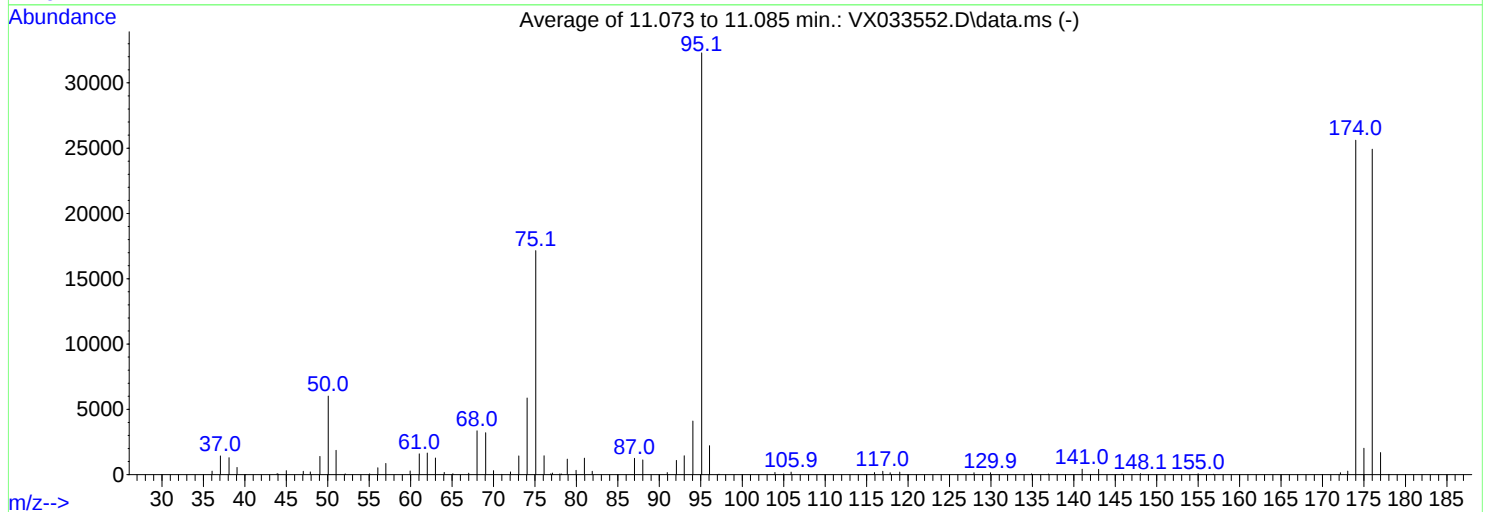


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122322\
 Data File : VX033552.D
 Acq On : 23 Dec 2022 09:55
 Operator : JC/MD
 Sample : BFB602
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB602

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM12222WMA.M
 Title : VOC Analysis
 Last Update : Sat Dec 24 00:26:44 2022

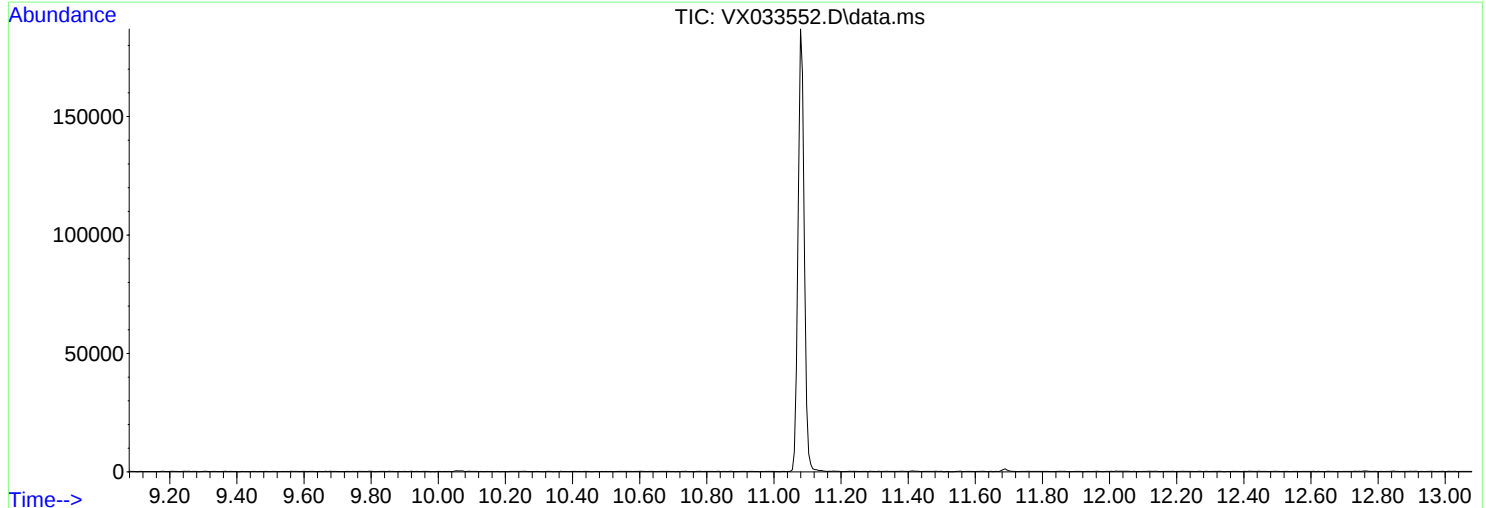

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	6023	PASS
75	95	30	80	53.1	17154	PASS
95	95	100	100	100.0	32299	PASS
96	95	5	9	6.9	2217	PASS
173	174	0.00	2	1.1	272	PASS
174	95	50	120	79.3	25603	PASS
175	174	5	9	7.9	2016	PASS
176	174	95	101	97.4	24925	PASS
177	176	5	9	6.8	1692	PASS

Scan 1633 (11.043 min): VX033552.D\data.ms
BFB602

m/z	Abundance
40.00	116.0
44.10	107.0

Instrument :
MSVOA_X
ClientSampleId :
BFB602

m/z	Abundance
36.10	238.0
37.10	1480.0
38.10	1139.0
39.10	463.0
40.10	119.0
43.90	251.0
45.00	202.0
47.20	150.0
47.90	240.0
49.00	1247.0
50.00	5183.0
51.00	1632.0
52.10	87.0
55.00	68.0
56.00	451.0
57.00	713.0
59.90	231.0
61.10	1327.0
62.00	1317.0
63.00	1147.0
64.00	160.0
65.20	73.0
67.00	146.0
68.00	2962.0
69.00	2465.0
70.00	273.0
72.00	182.0
73.10	1168.0
74.00	4573.0
75.10	14079.0
76.10	1360.0
76.90	175.0
78.00	66.0
78.90	963.0
80.00	314.0
80.90	1045.0
81.90	227.0
87.00	1025.0
88.00	992.0
91.00	144.0
92.00	813.0
93.00	1168.0
94.10	3197.0
95.10	24848.0
96.00	1999.0
97.30	54.0
104.00	134.0
105.80	94.0
116.00	116.0
116.90	264.0
117.90	132.0
118.90	182.0
128.00	135.0
129.90	129.0
141.00	316.0
143.00	240.0
145.10	50.0
155.20	59.0
173.00	224.0
174.00	16480.0
175.00	1327.0
176.00	16006.0
177.00	1155.0

Instrument :
MSVOA_X
ClientSampleId :
BFB602

m/z	Abundance
36.10	318.0
37.00	1497.0
38.10	1634.0
39.00	670.0
40.00	124.0
44.10	233.0
45.00	425.0
47.00	367.0
47.90	191.0
49.10	1599.0
50.10	7085.0
51.00	2218.0
52.10	98.0
55.10	107.0
56.00	661.0
57.00	1023.0
60.00	297.0
61.00	1975.0
62.00	1945.0
63.00	1510.0
64.00	171.0
65.10	99.0
67.00	100.0
68.00	3932.0
69.00	3878.0
70.00	377.0
72.00	237.0
73.10	1651.0
74.10	7046.0
75.10	20928.0
76.10	1612.0
77.10	157.0
78.20	146.0
78.90	1316.0
79.90	342.0
80.90	1502.0
81.90	274.0
87.00	1470.0
88.00	1100.0
90.90	160.0
92.10	1236.0
93.00	1712.0
94.10	4909.0
95.10	38736.0
96.10	2473.0
97.10	55.0
103.90	209.0
105.00	90.0
105.90	204.0
115.90	191.0
116.90	300.0
117.80	148.0
119.00	236.0
127.90	140.0
130.00	195.0
134.90	85.0
136.90	76.0
141.00	479.0
142.00	59.0
143.00	453.0
145.80	70.0
148.00	106.0
155.00	101.0
156.90	59.0
172.20	176.0
173.00	286.0
174.00	30152.0
175.00	2410.0
176.00	29176.0
177.00	1907.0
178.00	62.0

Instrument :
MSVOA_X
ClientSampleId :
BFB602

m/z	Abundance
36.00	255.0
37.00	1330.0
38.10	1114.0
39.00	517.0
40.00	112.0
44.00	194.0
45.00	300.0
47.00	271.0
47.90	204.0
49.00	1333.0
50.00	5800.0
51.00	1726.0
56.10	474.0
57.00	843.0
60.00	333.0
61.00	1493.0
62.00	1697.0
63.00	1157.0
64.10	166.0
65.00	59.0
67.00	82.0
68.00	3190.0
69.10	3283.0
70.00	278.0
71.00	76.0
72.10	216.0
73.00	1471.0
74.00	5990.0
75.10	16456.0
76.10	1353.0
77.10	202.0
78.00	107.0
78.90	1287.0
79.90	332.0
81.00	1256.0
81.90	283.0
87.00	1250.0
88.00	1283.0
90.90	179.0
92.00	1238.0
93.00	1447.0
94.00	4195.0
95.10	33312.0
96.10	2179.0
104.00	172.0
105.00	81.0
106.00	281.0
114.80	53.0
115.90	177.0
117.00	222.0
117.80	173.0
119.10	190.0
127.90	172.0
129.90	132.0
134.90	85.0
137.00	70.0
141.00	459.0
143.00	526.0
145.80	87.0
148.10	102.0
154.90	62.0
156.80	59.0
172.10	264.0
173.10	305.0
174.00	30176.0
175.00	2312.0
176.00	29592.0
177.00	2013.0

Instrument :
MSVOA_X
ClientSampleId :
BFB602