

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX122418\
 Data File : VX006803.D
 Acq On : 24 Dec 2018 18:51
 Operator : JC/MD
 Sample : J6533-13
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMP-3


Quant Time: Dec 25 01:25:30 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X121818W.M
 Quant Title : SW846 8260
 QLast Update : Wed Dec 19 15:20:58 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	716327	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	1049862	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	963902	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	494175	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.07	65	357797	46.35	ug/l	0.00
Spiked Amount			Recovery	=	92.70%	
35) Dibromofluoromethane	5.50	113	308026	46.40	ug/l	0.00
Spiked Amount			Recovery	=	92.80%	
50) Toluene-d8	8.71	98	1244133	49.71	ug/l	0.00
Spiked Amount			Recovery	=	99.42%	
62) 4-Bromofluorobenzene	11.13	95	451750	49.28	ug/l	0.00
Spiked Amount			Recovery	=	98.56%	

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
5) Bromomethane	1.60	94	551	Below Cal	#	66
11) Tert butyl alcohol	3.07	59	3295611	1912.771	ug/l	99
13) Acrolein	2.30	56	2519	2.167	ug/l #	51
14) Allyl chloride	2.71	41	2841	0.264	ug/l #	49
15) Acrylonitrile	3.07	53	29849	7.803	ug/l #	23
16) Acetone	2.45	43	540577	152.407	ug/l	100
18) Methyl Acetate	2.78	43	31239	2.995	ug/l	95
20) Methylene Chloride	2.86	84	2941	0.401	ug/l #	87
25) 2-Butanone	4.70	43	244147	48.935	ug/l	95
28) Bromochloromethane	5.02	49	230	Below Cal	#	52
36) 1,1-Dichloropropene	5.66	75	45873	5.276	ug/l #	48
37) Ethyl Acetate	4.70	43	244147	26.977	ug/l #	66
38) Carbon Tetrachloride	5.67	117	62317	7.374	ug/l #	14
40) Benzene	6.14	78	33958	1.285	ug/l	96
48) Methyl methacrylate	7.77	41	48798	6.969	ug/l	98
49) 1,4-Dioxane	7.75	88	3089	Below Cal	#	47
51) 4-Methyl-2-Pentanone	8.65	43	8845	1.010	ug/l	96
52) Toluene	8.79	92	28516	1.670	ug/l	99
60) Dibromochloromethane	9.65	129	180	2.348	ug/l	81
67) Ethyl Benzene	10.25	91	9142	0.274	ug/l	98
68) m/p-Xylenes	10.35	106	16846	1.281	ug/l	100
69) o-Xylene	10.69	106	6662	0.513	ug/l	99
70) Styrene	10.71	104	50536	2.460	ug/l	92
76) 1,2,3-Trichloropropane	11.13	75	213969	23.298	ug/l #	40
81) trans-1,4-Dichloro-2-buten	11.13	75	213969	69.134	ug/l #	10
90) Hexachloroethane	12.55	117	435	3.380	ug/l #	6
95) Naphthalene	13.83	128	46835	1.291	ug/l	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 740

Delta R.T. 0.01 min

Lab File: VX006803.D

Acq: 24 Dec 2018 18:51

Instrument :

MSVOA_X

ClientSampleId :


COMP-3

Tot Ion:168 Resp: 716327

Ion Ratio Lower Upper

168 100

99 46.6 41.8 62.8



Abundance Ion 167.90 (167.60 to 168.60): VX006591.D (-725) (-)

Ion 98.90 (98.60 to 99.60): VX006591.D (-725) (-)

5.67

250000

200000



150000

100000

50000

0

Time-->



#5

Bromomethane

Concen: Below Cal

RT: 1.60 min Scan# 73

Delta R.T. -0.04 min

Lab File: VX006803.D


Acq: 24 Dec 2018 18:51

Tgt Ion: 94 Resp: 551

Ion Ratio Lower Upper

94 100

96 59.4 73.4 110.2#



Abundance Ion 93.90 (93.60 to 94.60): VX006591.D (-69) (-)

Ion 95.90 (95.60 to 96.60): VX006591.D (-69) (-)

1.60

500

400


300


200

100

0

Time-->









#11

Tert butyl alcohol
 Concen: 1912.771 ug/l
 RT: 3.07 min Scan# 314
 Delta R.T. -0.01 min
 Lab File: VX006803.D
 Acq: 24 Dec 2018 18:51

Instrument :
 MSVOA_X
 ClientSampleId :
 COMP-3




Tot Ion: 59 Resp: 3295611
 Ion Ratio Lower Upper
 59 100
 57 10.2 8.5 12.7

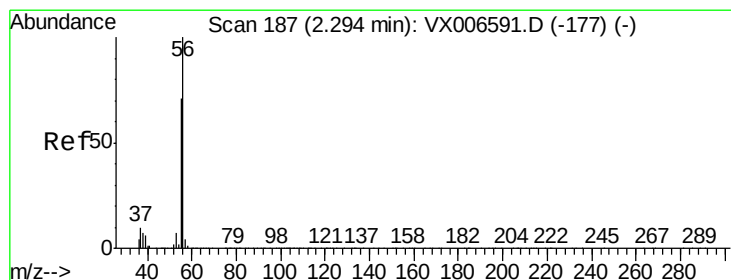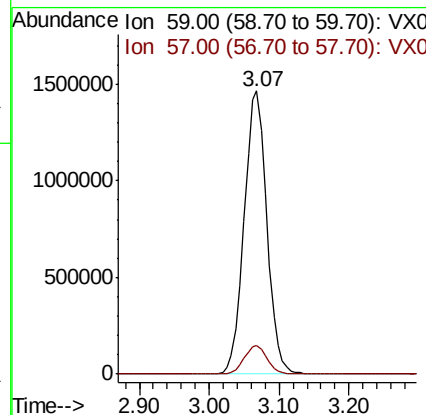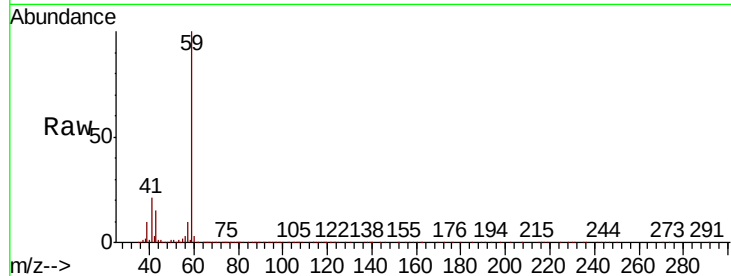


#13

Acrolein
 Concen: 2.167 ug/l
 RT: 2.30 min Scan# 188
 Delta R.T. 0.01 min
 Lab File: VX006803.D
 Acq: 24 Dec 2018 18:51

Tgt Ion: 56 Resp: 2519
 Ion Ratio Lower Upper
 56 100
 55 32.0 58.2 87.4#

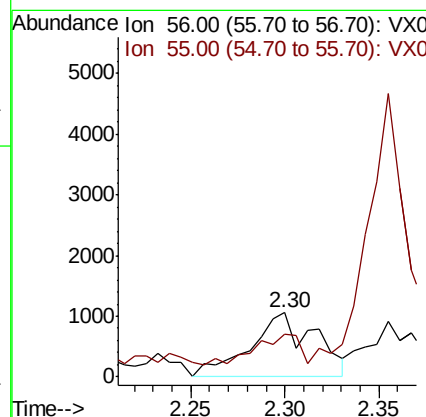



#14

Allvl chloride

Concen: 0.264 ug/l

RT: 2.71 min Scan# 256

Delta R.T. -0.01 min

Lab File: VX006803.D

Acq: 24 Dec 2018 18:51

Instrument :

MSVOA_X

ClientSampleId :

COMP-3


Tot Ion: 41 Resp: 2841

Ion Ratio Lower Upper

41 100

39 24.2 53.6 80.4#




76 7.5 27.4 41.2#

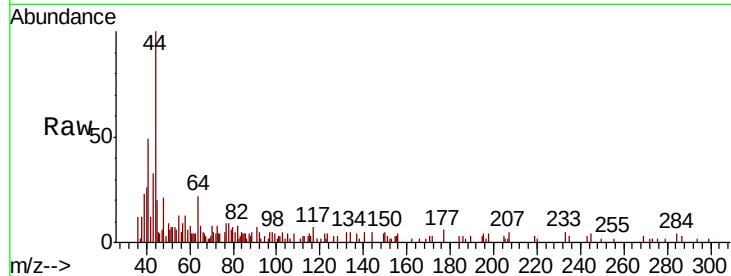

Abundance Ion 41.00 (40.70 to 41.70): VX0

Ion 39.00 (38.70 to 39.70): VX0

Ion 75.90 (75.60 to 76.60): VX0

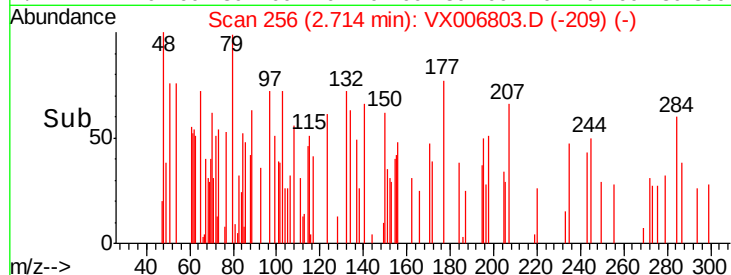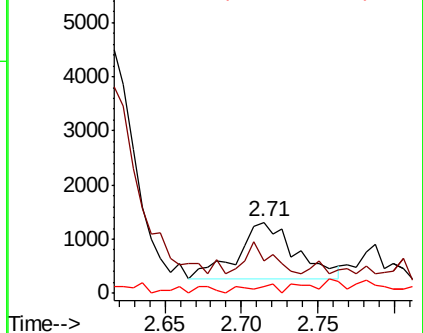

#15

Acrylonitrile

Concen: 7.803 ug/l

RT: 3.07 min Scan# 314

Delta R.T. -0.08 min

Lab File: VX006803.D

Acq: 24 Dec 2018 18:51


Tgt Ion: 53 Resp: 29849

Ion Ratio Lower Upper

53 100

52 24.5 66.0 99.0#



51 98.2 28.6 42.8#

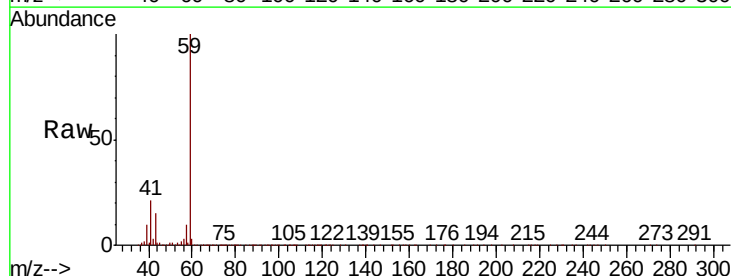


Abundance Ion 53.00 (52.70 to 53.70): VX0

Ion 52.00 (51.70 to 52.70): VX0

Ion 51.00 (50.70 to 51.70): VX0




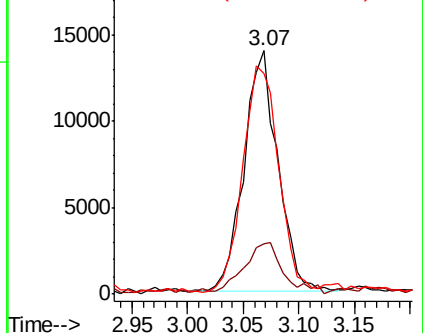




#16
Acetone
Concen: 152.407 ug/l
RT: 2.45 min Scan# 212
Delta R.T. -0.00 min
Lab File: VX006803.D
Acq: 24 Dec 2018 18:51




Instrument :
MSVOA_X
ClientSampleId :
COMP-3


Tot Ion: 43 Resp: 540577
Ion Ratio Lower Upper
43 100
58 31.5 25.0 37.6

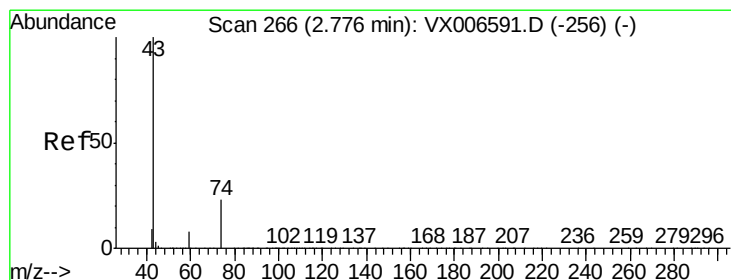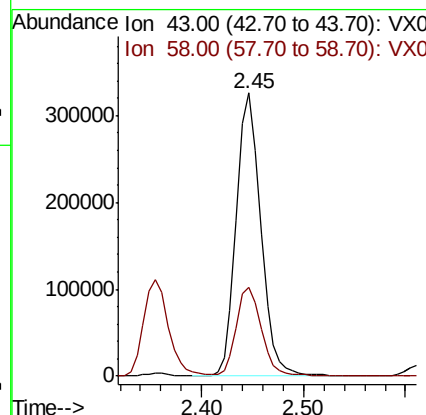

#18
Methyl Acetate
Concen: 2.995 ug/l
RT: 2.78 min Scan# 267
Delta R.T. 0.01 min
Lab File: VX006803.D
Acq: 24 Dec 2018 18:51

Tgt Ion: 43 Resp: 31239
Ion Ratio Lower Upper
43 100
74 25.6 18.6 28.0



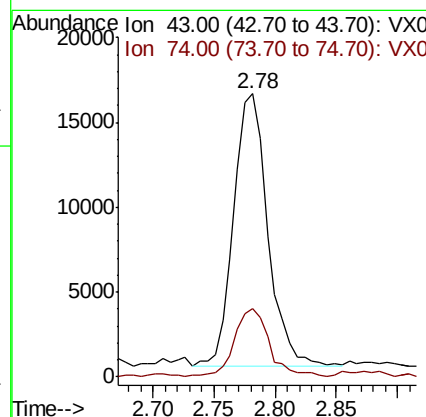
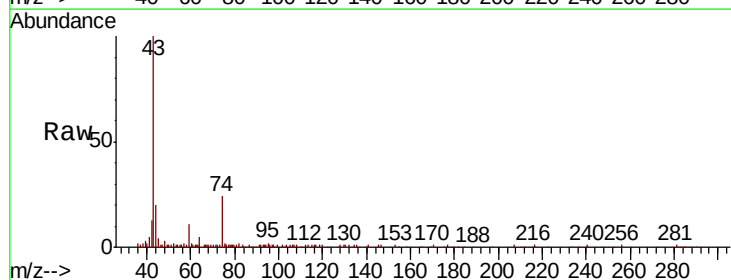




#20
Methylene Chloride
Concen: 0.401 ug/l
RT: 2.86 min Scan# 280
Delta R.T. -0.00 min
Lab File: VX006803.D
Acq: 24 Dec 2018 18:51




Instrument :
MSVOA_X
ClientSampleId :
COMP-3


Tot Ion: 84 Resp: 2941
Ion Ratio Lower Upper
84 100
49 106.5 91.8 137.6
51 20.7 28.5 42.7#
86 50.9 50.2 75.2

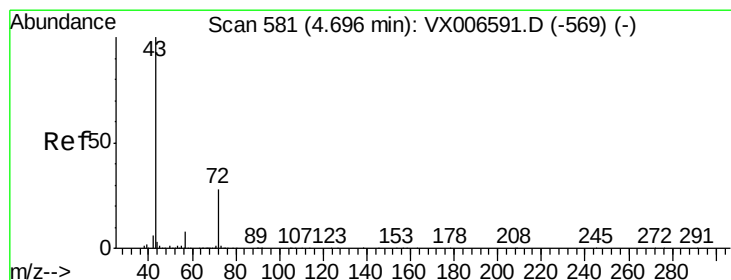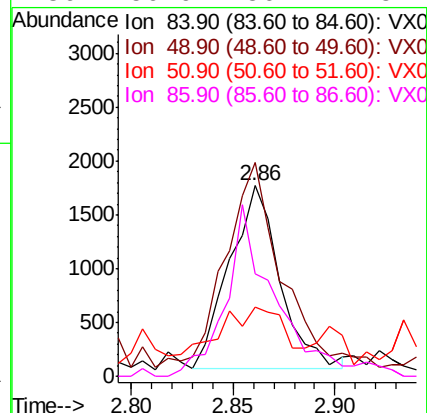

#25
2-Butanone
Concen: 48.935 ug/l
RT: 4.70 min Scan# 581
Delta R.T. -0.00 min
Lab File: VX006803.D
Acq: 24 Dec 2018 18:51

Tgt Ion: 43 Resp: 244147
Ion Ratio Lower Upper
43 100
72 25.3 22.4 33.6

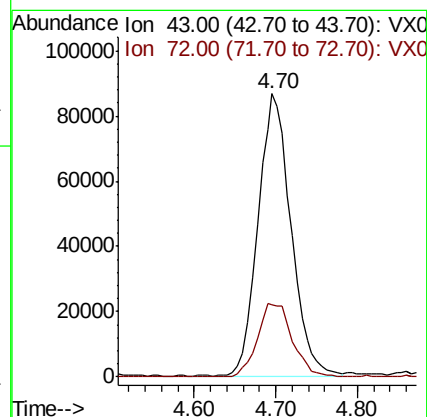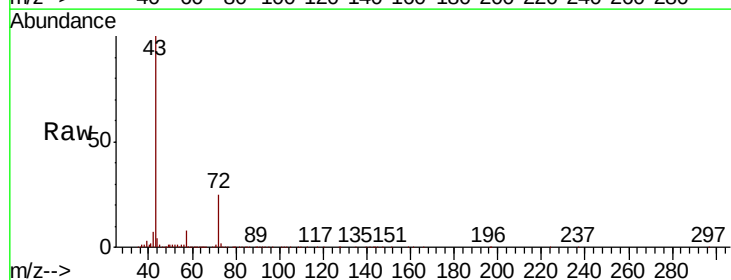

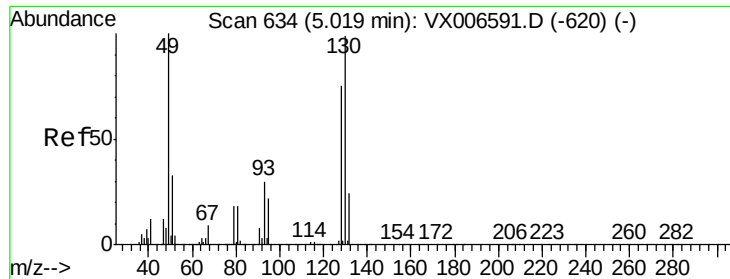

#28

Bromochloromethane

Concen: Below Cal

RT: 5.02 min Scan# 634

Delta R.T. -0.00 min

Lab File: VX006803.D

Acq: 24 Dec 2018 18:51

Instrument :

MSVOA_X

ClientSampleId :

COMP-3


Tot Ion: 49 Resp: 230

Ion Ratio Lower Upper

49 100

129 0.0 0.0 5.4




130 49.1 77.7 116.5#

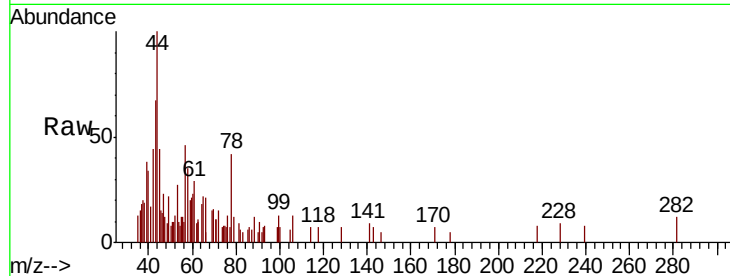

Abundance Ion 48.90 (48.60 to 49.60): VX0

Ion 128.80 (128.50 to 129.50): V

Ion 129.80 (129.50 to 130.50): V

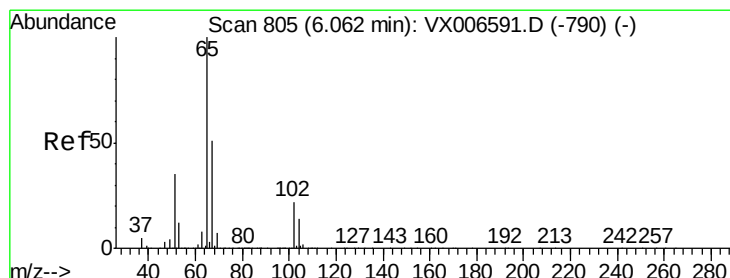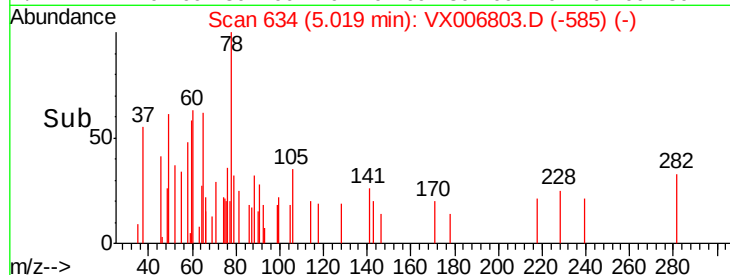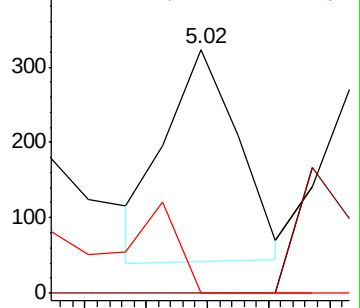

#33

1,2-Dichloroethane-d4

Concen: 46.345 ug/l

RT: 6.07 min Scan# 806

Delta R.T. 0.01 min

Lab File: VX006803.D


Acq: 24 Dec 2018 18:51

Tgt Ion: 65 Resp: 357797

Ion Ratio Lower Upper



65 100


67 53.5 0.0 105.0

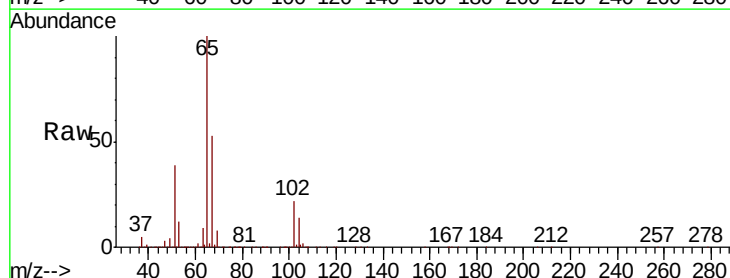

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

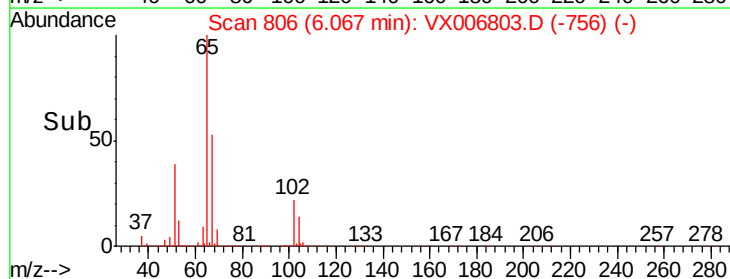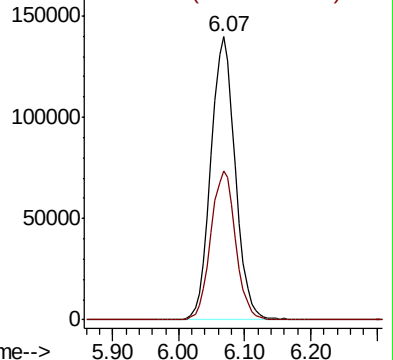







#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.86 min Scan# 936
 Delta R.T. -0.00 min
 Lab File: VX006803.D
 Acq: 24 Dec 2018 18:51

Instrument :
 MSVOA_X
 ClientSampleId :
 COMP-3

Tot Ion:114 Resp: 1049862




Ion	Ratio	Lower	Upper
114	100		
63	17.8	0.0	34.8
88	15.2	0.0	28.8

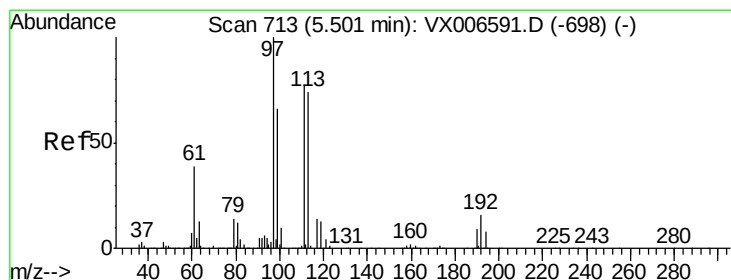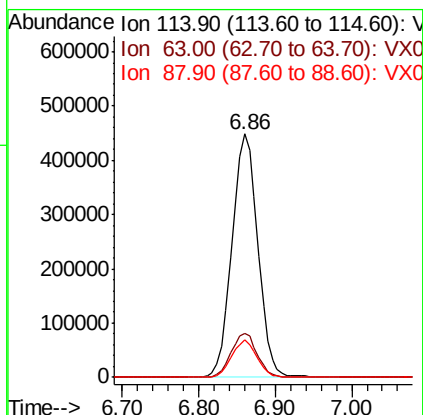


#35
 Dibromofluoromethane
 Concen: 46.396 ug/l
 RT: 5.50 min Scan# 713
 Delta R.T. -0.00 min
 Lab File: VX006803.D
 Acq: 24 Dec 2018 18:51

Tgt Ion:113 Resp: 308026

Ion	Ratio	Lower	Upper
113	100		
111	102.7	81.6	122.4
192	22.3	16.7	25.1

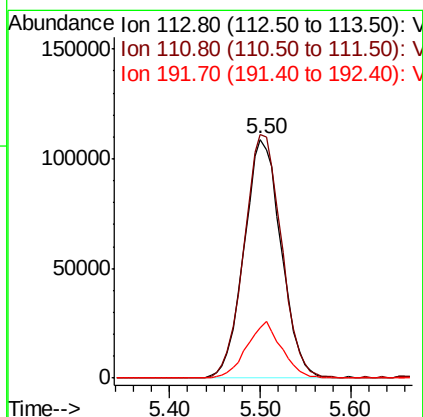



#36

1,1-Dichloropropene

Concen: 5.276 ug/l

RT: 5.66 min Scan# 739

Delta R.T. -0.14 min

Lab File: VX006803.D

Acq: 24 Dec 2018 18:51

Instrument :

MSVOA_X

ClientSampleId :

COMP-3


Tot Ion: 75 Resp: 45873

Ion Ratio Lower Upper

75 100

110 9.8 20.2 60.5#




77 0.5 24.8 37.2#

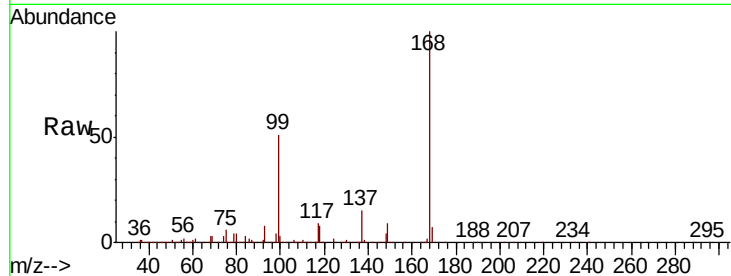

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 109.90 (109.60 to 110.60): VX0

Ion 76.90 (76.60 to 77.60): VX0

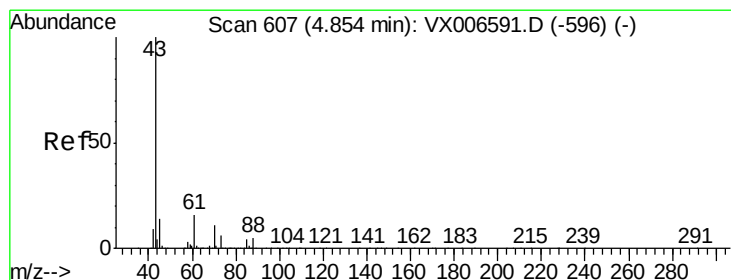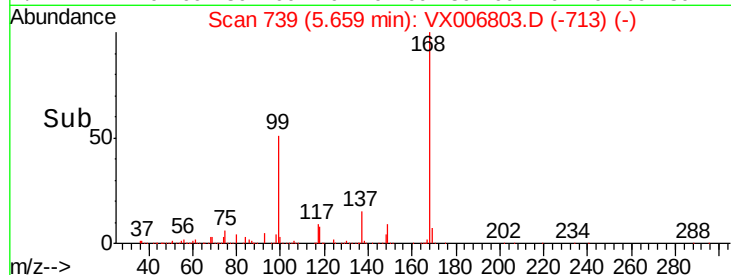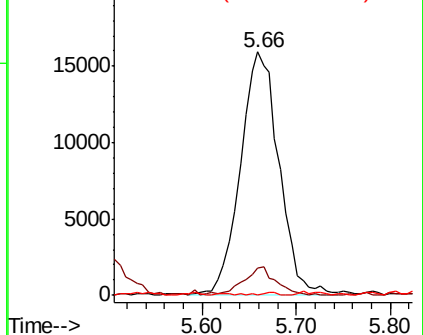

#37

Ethyl Acetate

Concen: 26.977 ug/l

RT: 4.70 min Scan# 581

Delta R.T. -0.16 min

Lab File: VX006803.D

Acq: 24 Dec 2018 18:51


Tgt Ion: 43 Resp: 244147

Ion Ratio Lower Upper

43 100

61 0.0 11.9 17.9#



70 0.1 9.7 14.5#




Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 60.90 (60.60 to 61.60): VX0

Ion 70.00 (69.70 to 70.70): VX0

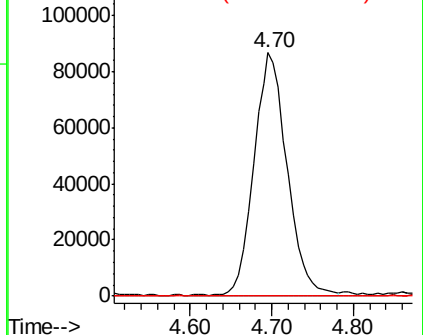



#38

Carbon Tetrachloride

Concen: 7.374 ug/l

RT: 5.67 min Scan# 740

Delta R.T. -0.12 min

Lab File: VX006803.D

Acq: 24 Dec 2018 18:51

Instrument :

MSVOA_X

ClientSampleId :

COMP-3


Tot Ion:117 Resp: 62317

Ion Ratio Lower Upper

117 100

119 4.7 79.4 119.2#




121 0.0 24.0 36.0#

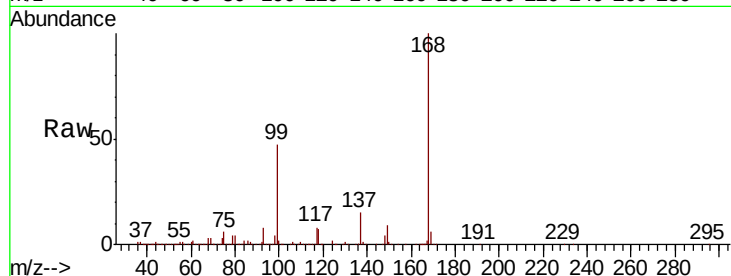

Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

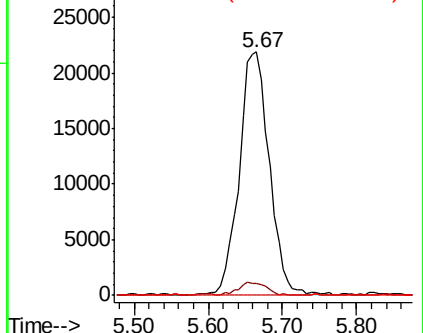

#40

Benzene

Concen: 1.285 ug/l

RT: 6.14 min Scan# 818

Delta R.T. -0.00 min

Lab File: VX006803.D


Acq: 24 Dec 2018 18:51

Tgt Ion: 78 Resp: 33958

Ion Ratio Lower Upper



78 100


77 21.9 19.2 28.8



Abundance Ion 78.00 (77.70 to 78.70): VX0

Ion 77.00 (76.70 to 77.70): VX0




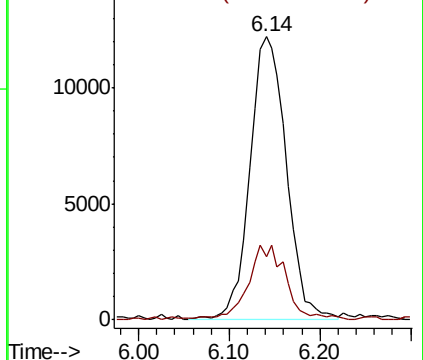


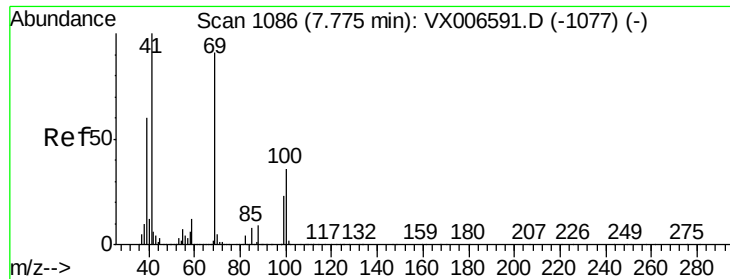

#48
Methvl methacrylate
Concen: 6.969 ug/l
RT: 7.77 min Scan# 1086
Delta R.T. -0.00 min
Lab File: VX006803.D
Acq: 24 Dec 2018 18:51




Instrument :
MSVOA_X
ClientSampleId :
COMP-3


Tot Ion	Ratio	Lower	Upper
41	100		
69	89.6	72.4	108.6
39	59.5	45.8	68.8

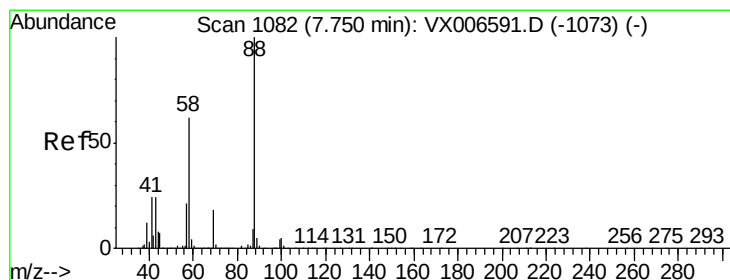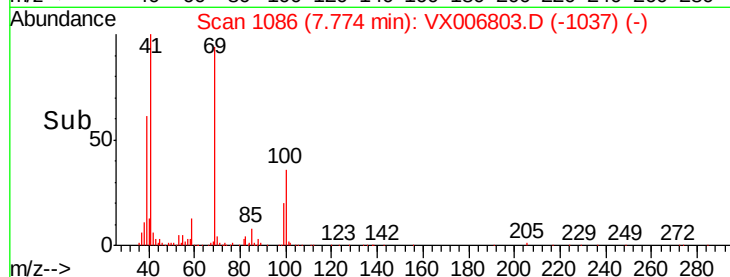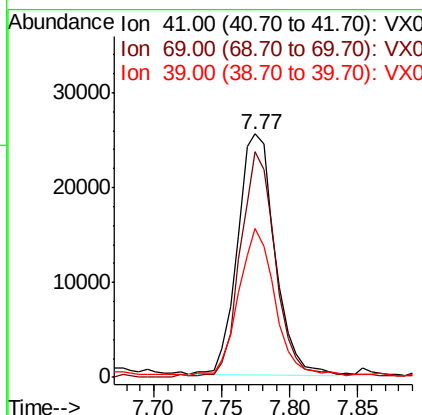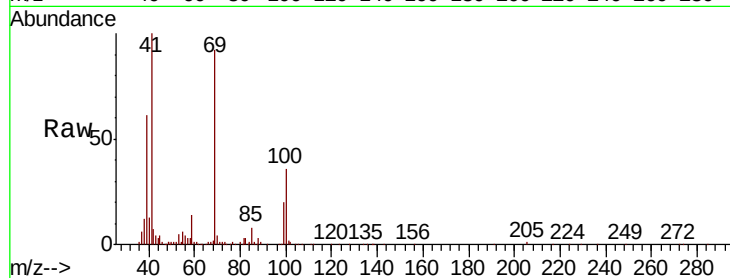

#49
1,4-Dioxane
Concen: Below Cal
RT: 7.75 min Scan# 1082
Delta R.T. 0.00 min
Lab File: VX006803.D
Acq: 24 Dec 2018 18:51

Tgt Ion	Ratio	Lower	Upper
88	100		
43	70.3	22.2	33.4#
58	95.2	51.0	76.4#

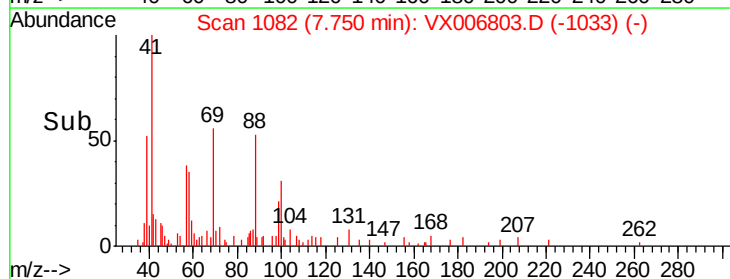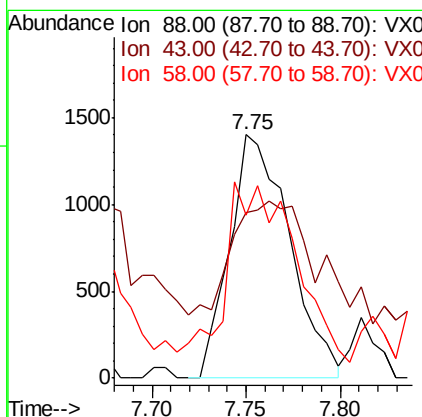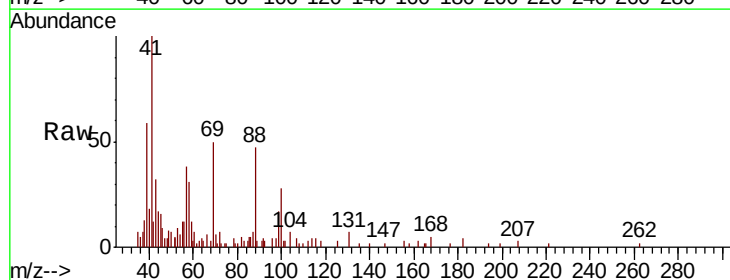



#50

Toluene-d8

Concen: 49.706 ug/l

RT: 8.71 min Scan# 1240

Delta R.T. -0.00 min

Lab File: VX006803.D

Acq: 24 Dec 2018 18:51

Instrument :

MSVOA_X

ClientSampleId :





COMP-3

Tot Ion: 98 Resp: 1244133

Ion Ratio Lower Upper

98 100

100 64.2 52.0 78.0

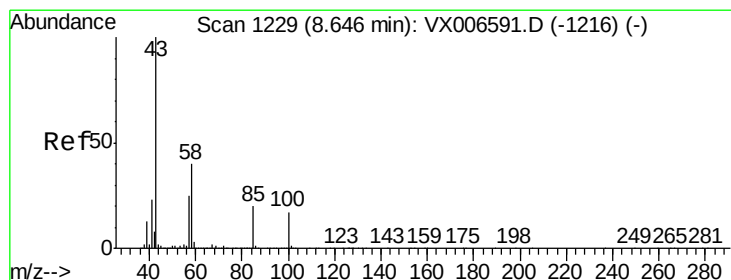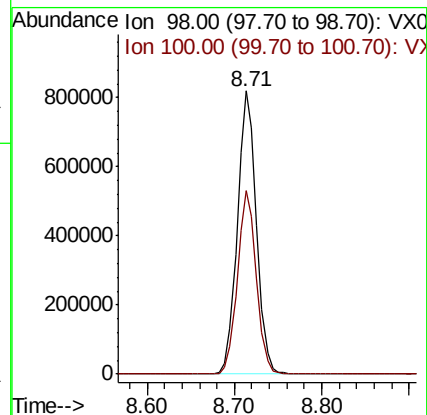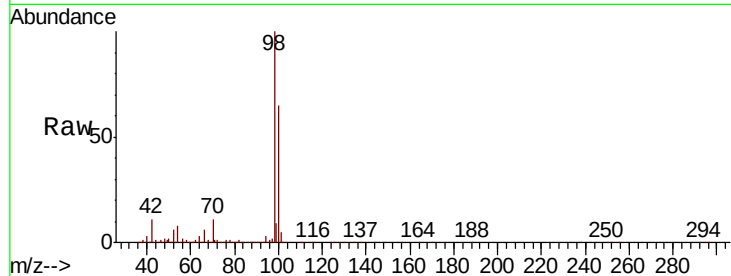

#51

4-Methyl-2-Pentanone

Concen: 1.010 ug/l

RT: 8.65 min Scan# 1230

Delta R.T. 0.01 min

Lab File: VX006803.D




Acq: 24 Dec 2018 18:51


Tgt Ion: 43 Resp: 8845

Ion Ratio Lower Upper

43 100

58 37.2 31.8 47.6

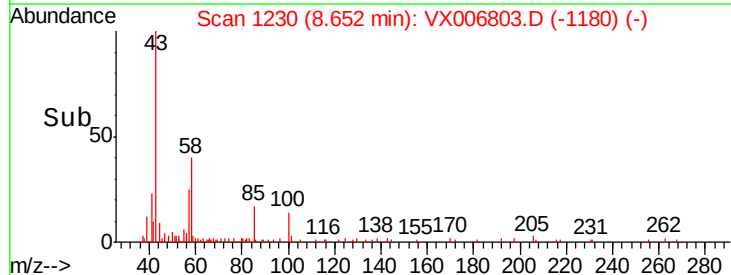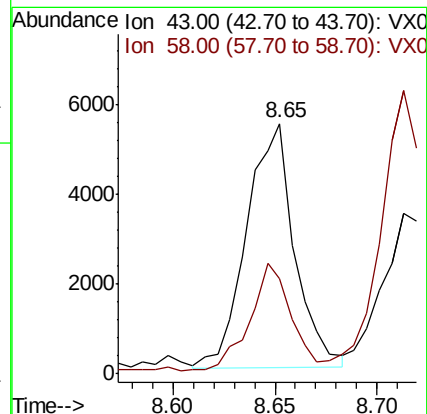



#52

Toluene

Concen: 1.670 ug/l

RT: 8.79 min Scan# 1252

Delta R.T. -0.00 min

Lab File: VX006803.D

Acq: 24 Dec 2018 18:51

Instrument :

MSVOA_X

ClientSampled :





COMP-3

Tot Ion: 92 Resp: 28516

Ion Ratio Lower Upper

92 100

91 172.9 137.6 206.4

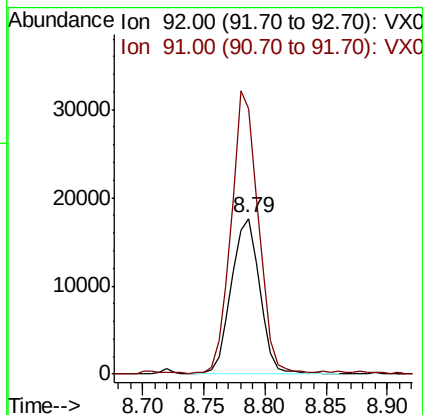

#60

Dibromochloromethane

Concen: 2.348 ug/l

RT: 9.65 min Scan# 1393

Delta R.T. 0.07 min

Lab File: VX006803.D




Acq: 24 Dec 2018 18:51


Tgt Ion: 129 Resp: 180

Ion Ratio Lower Upper

129 100

127 61.7 39.3 117.8



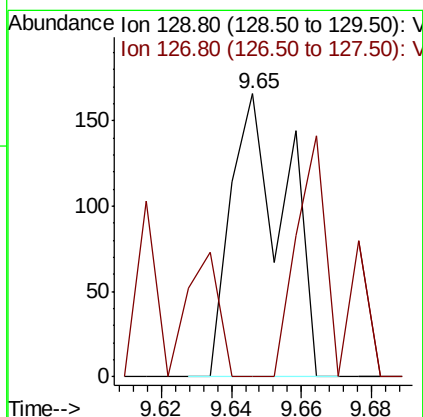



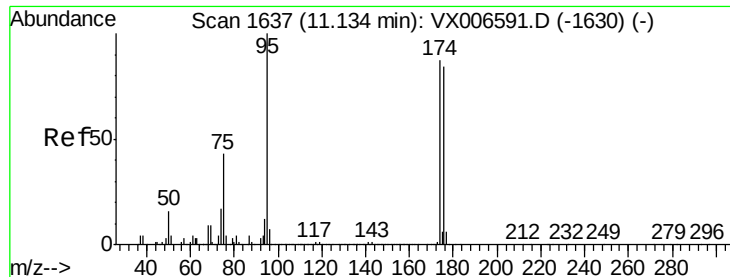

#62
4-Bromofluorobenzene
Concen: 49.280 ug/l
RT: 11.13 min Scan# 1637
Delta R.T. -0.00 min
Lab File: VX006803.D
Acq: 24 Dec 2018 18:51




Instrument :
MSVOA_X
ClientSampleId :
COMP-3


Tot Ion	Ratio	Lower	Upper
95	100		
174	93.4	0.0	182.2
176	91.6	0.0	178.8

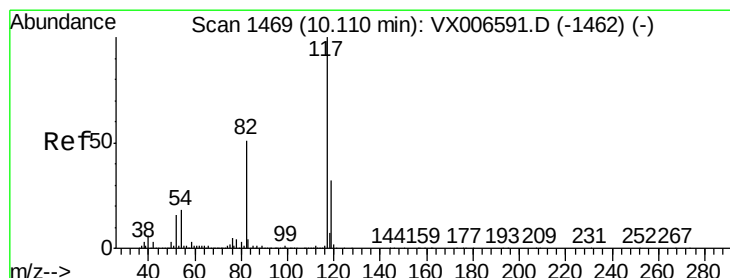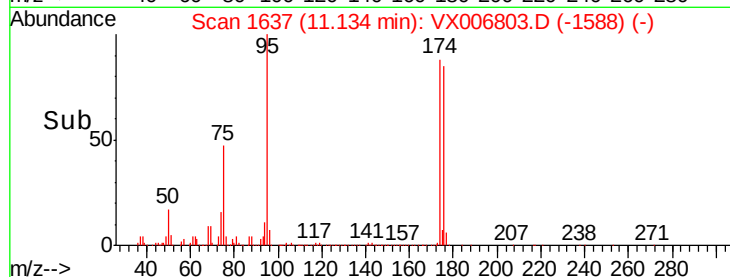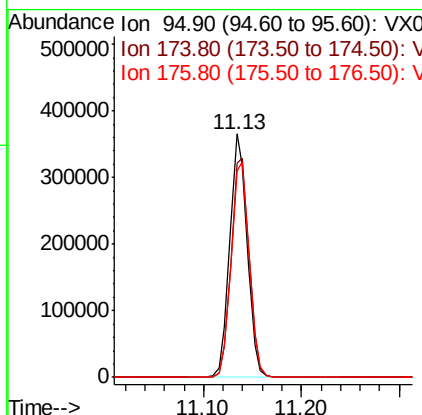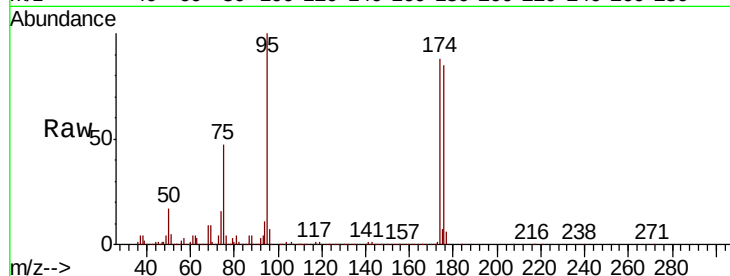

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.11 min Scan# 1469
Delta R.T. -0.00 min
Lab File: VX006803.D
Acq: 24 Dec 2018 18:51

Tgt Ion	Ratio	Lower	Upper
117	100		
82	51.6	41.0	61.6
119	32.5	25.4	38.0

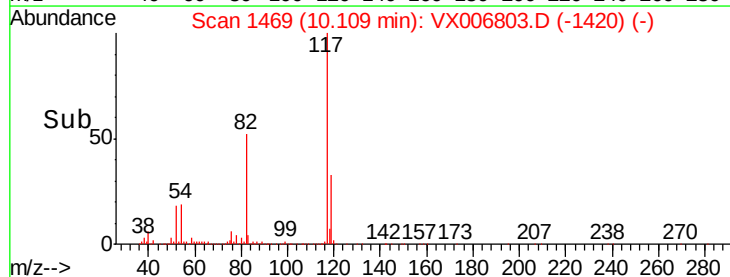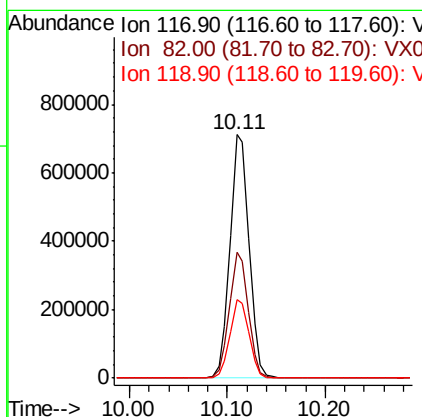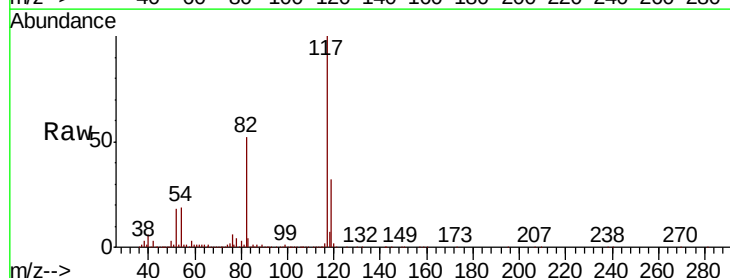

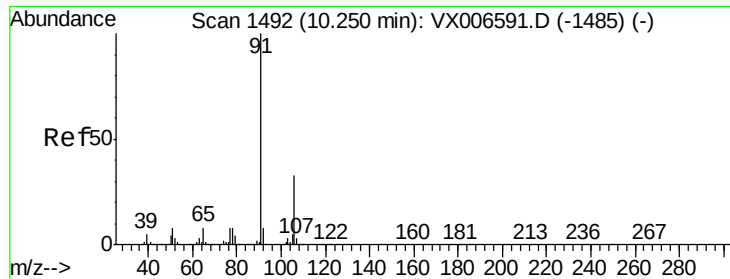

#67

Ethyl Benzene

Concen: 0.274 ug/l

RT: 10.25 min Scan# 1492

Delta R.T. -0.00 min

Lab File: VX006803.D

Acq: 24 Dec 2018 18:51

Instrument :

MSVOA_X

ClientSampleId :


COMP-3

Tot Ion: 91 Resp: 9142




Ion Ratio Lower Upper

91 100

106 31.9 26.4 39.6

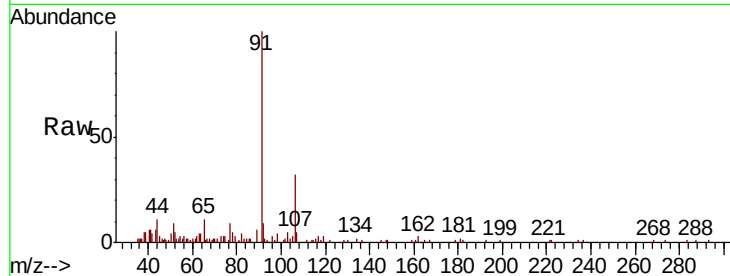

Abundance Ion 91.00 (90.70 to 91.70): VX006591.D (-1485) (-)

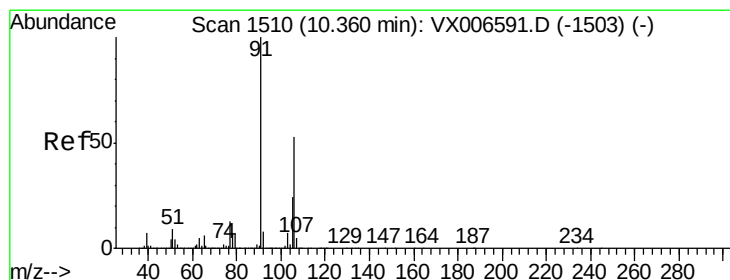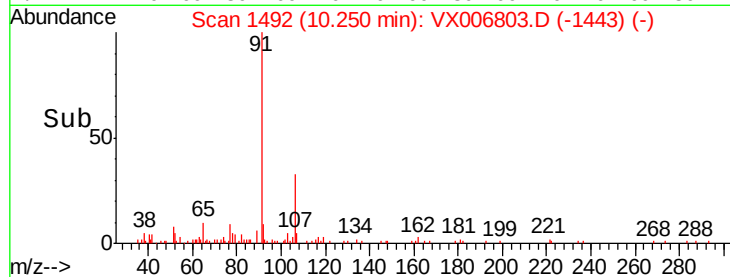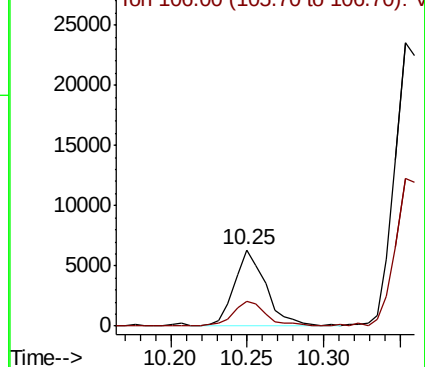

#68

m/p-Xylenes

Concen: 1.281 ug/l

RT: 10.35 min Scan# 1509

Delta R.T. -0.01 min

Lab File: VX006803.D


Acq: 24 Dec 2018 18:51

Tgt Ion: 106 Resp: 16846



Ion Ratio Lower Upper


106 100

91 195.4 155.8 233.6

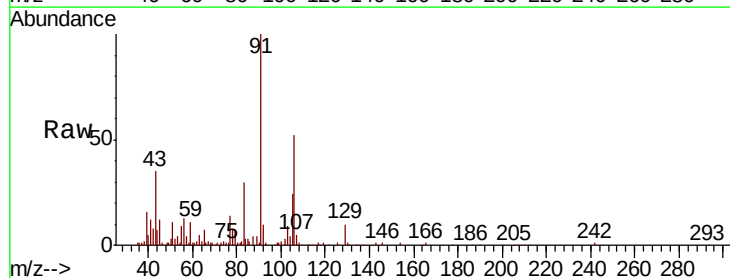

Abundance Ion 106.00 (105.70 to 106.70): VX006591.D (-1503) (-)



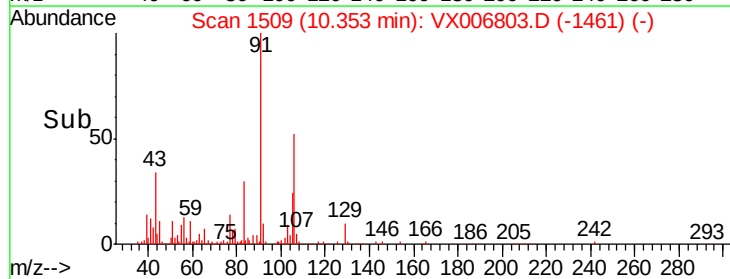
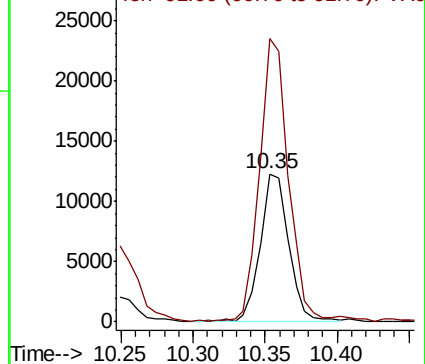




#69
o-Xylene
Concen: 0.513 ug/l
RT: 10.69 min Scan# 1565
Delta R.T. -0.01 min
Lab File: VX006803.D
Acq: 24 Dec 2018 18:51




Instrument :
MSVOA_X
ClientSampled :
COMP-3


Tot Ion:106 Resp: 6662
Ion Ratio Lower Upper
106 100
91 201.6 101.3 303.7

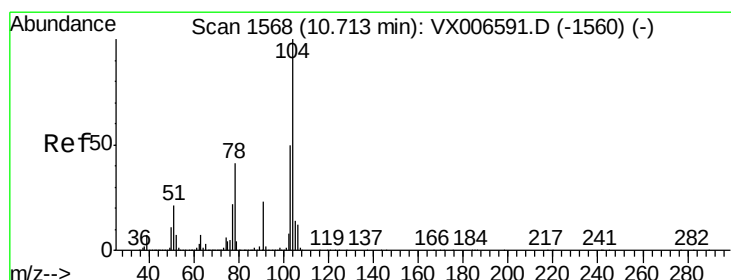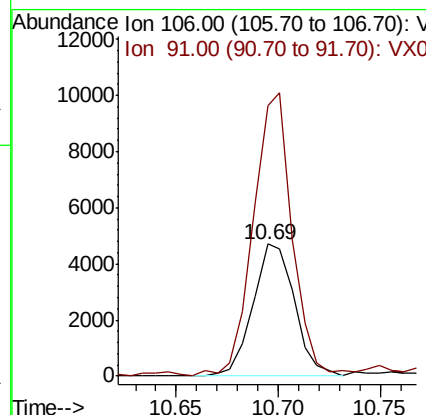

#70
Styrene
Concen: 2.460 ug/l
RT: 10.71 min Scan# 1568
Delta R.T. -0.00 min
Lab File: VX006803.D
Acq: 24 Dec 2018 18:51

Tgt Ion:104 Resp: 50536
Ion Ratio Lower Upper
104 100
78 41.6 37.7 56.5
103 48.5 43.8 65.8

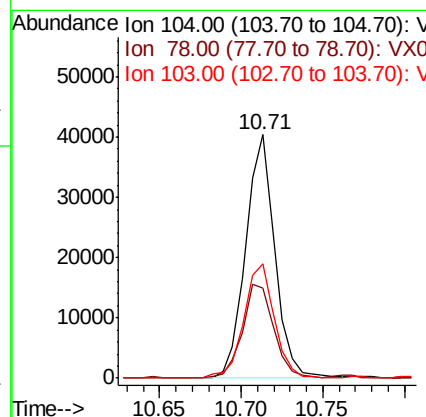







#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.08 min Scan# 1792
 Delta R.T. -0.00 min
 Lab File: VX006803.D
 Acq: 24 Dec 2018 18:51

Instrument :
 MSVOA_X
 ClientSampled :
 COMP-3

Tot Ion:152 Resp: 494175
 Ion Ratio Lower Upper
 152 100
 115 54.5 39.1 117.2
 150 154.6 0.0 344.8

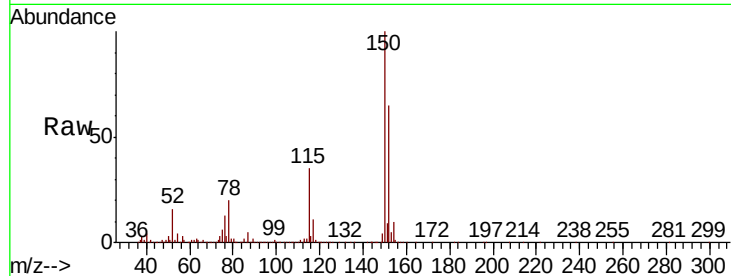


Abundance Ion 151.90 (151.60 to 152.60): V
 Ion 114.90 (114.60 to 115.60): V
 Ion 149.90 (149.60 to 150.60): V

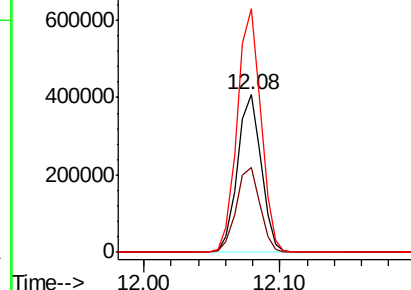




#76
 1,2,3-Trichloropropane
 Concen: 23.298 ug/l
 RT: 11.13 min Scan# 1637
 Delta R.T. -0.16 min
 Lab File: VX006803.D
 Acq: 24 Dec 2018 18:51

Tgt Ion: 75 Resp: 213969
 Ion Ratio Lower Upper
 75 100
 77 1.3 18.5 55.5#



Abundance Ion 74.90 (74.60 to 75.60): VX0
 Ion 77.00 (76.70 to 77.70): VX0

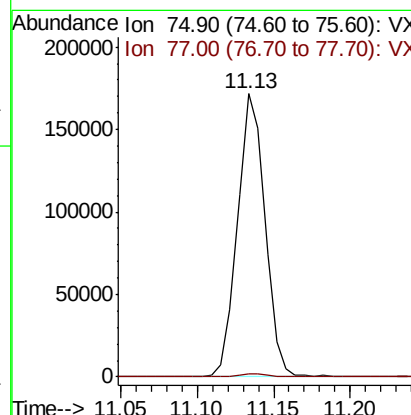

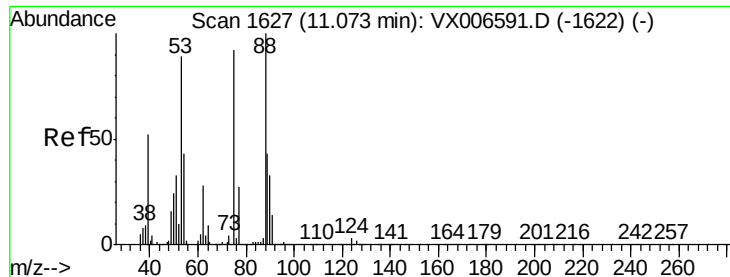

#81

trans-1,4-Dichloro-2-butene

Concen: 69.134 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. 0.06 min

Lab File: VX006803.D

Acq: 24 Dec 2018 18:51

Instrument :

MSVOA_X

ClientSampleId :

COMP-3


Tot Ion: 75 Resp: 213969

Ion Ratio Lower Upper

75 100

53 0.0 79.7 119.5#




89 0.1 38.0 57.0#

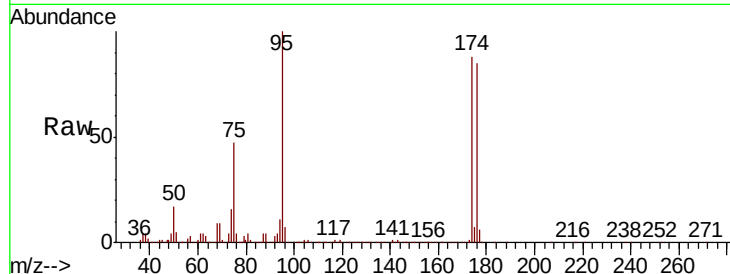

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 53.00 (52.70 to 53.70): VX0

Ion 88.90 (88.60 to 89.60): VX0

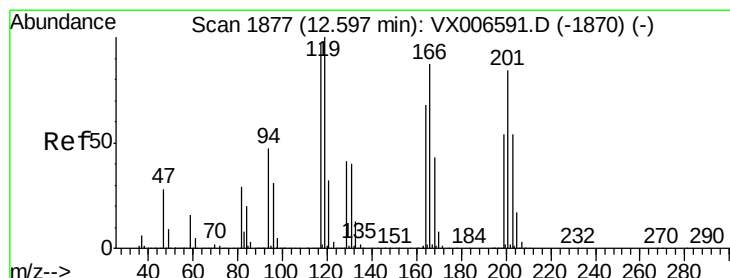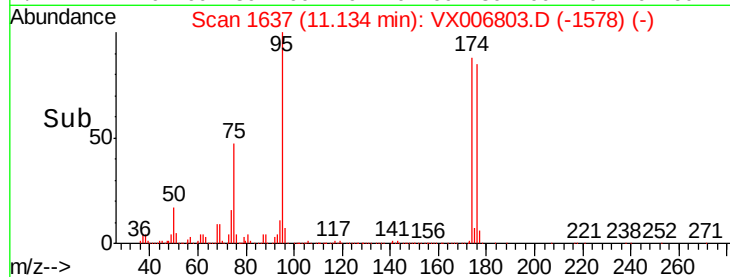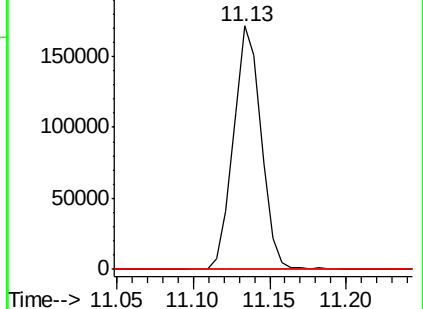

#90

Hexachloroethane

Concen: 3.380 ug/l

RT: 12.55 min Scan# 1870

Delta R.T. -0.04 min

Lab File: VX006803.D


Acq: 24 Dec 2018 18:51

Tgt Ion: 117 Resp: 435

Ion Ratio Lower Upper



117 100


201 0.0 42.9 128.7#

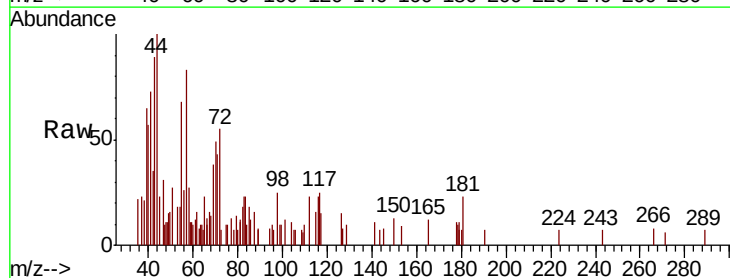

Abundance Ion 116.80 (116.50 to 117.50): V

Ion 200.70 (200.40 to 201.40): V

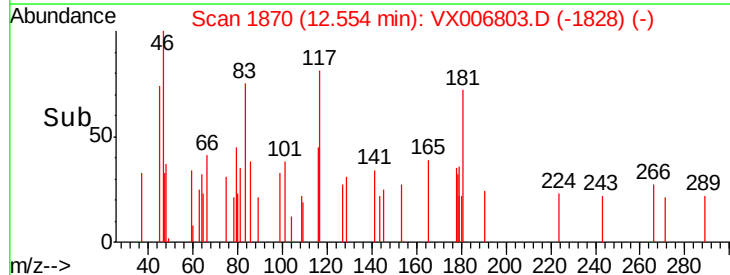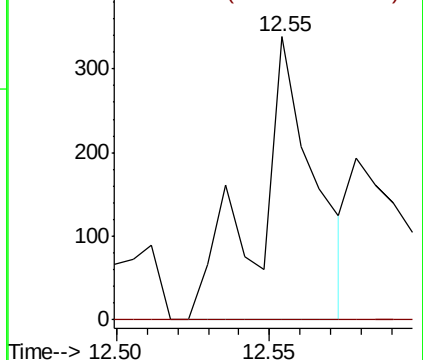




#95
Naphthalene
Concen: 1.291 ug/l
RT: 13.83 min Scan# 2080
Delta R.T. -0.00 min
Lab File: VX006803.D
Acq: 24 Dec 2018 18:51

Instrument :
MSVOA_X
ClientSampleId :
COMP-3

Tot Ion	Ratio	Lower	Upper
128	100		
127	13.9	10.1	15.1
129	11.6	8.6	13.0



Abundance

Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

