

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX122418\
 Data File : VX006793.D
 Acq On : 24 Dec 2018 14:24
 Operator : JC/MD
 Sample : J6533-07
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMP-1

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X121818W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.404	36	41	46	rBV2	37542	57836	1.98%	0.286%
2	1.489	51	55	66	rVV	2308992	2682434	91.68%	13.260%
3	1.611	67	75	79	rVB3	34669	78394	2.68%	0.388%
4	2.446	207	212	218	rVB	54862	86031	2.94%	0.425%
5	3.032	301	308	311	rBV2	15765	37651	1.29%	0.186%
6	3.781	424	431	443	rVB3	38399	108008	3.69%	0.534%
7	4.354	515	525	537	rVB2	18723	52932	1.81%	0.262%
8	4.702	574	582	593	rBV	36021	104920	3.59%	0.519%
9	5.507	700	714	724	rBV	345806	982287	33.57%	4.856%
10	5.665	729	740	751	rVV	627332	1736420	59.35%	8.584%
11	6.068	794	806	814	rBV	363642	944792	32.29%	4.670%
12	6.147	814	819	830	rVB2	57689	149390	5.11%	0.738%
13	6.860	924	936	949	rBV	904213	2129638	72.79%	10.527%
14	8.713	1233	1240	1247	rBV	1952899	2925890	100.00%	14.463%
15	8.781	1247	1251	1261	rVB	91180	152988	5.23%	0.756%
16	10.110	1463	1469	1480	rBV	1882737	2560337	87.51%	12.656%
17	10.360	1503	1510	1515	rBV	57885	86837	2.97%	0.429%
18	10.701	1558	1566	1571	rBV	27493	44755	1.53%	0.221%
19	10.811	1579	1584	1590	rBV	30009	45776	1.56%	0.226%
20	11.134	1631	1637	1643	rBV	1583391	2042179	69.80%	10.095%
21	11.189	1643	1646	1652	rVB2	41542	54952	1.88%	0.272%
22	11.628	1713	1718	1721	rBV	53971	77705	2.66%	0.384%
23	11.658	1721	1723	1732	rVV4	23008	36854	1.26%	0.182%
24	11.737	1732	1736	1743	rVV	126260	161202	5.51%	0.797%
25	11.804	1743	1747	1753	rVB	24812	34369	1.17%	0.170%
26	11.920	1762	1766	1774	rVB	100620	140755	4.81%	0.696%
27	12.079	1786	1792	1800	rVB	1996584	2542939	86.91%	12.570%
28	12.274	1818	1824	1835	rBV	95687	171268	5.85%	0.847%


Sum of corrected areas: 20229539

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX122418\
Data File : VX006793.D
Acq On : 24 Dec 2018 14:24
Operator : JC/MD
Sample : J6533-07
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMP-1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X121818W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

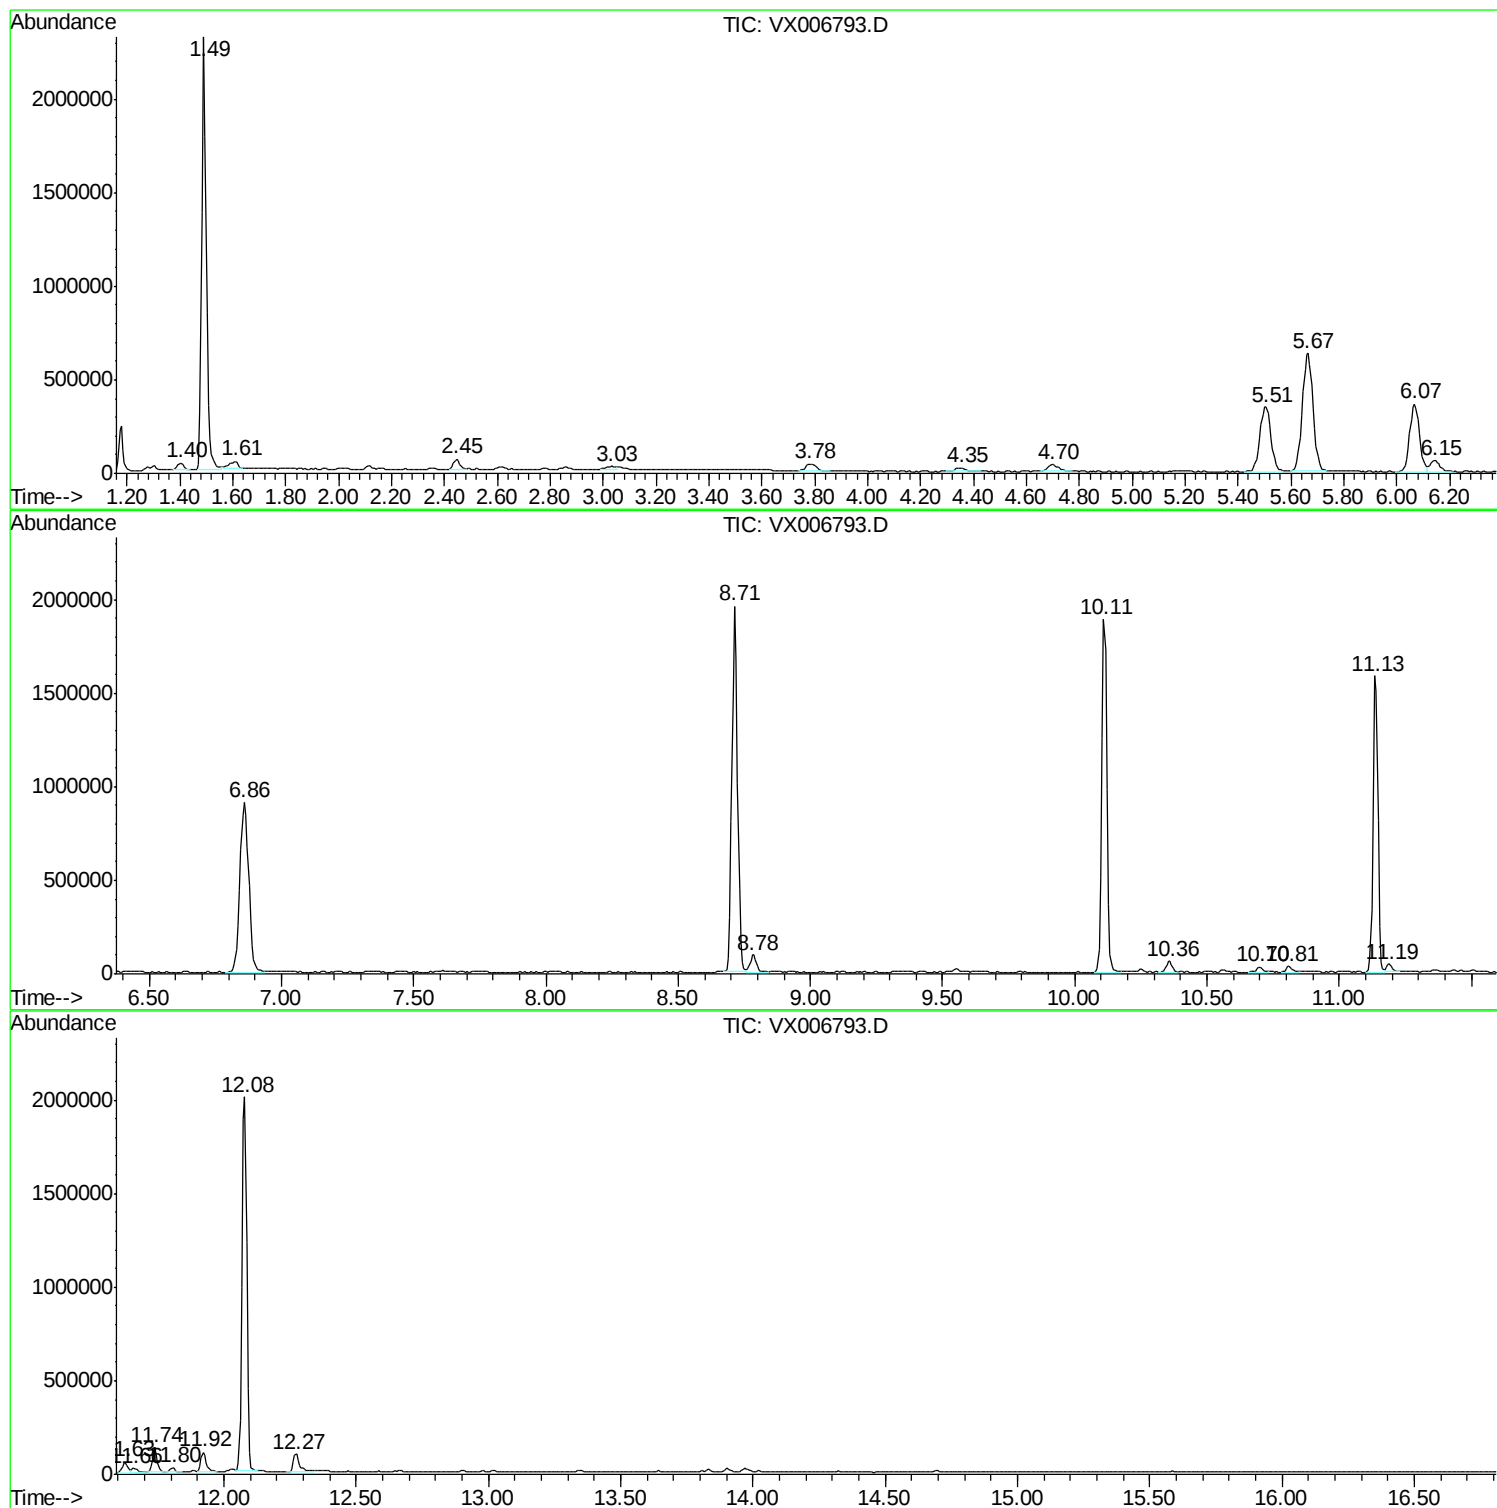

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX122418\
Data File : VX006793.D
Acq On : 24 Dec 2018 14:24
Operator : JC/MD
Sample : J6533-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMP-1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X121818W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX122418\
Data File : VX006793.D
Acq On : 24 Dec 2018 14:24
Operator : JC/MD
Sample : J6533-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMP-1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X121818W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc