


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122420\
 Data File : VX020375.D
 Acq On : 24 Dec 2020 08:38
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X121820W.M
 Title : SW846 8260
 Last Update : Fri Dec 18 13:09:49 2020

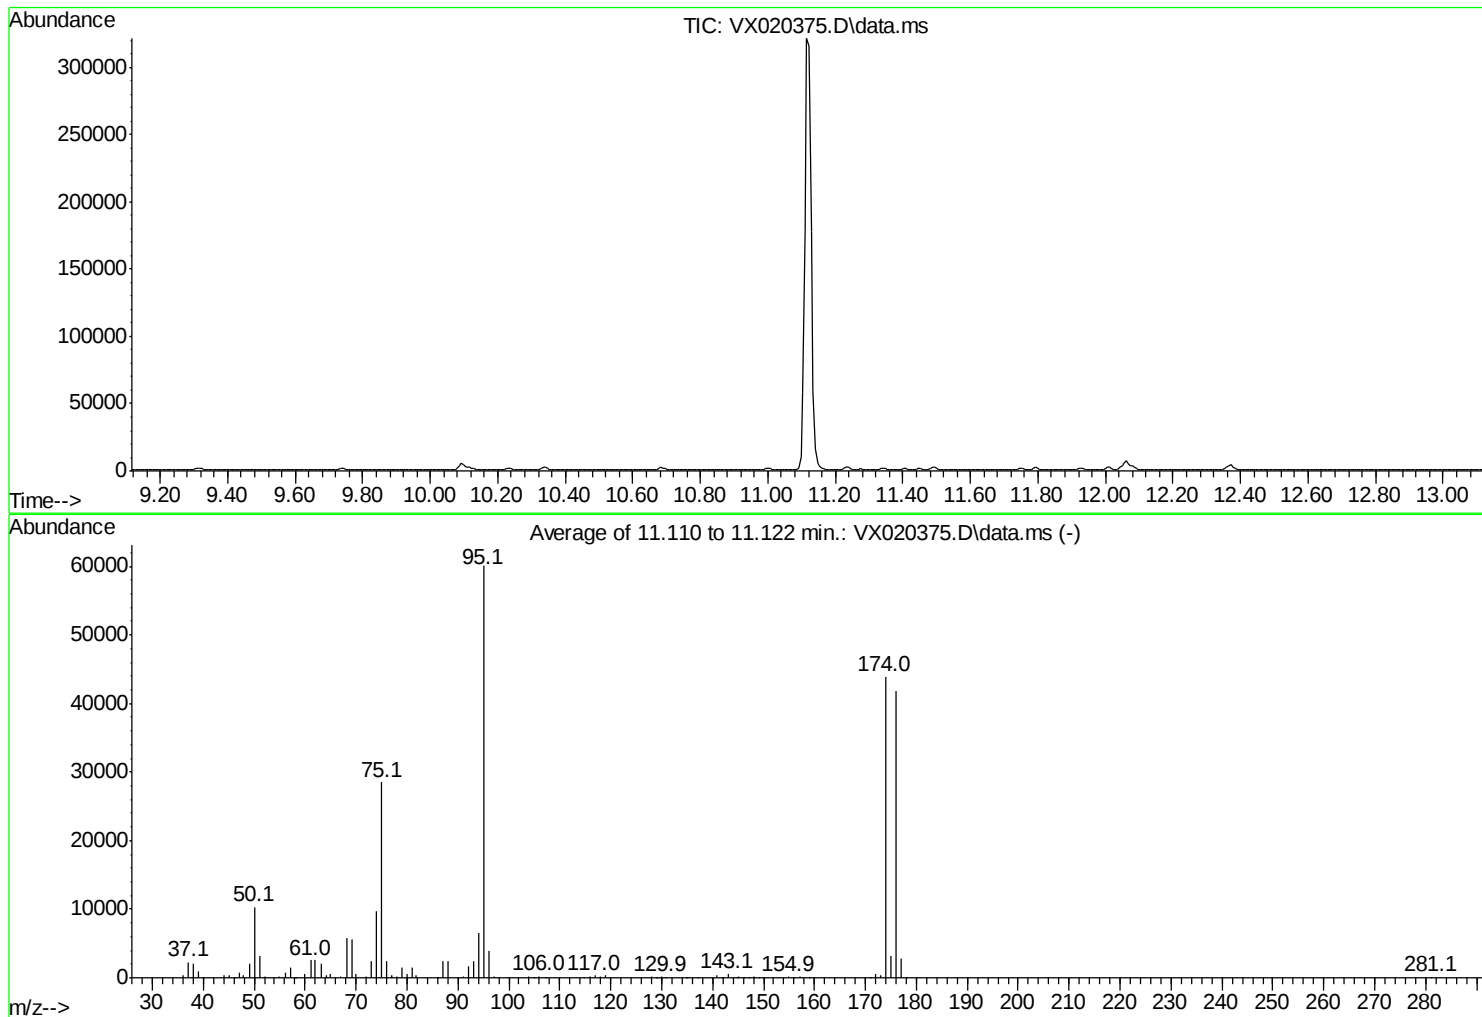

AutoFind: Scans 1644, 1645, 1646; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	10353	PASS
75	95	30	60	47.5	28547	PASS
95	95	100	100	100.0	60072	PASS
96	95	5	9	6.6	3952	PASS
173	174	0.00	2	1.0	428	PASS
174	95	50	100	73.0	43875	PASS
175	174	5	9	7.5	3271	PASS
176	174	95	101	95.1	41747	PASS
177	176	5	9	6.6	2774	PASS