

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122421\
 Data File : VX026012.D
 Acq On : 24 Dec 2021 13:54
 Operator : JC/MD
 Sample : M5126-07
 Misc : 5.00mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J24

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis

Signal : TIC: VX026012.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.373	43	47	56	rVB	139386	136659	13.58%	1.795%
2	1.672	91	96	105	rVB	98436	124167	12.34%	1.631%
3	2.312	195	201	211	rBV	209727	343193	34.10%	4.508%
4	2.794	277	280	286	rVB4	922	1439	0.14%	0.019%
5	2.843	286	288	292	rVB2	265	265	0.03%	0.003%
6	2.995	312	313	316	rBV2	339	271	0.03%	0.004%
7	3.105	329	331	333	rVV2	474	426	0.04%	0.006%
8	3.489	389	394	396	rBV2	176	312	0.03%	0.004%
9	3.550	401	404	405	rBV	306	241	0.02%	0.003%
10	3.592	409	411	414	rVV2	320	393	0.04%	0.005%
11	3.617	414	415	419	rVB2	449	387	0.04%	0.005%
12	4.117	495	497	499	rVV2	297	245	0.02%	0.003%
13	4.458	544	553	569	rBV	76902	229181	22.77%	3.010%
14	4.720	594	596	598	rBV2	272	303	0.03%	0.004%
15	4.903	625	626	629	rBV2	284	266	0.03%	0.003%
16	5.062	639	652	668	rBV	123898	396222	39.37%	5.204%
17	5.391	698	706	714	rBV6	2494	6460	0.64%	0.085%
18	5.562	728	734	735	rBV3	469	775	0.08%	0.010%
19	5.970	789	801	818	rBV2	336358	1006522	100.00%	13.220%
20	6.525	889	892	893	rBV2	316	265	0.03%	0.003%
21	6.763	920	931	949	rVV	232733	553182	54.96%	7.266%
22	6.939	958	960	963	rVB	377	260	0.03%	0.003%
23	6.976	963	966	968	rVB2	285	339	0.03%	0.004%
24	7.000	968	970	973	rBV2	200	239	0.02%	0.003%
25	7.128	982	991	1000	rBV2	16486	37910	3.77%	0.498%
26	7.311	1011	1021	1033	rBV	209916	457097	45.41%	6.004%
27	7.421	1037	1039	1045	rVB3	671	980	0.10%	0.013%
28	7.470	1045	1047	1048	rBV	535	508	0.05%	0.007%
29	7.927	1117	1122	1126	rBV2	518	962	0.10%	0.013%
30	8.018	1130	1137	1138	rVB2	217	341	0.03%	0.004%
31	8.323	1181	1187	1206	rVV	133946	218095	21.67%	2.865%
32	8.646	1234	1240	1248	rBV	501933	816516	81.12%	10.725%
33	8.720	1249	1252	1260	rVB	8020	12351	1.23%	0.162%
34	8.799	1260	1265	1266	rVB3	307	433	0.04%	0.006%
35	8.951	1284	1290	1299	rBV	91529	135977	13.51%	1.786%
36	9.110	1314	1316	1319	rBV2	326	417	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122421\
 Data File : VX026012.D
 Acq On : 24 Dec 2021 13:54
 Operator : JC/MD
 Sample : M5126-07
 Misc : 5.00mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J24

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis

37	9.140	1319	1321	1326	rVB3	321	398	0.04%	0.005%
38	9.274	1338	1343	1349	rBV3	27624	44900	4.46%	0.590%
39	9.384	1356	1361	1376	rVB	356354	502410	49.92%	6.599%
40	10.055	1465	1471	1483	rBV	510172	674787	67.04%	8.863%
41	10.195	1492	1494	1497	rVV2	683	611	0.06%	0.008%
42	10.244	1499	1502	1507	rVB2	1174	1511	0.15%	0.020%
43	10.299	1508	1511	1517	rVB3	1834	2323	0.23%	0.031%
44	10.445	1531	1535	1539	rBV	366	404	0.04%	0.005%
45	10.573	1552	1556	1559	rVV2	233	333	0.03%	0.004%
46	10.652	1565	1569	1574	rVV4	769	1227	0.12%	0.016%
47	10.750	1583	1585	1590	rBV2	252	405	0.04%	0.005%
48	10.866	1603	1604	1609	rBV2	289	327	0.03%	0.004%
49	10.969	1617	1621	1625	rVB2	624	862	0.09%	0.011%
50	11.122	1641	1646	1652	rBV2	3810	4637	0.46%	0.061%
51	11.195	1652	1658	1666	rBV	383783	479460	47.64%	6.297%
52	11.317	1674	1678	1685	rVB2	3901	6388	0.63%	0.084%
53	11.384	1685	1689	1690	rBV	199	249	0.02%	0.003%
54	11.481	1695	1705	1707	rBV5	1462	3075	0.31%	0.040%
55	11.542	1711	1715	1718	rBV	306	479	0.05%	0.006%
56	11.621	1724	1728	1729	rBV	315	288	0.03%	0.004%
57	11.676	1734	1737	1742	rBV2	545	898	0.09%	0.012%
58	11.750	1742	1749	1759	rVB6	4060	6367	0.63%	0.084%
59	11.847	1761	1765	1773	rVB4	832	1375	0.14%	0.018%
60	11.932	1776	1779	1783	rBV2	2026	2516	0.25%	0.033%
61	11.969	1783	1785	1788	rBV	531	511	0.05%	0.007%
62	12.024	1789	1794	1800	rBV	525024	652985	64.88%	8.577%
63	12.128	1808	1811	1813	rBV3	1094	1345	0.13%	0.018%
64	12.152	1813	1815	1821	rVB3	3087	3475	0.35%	0.046%
65	12.219	1821	1826	1831	rBV	10712	15022	1.49%	0.197%
66	12.323	1837	1843	1852	rVB	544071	695838	69.13%	9.140%
67	12.426	1857	1860	1864	rVB4	1387	1973	0.20%	0.026%
68	12.481	1866	1869	1876	rVB4	1119	1762	0.18%	0.023%
69	12.579	1883	1885	1889	rBV2	542	662	0.07%	0.009%
70	12.621	1890	1892	1895	rVB2	383	258	0.03%	0.003%
71	12.664	1895	1899	1904	rBV3	801	1442	0.14%	0.019%
72	12.768	1912	1916	1921	rVB2	1936	2729	0.27%	0.036%
73	12.822	1922	1925	1927	rBV	352	316	0.03%	0.004%
74	12.969	1945	1949	1950	rBV2	395	365	0.04%	0.005%
75	13.054	1960	1963	1967	rVV3	873	1072	0.11%	0.014%
76	13.109	1970	1972	1975	rBV2	501	434	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122421\
 Data File : VX026012.D
 Acq On : 24 Dec 2021 13:54
 Operator : JC/MD
 Sample : M5126-07
 Misc : 5.00mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J24

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
 Title : VOC Analysis

77	13.152	1977	1979	1982	rBV	190	237	0.02%	0.003%
78	13.213	1987	1989	1992	rVB	331	322	0.03%	0.004%
79	13.249	1992	1995	1997	rBV	294	310	0.03%	0.004%
80	13.517	2035	2039	2041	rBV2	307	495	0.05%	0.007%
81	13.725	2071	2073	2075	rBV	454	389	0.04%	0.005%
82	13.780	2079	2082	2086	rVV	856	1003	0.10%	0.013%
83	13.889	2097	2100	2103	rVB3	331	409	0.04%	0.005%
84	13.963	2110	2112	2115	rVB2	350	358	0.04%	0.005%
85	14.133	2136	2140	2146	rVB	2971	4240	0.42%	0.056%
86	14.200	2149	2151	2152	rBV	357	241	0.02%	0.003%
87	14.231	2155	2156	2160	rVB	337	267	0.03%	0.004%
88	14.645	2221	2224	2227	rVB3	720	783	0.08%	0.010%
89	14.810	2249	2251	2253	rVB	432	254	0.03%	0.003%
90	14.883	2261	2263	2264	rBV2	418	266	0.03%	0.003%
91	14.950	2272	2274	2278	rVB2	443	410	0.04%	0.005%
92	14.987	2278	2280	2283	rBV2	316	373	0.04%	0.005%
93	15.029	2286	2287	2292	rVV3	346	365	0.04%	0.005%
94	15.170	2309	2310	2311	rBV	475	249	0.02%	0.003%
95	15.225	2317	2319	2321	rBV3	403	304	0.03%	0.004%
96	15.694	2394	2396	2399	rBV2	530	536	0.05%	0.007%
97	16.005	2444	2447	2449	rBV2	477	523	0.05%	0.007%
98	16.584	2540	2542	2544	rBV2	481	370	0.04%	0.005%
99	16.608	2544	2546	2549	rVB2	641	437	0.04%	0.006%
100	16.639	2549	2551	2553	rBV3	417	354	0.04%	0.005%


Sum of corrected areas: 7613513

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122421\
Data File : VX026012.D
Acq On : 24 Dec 2021 13:54
Operator : JC/MD
Sample : M5126-07
Misc : 5.00mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

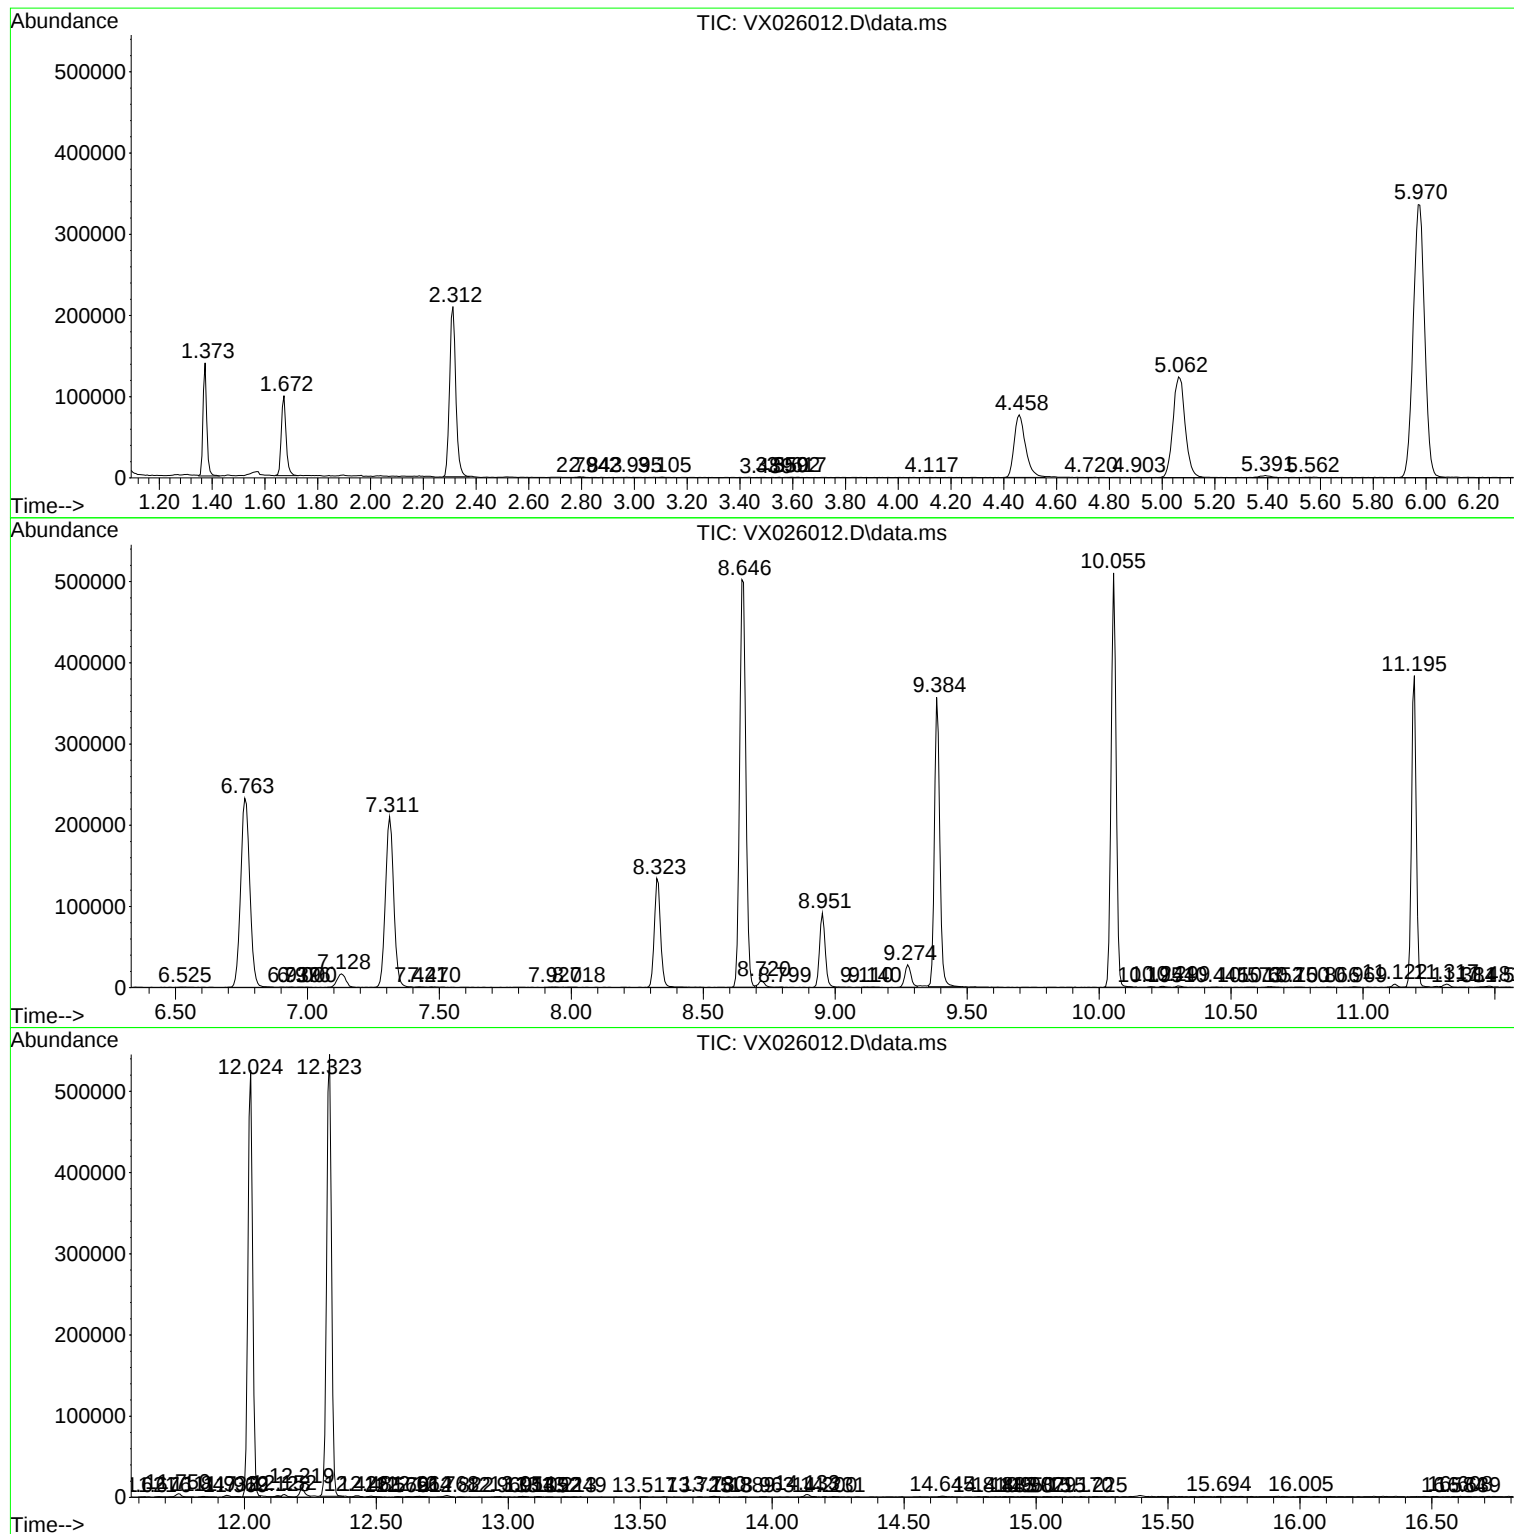

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122421\
Data File : VX026012.D
Acq On : 24 Dec 2021 13:54
Operator : JC/MD
Sample : M5126-07
Misc : 5.00mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122421\
Data File : VX026012.D
Acq On : 24 Dec 2021 13:54
Operator : JC/MD
Sample : M5126-07
Misc : 5.00mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------