

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122421\
 Data File : VX026013.D
 Acq On : 24 Dec 2021 14:35
 Operator : JC/MD
 Sample : M5126-11
 Misc : 5.00mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J18

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis

Signal : TIC: VX026013.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.373	43	47	56	rVB	159217	162251	13.75%	1.833%
2	1.672	91	96	104	rBV	121108	150748	12.77%	1.703%
3	2.306	194	200	209	rBV	256130	417473	35.37%	4.717%
4	2.513	231	234	236	rBV2	736	1081	0.09%	0.012%
5	2.702	261	265	272	rVB2	404	656	0.06%	0.007%
6	2.965	299	308	315	rVB2	743	2062	0.17%	0.023%
7	3.330	363	368	373	rVV3	954	1995	0.17%	0.023%
8	3.385	373	377	381	rVV2	228	376	0.03%	0.004%
9	3.428	381	384	385	rVV2	221	226	0.02%	0.003%
10	3.495	393	395	398	rVV	274	260	0.02%	0.003%
11	3.611	410	414	420	rVB4	471	998	0.08%	0.011%
12	3.653	420	421	427	rBV	200	222	0.02%	0.003%
13	3.806	443	446	447	rBV2	287	301	0.03%	0.003%
14	3.824	447	449	452	rVB2	240	256	0.02%	0.003%
15	4.056	485	487	490	rVB2	328	288	0.02%	0.003%
16	4.086	490	492	495	rBV2	206	276	0.02%	0.003%
17	4.220	507	514	518	rBV4	968	2250	0.19%	0.025%
18	4.275	522	523	526	rVB2	289	226	0.02%	0.003%
19	4.452	543	552	568	rBV	82827	244132	20.68%	2.758%
20	4.641	581	583	588	rVB3	258	312	0.03%	0.004%
21	4.751	599	601	603	rBV2	276	257	0.02%	0.003%
22	4.928	629	630	633	rVB2	323	259	0.02%	0.003%
23	5.062	637	652	671	rBV	143077	466706	39.54%	5.273%
24	5.220	674	678	681	rBV2	208	407	0.03%	0.005%
25	5.385	699	705	714	rVB5	963	2895	0.25%	0.033%
26	5.501	721	724	726	rBV2	202	293	0.02%	0.003%
27	5.879	783	786	788	rBV2	289	343	0.03%	0.004%
28	5.970	788	801	815	rBV2	399989	1180425	100.00%	13.337%
29	6.165	832	833	836	rVB2	418	299	0.03%	0.003%
30	6.653	911	913	915	rBV2	224	219	0.02%	0.002%
31	6.683	915	918	919	rBV	271	220	0.02%	0.002%
32	6.763	921	931	947	rVV	265874	645291	54.67%	7.291%
33	6.927	957	958	960	rVB2	337	220	0.02%	0.002%
34	7.128	983	991	1001	rVB5	8156	19064	1.62%	0.215%
35	7.208	1003	1004	1008	rBV	280	274	0.02%	0.003%
36	7.305	1010	1020	1032	rBV	245208	543974	46.08%	6.146%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122421\
 Data File : VX026013.D
 Acq On : 24 Dec 2021 14:35
 Operator : JC/MD
 Sample : M5126-11
 Misc : 5.00mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J18

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis

37	7.427	1036	1040	1046	rVB4	1931	3485	0.30%	0.039%
38	7.592	1060	1067	1071	rBV3	1092	2113	0.18%	0.024%
39	7.781	1096	1098	1099	rBV2	284	295	0.02%	0.003%
40	7.854	1105	1110	1117	rVV4	2561	4857	0.41%	0.055%
41	7.933	1120	1123	1129	rVB2	524	790	0.07%	0.009%
42	8.323	1180	1187	1201	rBV	160301	254463	21.56%	2.875%
43	8.579	1225	1229	1231	rBV3	694	919	0.08%	0.010%
44	8.646	1233	1240	1248	rBV	618038	968027	82.01%	10.937%
45	8.720	1248	1252	1259	rVV	9275	15529	1.32%	0.175%
46	8.951	1283	1290	1304	rBV	106451	154684	13.10%	1.748%
47	9.043	1304	1305	1308	rVB2	365	309	0.03%	0.003%
48	9.213	1331	1333	1336	rBV2	185	242	0.02%	0.003%
49	9.274	1338	1343	1348	rBV3	4313	8759	0.74%	0.099%
50	9.384	1355	1361	1375	rVB	405155	559461	47.39%	6.321%
51	9.774	1422	1425	1426	rBV2	295	316	0.03%	0.004%
52	9.908	1444	1447	1450	rBV2	227	225	0.02%	0.003%
53	10.055	1465	1471	1484	rBV	579272	784391	66.45%	8.863%
54	10.195	1491	1494	1497	rVB4	773	853	0.07%	0.010%
55	10.238	1498	1501	1508	rVB2	1383	1901	0.16%	0.021%
56	10.305	1508	1512	1517	rVB2	1544	2197	0.19%	0.025%
57	10.652	1563	1569	1573	rBV5	1137	1898	0.16%	0.021%
58	10.768	1581	1588	1592	rBV4	362	872	0.07%	0.010%
59	10.860	1599	1603	1606	rVB2	536	639	0.05%	0.007%
60	10.963	1617	1620	1623	rVB2	294	365	0.03%	0.004%
61	11.030	1626	1631	1636	rBV4	1401	2172	0.18%	0.025%
62	11.122	1641	1646	1650	rBV2	4668	6062	0.51%	0.068%
63	11.195	1652	1658	1665	rBV	401745	533230	45.17%	6.025%
64	11.280	1670	1672	1674	rBV2	816	767	0.06%	0.009%
65	11.378	1686	1688	1692	rBV3	626	739	0.06%	0.008%
66	11.451	1697	1700	1701	rBV2	666	646	0.05%	0.007%
67	11.475	1701	1704	1709	rVV5	1640	2913	0.25%	0.033%
68	11.548	1713	1716	1722	rVB3	643	870	0.07%	0.010%
69	11.750	1745	1749	1755	rVB3	5150	6998	0.59%	0.079%
70	11.841	1759	1764	1769	rVB3	1029	1389	0.12%	0.016%
71	11.932	1775	1779	1783	rBV2	2497	3621	0.31%	0.041%
72	12.024	1788	1794	1800	rBV	636131	793417	67.21%	8.965%
73	12.121	1806	1810	1812	rBV3	1910	2639	0.22%	0.030%
74	12.219	1821	1826	1836	rBV2	9948	16173	1.37%	0.183%
75	12.323	1837	1843	1851	rVB	656622	842869	71.40%	9.523%
76	12.426	1857	1860	1864	rVB3	1289	1762	0.15%	0.020%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122421\
 Data File : VX026013.D
 Acq On : 24 Dec 2021 14:35
 Operator : JC/MD
 Sample : M5126-11
 Misc : 5.00mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J18

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
 Title : VOC Analysis

77	12.481	1867	1869	1874	rVB4	1034	1210	0.10%	0.014%
78	12.603	1886	1889	1891	rVV2	501	510	0.04%	0.006%
79	12.762	1911	1915	1920	rBV2	1369	2238	0.19%	0.025%
80	12.810	1920	1923	1927	rBV3	553	786	0.07%	0.009%
81	13.109	1971	1972	1973	rBV	455	279	0.02%	0.003%
82	13.188	1983	1985	1988	rBV2	302	414	0.04%	0.005%
83	13.280	1998	2000	2002	rVB	251	257	0.02%	0.003%
84	13.426	2023	2024	2029	rBV2	212	298	0.03%	0.003%
85	13.591	2049	2051	2054	rBV2	664	511	0.04%	0.006%
86	13.694	2066	2068	2069	rVB	383	275	0.02%	0.003%
87	13.780	2078	2082	2087	rVB	2355	2861	0.24%	0.032%
88	13.883	2097	2099	2102	rBV2	372	386	0.03%	0.004%
89	13.969	2108	2113	2116	rVB4	498	928	0.08%	0.010%
90	14.030	2120	2123	2125	rBV	209	236	0.02%	0.003%
91	14.133	2132	2140	2146	rBV2	1991	3323	0.28%	0.038%
92	14.505	2199	2201	2205	rBV2	340	590	0.05%	0.007%
93	14.639	2221	2223	2228	rVV4	638	682	0.06%	0.008%
94	14.786	2243	2247	2251	rVB3	731	1332	0.11%	0.015%
95	14.889	2261	2264	2265	rBV2	294	290	0.02%	0.003%
96	15.029	2285	2287	2289	rVB2	455	383	0.03%	0.004%
97	15.694	2395	2396	2398	rVB2	516	231	0.02%	0.003%
98	15.956	2436	2439	2440	rBV	598	464	0.04%	0.005%
99	16.352	2502	2504	2506	rBV2	409	354	0.03%	0.004%
100	16.450	2518	2520	2522	rBV	570	368	0.03%	0.004%


Sum of corrected areas: 8850598

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122421\
Data File : VX026013.D
Acq On : 24 Dec 2021 14:35
Operator : JC/MD
Sample : M5126-11
Misc : 5.00mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J18

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

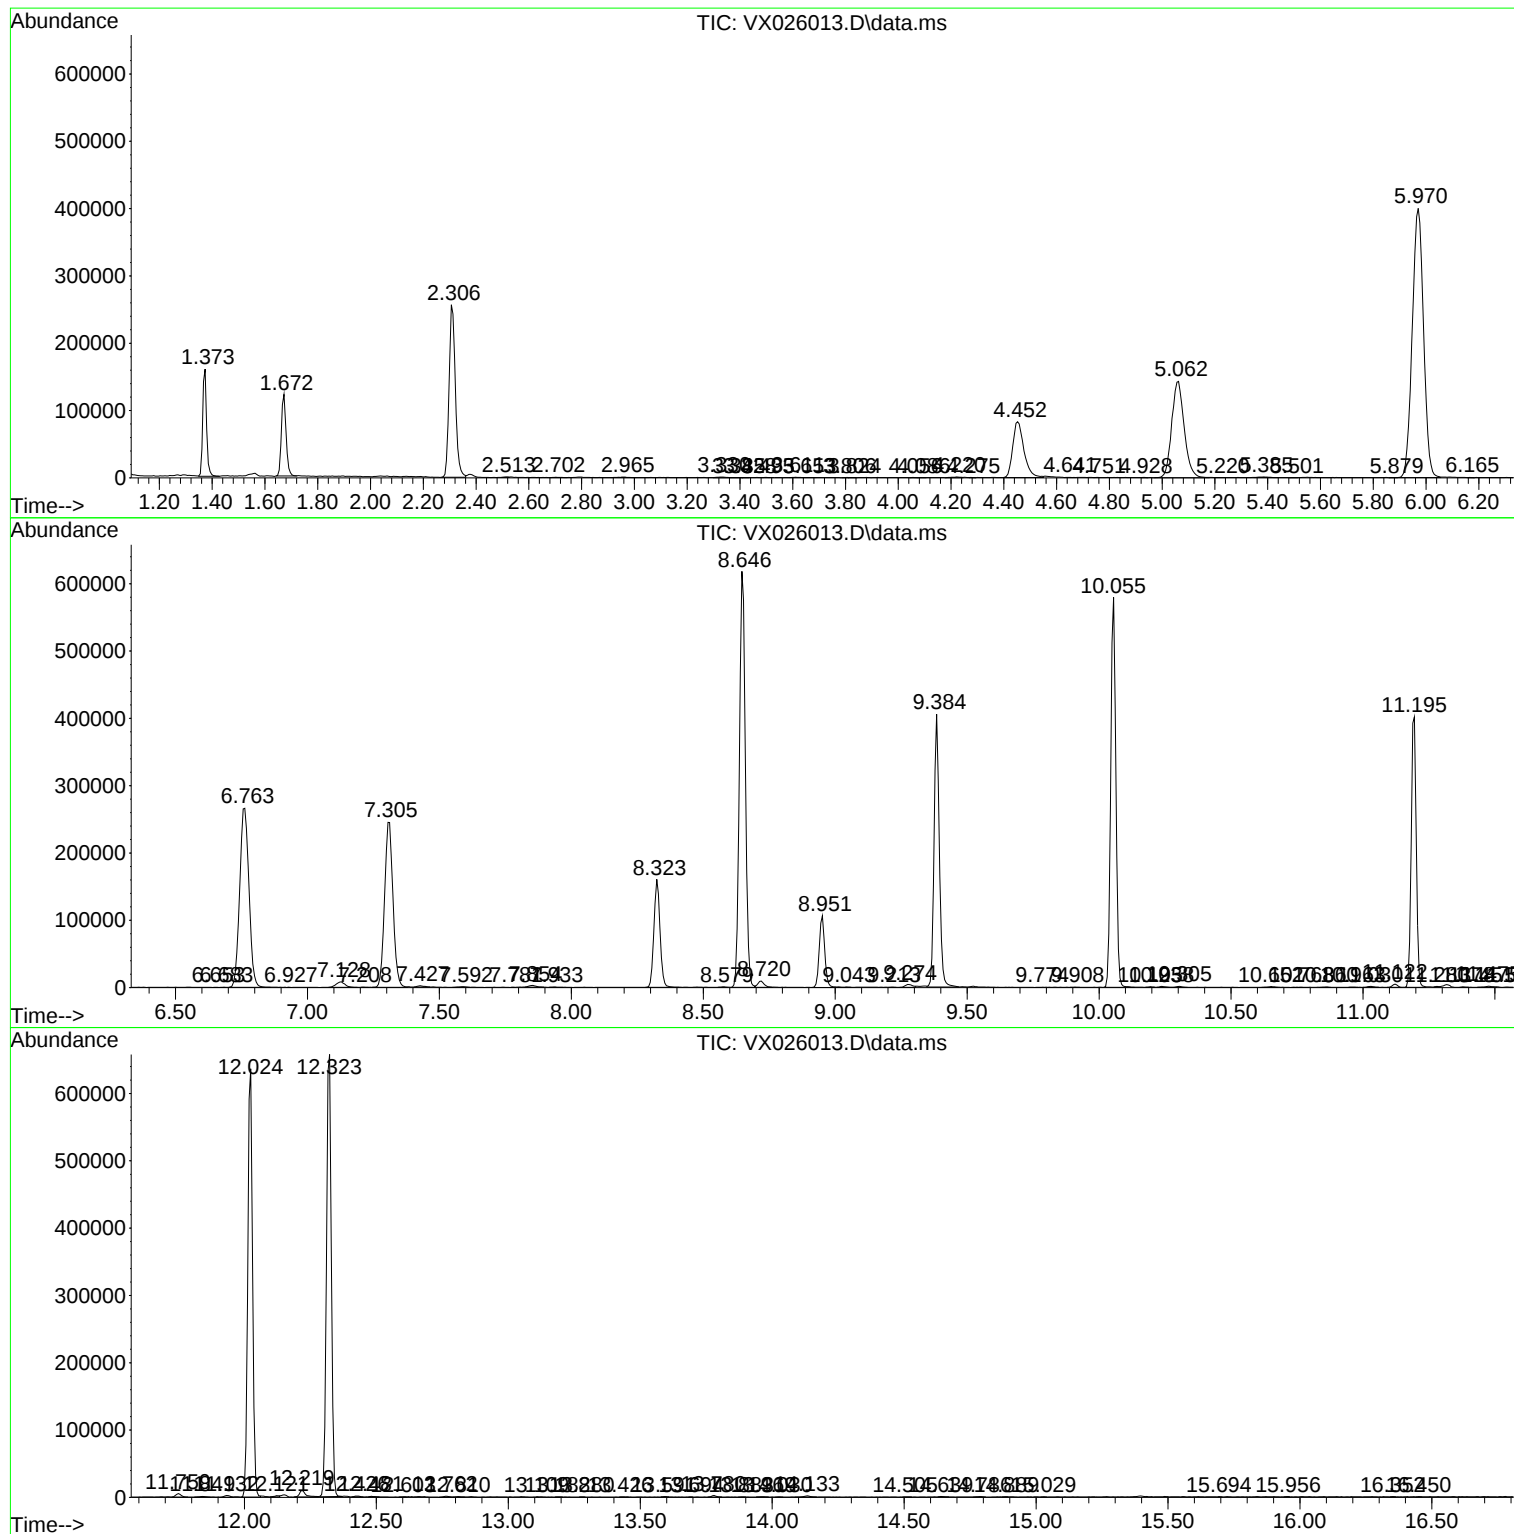

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122421\
Data File : VX026013.D
Acq On : 24 Dec 2021 14:35
Operator : JC/MD
Sample : M5126-11
Misc : 5.00mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J18

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122421\
Data File : VX026013.D
Acq On : 24 Dec 2021 14:35
Operator : JC/MD
Sample : M5126-11
Misc : 5.00mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J18

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc