

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122421\
 Data File : VX026014.D
 Acq On : 24 Dec 2021 14:59
 Operator : JC/MD
 Sample : M5126-15
 Misc : 5.00mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J26

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis

Signal : TIC: VX026014.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	53	rVB	130290	127889	13.25%	1.755%
2	1.672	91	96	107	rBV	92328	121476	12.59%	1.667%
3	2.312	195	201	210	rBV	215686	347797	36.04%	4.773%
4	2.538	233	238	244	rBV3	1615	3024	0.31%	0.041%
5	2.703	262	265	267	rBV	529	529	0.05%	0.007%
6	2.788	276	279	286	rBV3	1133	1922	0.20%	0.026%
7	2.898	293	297	299	rBV2	463	456	0.05%	0.006%
8	3.117	330	333	335	rBV3	596	680	0.07%	0.009%
9	3.428	383	384	387	rBV	338	236	0.02%	0.003%
10	3.605	410	413	414	rBV3	412	384	0.04%	0.005%
11	3.751	435	437	438	rVV	239	200	0.02%	0.003%
12	4.044	482	485	487	rVV	227	206	0.02%	0.003%
13	4.404	542	544	545	rBV	271	228	0.02%	0.003%
14	4.458	545	553	568	rBV	74405	217948	22.58%	2.991%
15	4.818	609	612	614	rVB2	229	234	0.02%	0.003%
16	4.916	625	628	630	rBV	215	220	0.02%	0.003%
17	5.062	640	652	669	rBV	119834	376020	38.96%	5.160%
18	5.336	696	697	698	rBV	466	261	0.03%	0.004%
19	5.391	698	706	715	rVB3	3473	9330	0.97%	0.128%
20	5.550	726	732	739	rBV3	595	1463	0.15%	0.020%
21	5.970	787	801	817	rBV2	319936	965139	100.00%	13.245%
22	6.117	824	825	828	rVB2	421	300	0.03%	0.004%
23	6.275	848	851	854	rBV2	266	357	0.04%	0.005%
24	6.397	870	871	875	rBV	236	330	0.03%	0.005%
25	6.464	879	882	883	rBV3	289	263	0.03%	0.004%
26	6.531	891	893	895	rBV2	254	269	0.03%	0.004%
27	6.647	910	912	914	rBV	239	219	0.02%	0.003%
28	6.763	921	931	944	rBV	217236	518473	53.72%	7.115%
29	7.013	970	972	976	rVB3	245	316	0.03%	0.004%
30	7.129	982	991	1002	rBV	21580	47583	4.93%	0.653%
31	7.214	1002	1005	1011	rVB2	322	430	0.04%	0.006%
32	7.312	1011	1021	1036	rBV	197684	439293	45.52%	6.029%
33	7.482	1046	1049	1052	rBV2	595	669	0.07%	0.009%
34	7.568	1061	1063	1066	rBV2	180	247	0.03%	0.003%
35	8.324	1181	1187	1196	rBV	129809	209078	21.66%	2.869%
36	8.427	1202	1204	1206	rVB	254	236	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122421\
 Data File : VX026014.D
 Acq On : 24 Dec 2021 14:59
 Operator : JC/MD
 Sample : M5126-15
 Misc : 5.00mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J26

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis

37	8.653	1234	1241	1248	rVV	498960	786450	81.49%	10.793%
38	8.720	1249	1252	1259	rVB	7354	11437	1.19%	0.157%
39	8.951	1284	1290	1299	rVV	88475	127240	13.18%	1.746%
40	9.281	1338	1344	1349	rBV3	7015	13096	1.36%	0.180%
41	9.384	1356	1361	1376	rVB	348344	486772	50.44%	6.680%
42	9.646	1402	1404	1408	rBV3	218	296	0.03%	0.004%
43	9.781	1423	1426	1428	rBV2	153	211	0.02%	0.003%
44	10.055	1465	1471	1481	rBV	498172	642663	66.59%	8.819%
45	10.189	1490	1493	1499	rVB3	483	1043	0.11%	0.014%
46	10.250	1499	1503	1506	rBV2	492	733	0.08%	0.010%
47	10.305	1508	1512	1516	rBV2	1285	1779	0.18%	0.024%
48	10.439	1532	1534	1536	rBV	344	223	0.02%	0.003%
49	10.646	1563	1568	1572	rVB3	485	835	0.09%	0.011%
50	10.756	1585	1586	1588	rVB2	363	208	0.02%	0.003%
51	10.805	1592	1594	1597	rVB2	320	302	0.03%	0.004%
52	10.841	1597	1600	1602	rBV2	299	386	0.04%	0.005%
53	10.963	1617	1620	1623	rVB3	399	468	0.05%	0.006%
54	11.122	1641	1646	1649	rBV2	3489	4540	0.47%	0.062%
55	11.195	1652	1658	1665	rVV	356704	463947	48.07%	6.367%
56	11.274	1669	1671	1673	rVV	945	1060	0.11%	0.015%
57	11.317	1673	1678	1683	rVV2	6518	10055	1.04%	0.138%
58	11.384	1687	1689	1692	rVV2	254	353	0.04%	0.005%
59	11.488	1697	1706	1709	rVV6	1346	3196	0.33%	0.044%
60	11.542	1713	1715	1719	rVB2	377	424	0.04%	0.006%
61	11.622	1725	1728	1732	rVB2	483	643	0.07%	0.009%
62	11.664	1734	1735	1737	rVV	308	213	0.02%	0.003%
63	11.683	1737	1738	1740	rVV2	394	262	0.03%	0.004%
64	11.713	1741	1743	1744	rVV	268	219	0.02%	0.003%
65	11.750	1745	1749	1754	rVB2	3451	4303	0.45%	0.059%
66	11.853	1761	1766	1768	rBV2	573	768	0.08%	0.011%
67	11.933	1776	1779	1783	rBV3	1430	1897	0.20%	0.026%
68	11.969	1783	1785	1788	rBV	452	399	0.04%	0.005%
69	12.024	1788	1794	1805	rBV	513438	631202	65.40%	8.662%
70	12.219	1822	1826	1831	rVV	4701	6640	0.69%	0.091%
71	12.323	1837	1843	1849	rVB	532354	670824	69.51%	9.206%
72	12.426	1857	1860	1863	rVB2	1130	1179	0.12%	0.016%
73	12.768	1911	1916	1922	rVB	2459	3544	0.37%	0.049%
74	12.817	1922	1924	1926	rBV	271	199	0.02%	0.003%
75	13.054	1959	1963	1966	rBV	558	784	0.08%	0.011%
76	13.121	1970	1974	1975	rBV2	317	309	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122421\
 Data File : VX026014.D
 Acq On : 24 Dec 2021 14:59
 Operator : JC/MD
 Sample : M5126-15
 Misc : 5.00mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J26

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
 Title : VOC Analysis

77	13.134	1975	1976	1979	rBV2	296	242	0.03%	0.003%
78	13.268	1997	1998	2002	rBV2	217	276	0.03%	0.004%
79	13.304	2002	2004	2007	rVB	276	233	0.02%	0.003%
80	13.335	2007	2009	2012	rBV2	236	223	0.02%	0.003%
81	13.780	2078	2082	2088	rVB2	650	1100	0.11%	0.015%
82	13.884	2097	2099	2101	rVB2	300	220	0.02%	0.003%
83	14.133	2135	2140	2147	rVV	3335	4030	0.42%	0.055%
84	14.243	2156	2158	2162	rBV2	218	277	0.03%	0.004%
85	14.286	2162	2165	2166	rVB2	263	237	0.02%	0.003%
86	14.390	2180	2182	2185	rVB2	264	214	0.02%	0.003%
87	14.438	2185	2190	2192	rBV2	304	434	0.04%	0.006%
88	14.511	2201	2202	2205	rVB	597	391	0.04%	0.005%
89	14.542	2205	2207	2208	rBV2	242	243	0.03%	0.003%
90	14.646	2220	2224	2226	rVV3	593	622	0.06%	0.009%
91	14.682	2228	2230	2234	rVV	308	329	0.03%	0.005%
92	14.792	2246	2248	2249	rBV	325	203	0.02%	0.003%
93	15.030	2285	2287	2288	rBV2	277	241	0.02%	0.003%
94	15.164	2307	2309	2312	rBV3	317	387	0.04%	0.005%
95	15.194	2312	2314	2315	rBV2	421	273	0.03%	0.004%
96	15.255	2323	2324	2326	rBV2	388	333	0.03%	0.005%
97	15.639	2385	2387	2388	rBV	312	215	0.02%	0.003%
98	15.688	2393	2395	2397	rVB2	617	467	0.05%	0.006%
99	16.468	2521	2523	2525	rBV2	507	456	0.05%	0.006%
100	16.724	2563	2565	2568	rBV2	408	426	0.04%	0.006%




Sum of corrected areas: 7286879

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122421\
Data File : VX026014.D
Acq On : 24 Dec 2021 14:59
Operator : JC/MD
Sample : M5126-15
Misc : 5.00mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

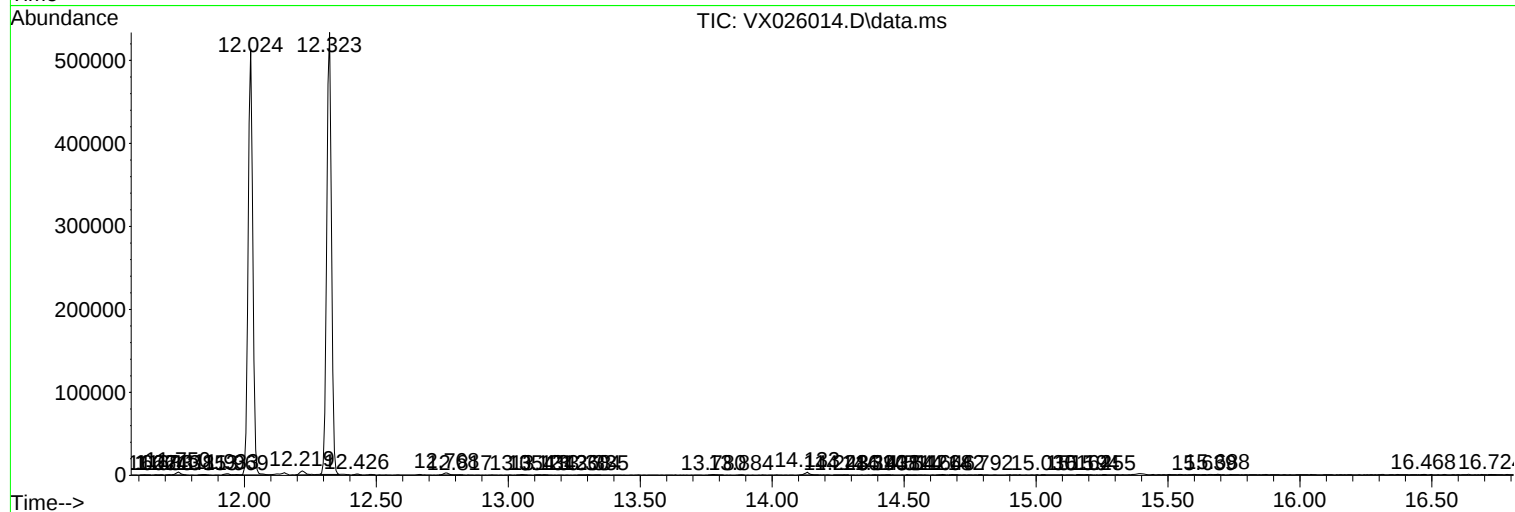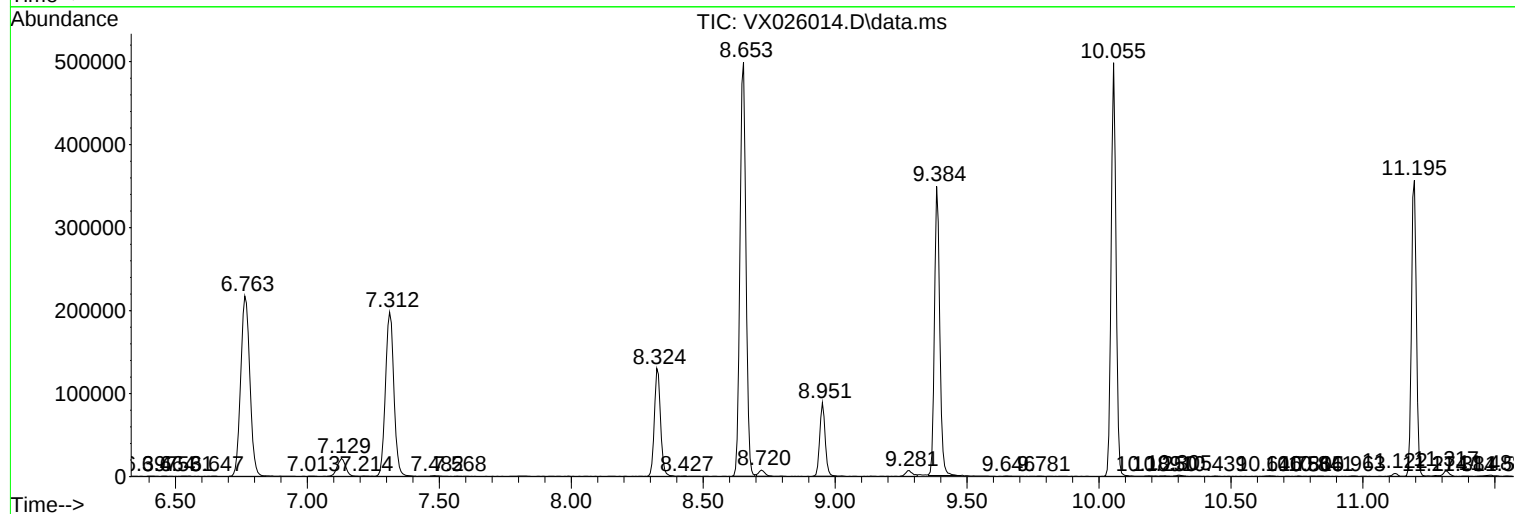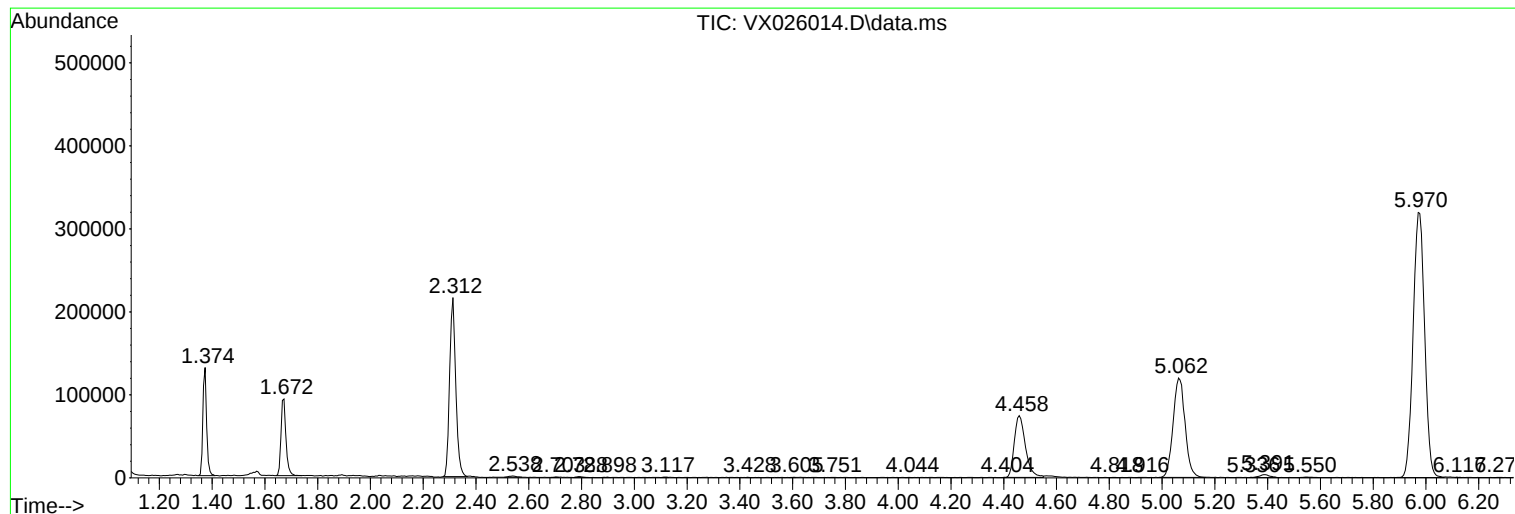

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122421\
Data File : VX026014.D
Acq On : 24 Dec 2021 14:59
Operator : JC/MD
Sample : M5126-15
Misc : 5.00mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122421\
Data File : VX026014.D
Acq On : 24 Dec 2021 14:59
Operator : JC/MD
Sample : M5126-15
Misc : 5.00mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc