

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122421\
 Data File : VX026016.D
 Acq On : 24 Dec 2021 15:46
 Operator : JC/MD
 Sample : M5126-17
 Misc : 5.00mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J19

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis

Signal : TIC: VX026016.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.270	27	30	33	rBV	6535	6529	0.70%	0.090%
2	1.368	43	46	54	rVB	125727	132448	14.14%	1.825%
3	1.666	91	95	105	rVB	98585	119174	12.73%	1.642%
4	2.313	194	201	217	rVB	196274	325427	34.75%	4.484%
5	2.623	248	252	255	rBV2	455	693	0.07%	0.010%
6	2.697	261	264	265	rBV	364	333	0.04%	0.005%
7	2.788	276	279	284	rBV3	731	1424	0.15%	0.020%
8	3.044	320	321	324	rBV2	195	247	0.03%	0.003%
9	3.184	340	344	347	rBV	339	460	0.05%	0.006%
10	3.300	360	363	365	rBV2	183	248	0.03%	0.003%
11	3.404	378	380	385	rBV2	179	306	0.03%	0.004%
12	4.245	516	518	522	rBV2	208	344	0.04%	0.005%
13	4.367	537	538	542	rBV2	214	326	0.03%	0.004%
14	4.458	544	553	569	rBV2	70862	224631	23.99%	3.095%
15	4.794	605	608	610	rVB2	287	316	0.03%	0.004%
16	5.068	639	653	673	rVV2	108486	370737	39.59%	5.109%
17	5.397	704	707	710	rVV3	271	446	0.05%	0.006%
18	5.464	715	718	725	rVV4	634	1284	0.14%	0.018%
19	5.550	729	732	739	rVB3	406	751	0.08%	0.010%
20	5.757	761	766	767	rBV2	172	266	0.03%	0.004%
21	5.977	789	802	819	rBV2	313294	936418	100.00%	12.903%
22	6.092	819	821	824	rVB3	425	345	0.04%	0.005%
23	6.208	837	840	843	rBV2	235	328	0.04%	0.005%
24	6.452	878	880	885	rBV2	206	392	0.04%	0.005%
25	6.519	888	891	893	rBV	333	304	0.03%	0.004%
26	6.763	920	931	944	rBV	217004	518878	55.41%	7.150%
27	6.946	960	961	965	rBV2	286	312	0.03%	0.004%
28	7.110	984	988	995	rVV4	979	2026	0.22%	0.028%
29	7.312	1012	1021	1036	rBV	194787	425908	45.48%	5.869%
30	7.458	1042	1045	1046	rBV	246	287	0.03%	0.004%
31	7.482	1046	1049	1052	rVV2	383	499	0.05%	0.007%
32	7.592	1064	1067	1070	rVV2	253	348	0.04%	0.005%
33	7.933	1121	1123	1127	rVB2	356	387	0.04%	0.005%
34	8.250	1172	1175	1179	rBV2	201	254	0.03%	0.003%
35	8.330	1181	1188	1199	rBV	119671	199280	21.28%	2.746%
36	8.653	1234	1241	1248	rVV	493818	787818	84.13%	10.856%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122421\
 Data File : VX026016.D
 Acq On : 24 Dec 2021 15:46
 Operator : JC/MD
 Sample : M5126-17
 Misc : 5.00mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J19

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis

37	8.720	1248	1252	1258	rVB	9750	15150	1.62%	0.209%
38	8.952	1284	1290	1301	rBV	87665	126567	13.52%	1.744%
39	9.122	1316	1318	1321	rBV3	364	529	0.06%	0.007%
40	9.275	1336	1343	1348	rBV3	6391	12304	1.31%	0.170%
41	9.384	1356	1361	1380	rVB	367546	522748	55.82%	7.203%
42	9.525	1381	1384	1390	rVB6	1614	2490	0.27%	0.034%
43	9.665	1404	1407	1408	rBV2	298	298	0.03%	0.004%
44	9.756	1420	1422	1426	rBV2	254	281	0.03%	0.004%
45	10.055	1465	1471	1483	rVB	506662	659791	70.46%	9.092%
46	10.195	1489	1494	1498	rVB4	485	969	0.10%	0.013%
47	10.238	1498	1501	1508	rBV3	963	1474	0.16%	0.020%
48	10.305	1508	1512	1517	rBV	1656	2020	0.22%	0.028%
49	10.451	1533	1536	1539	rBV2	310	434	0.05%	0.006%
50	10.653	1565	1569	1574	rBV3	739	1196	0.13%	0.016%
51	10.854	1601	1602	1607	rVB3	294	409	0.04%	0.006%
52	11.122	1642	1646	1652	rVV2	3523	5146	0.55%	0.071%
53	11.195	1652	1658	1666	rVV	364159	464806	49.64%	6.405%
54	11.274	1669	1671	1674	rVV2	885	1246	0.13%	0.017%
55	11.317	1674	1678	1683	rVV3	4517	7343	0.78%	0.101%
56	11.402	1691	1692	1694	rBV	287	292	0.03%	0.004%
57	11.451	1696	1700	1702	rBV2	769	973	0.10%	0.013%
58	11.476	1702	1704	1707	rVB2	1073	1026	0.11%	0.014%
59	11.549	1714	1716	1720	rVB3	423	530	0.06%	0.007%
60	11.610	1724	1726	1729	rBV2	279	294	0.03%	0.004%
61	11.683	1734	1738	1741	rVV4	522	851	0.09%	0.012%
62	11.750	1745	1749	1756	rVB3	3281	4718	0.50%	0.065%
63	11.841	1762	1764	1768	rBV2	869	996	0.11%	0.014%
64	11.933	1775	1779	1783	rBV3	1828	2501	0.27%	0.034%
65	11.969	1783	1785	1788	rBV	469	387	0.04%	0.005%
66	12.024	1788	1794	1800	rBV	514309	641560	68.51%	8.840%
67	12.128	1808	1811	1812	rBV2	1001	839	0.09%	0.012%
68	12.219	1822	1826	1831	rBV2	7810	11134	1.19%	0.153%
69	12.323	1837	1843	1853	rVB	534467	680792	72.70%	9.381%
70	12.427	1857	1860	1864	rVB4	1344	1694	0.18%	0.023%
71	12.481	1865	1869	1873	rVB3	956	1265	0.14%	0.017%
72	12.536	1876	1878	1881	rVB2	307	357	0.04%	0.005%
73	12.591	1881	1887	1889	rBV4	454	789	0.08%	0.011%
74	12.658	1896	1898	1902	rBV3	623	681	0.07%	0.009%
75	12.768	1912	1916	1923	rVB	1980	2918	0.31%	0.040%
76	13.201	1985	1987	1990	rBV2	382	303	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122421\
 Data File : VX026016.D
 Acq On : 24 Dec 2021 15:46
 Operator : JC/MD
 Sample : M5126-17
 Misc : 5.00mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J19

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis

77	13.280	1999	2000	2005	rBV2	240	344	0.04%	0.005%
78	13.585	2048	2050	2056	rVB3	487	672	0.07%	0.009%
79	13.780	2078	2082	2085	rBV2	792	904	0.10%	0.012%
80	13.926	2103	2106	2107	rVV	310	360	0.04%	0.005%
81	13.963	2110	2112	2114	rVB2	491	346	0.04%	0.005%
82	14.012	2118	2120	2123	rVV2	360	358	0.04%	0.005%
83	14.054	2126	2127	2130	rVB2	318	268	0.03%	0.004%
84	14.134	2136	2140	2146	rVB2	3238	4510	0.48%	0.062%
85	14.195	2148	2150	2155	rVB2	303	409	0.04%	0.006%
86	14.268	2160	2162	2166	rVB	356	246	0.03%	0.003%
87	14.408	2183	2185	2186	rBV	464	261	0.03%	0.004%
88	14.445	2187	2191	2195	rVB2	293	426	0.05%	0.006%
89	14.481	2195	2197	2200	rVB	434	390	0.04%	0.005%
90	14.518	2200	2203	2205	rBV3	491	553	0.06%	0.008%
91	14.774	2243	2245	2247	rBV2	363	396	0.04%	0.005%
92	14.883	2259	2263	2266	rBV2	413	475	0.05%	0.007%
93	14.914	2266	2268	2271	rVV2	436	353	0.04%	0.005%
94	15.280	2326	2328	2329	rBV	357	300	0.03%	0.004%
95	15.396	2341	2347	2352	rVB3	1740	3603	0.38%	0.050%
96	15.438	2352	2354	2355	rBV2	442	353	0.04%	0.005%
97	15.457	2355	2357	2358	rBV2	403	312	0.03%	0.004%
98	15.914	2431	2432	2434	rBV2	378	261	0.03%	0.004%
99	16.054	2451	2455	2456	rBV3	426	563	0.06%	0.008%
100	16.603	2543	2545	2548	rVB3	358	290	0.03%	0.004%




Sum of corrected areas: 7257228

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122421\
Data File : VX026016.D
Acq On : 24 Dec 2021 15:46
Operator : JC/MD
Sample : M5126-17
Misc : 5.00mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J19

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

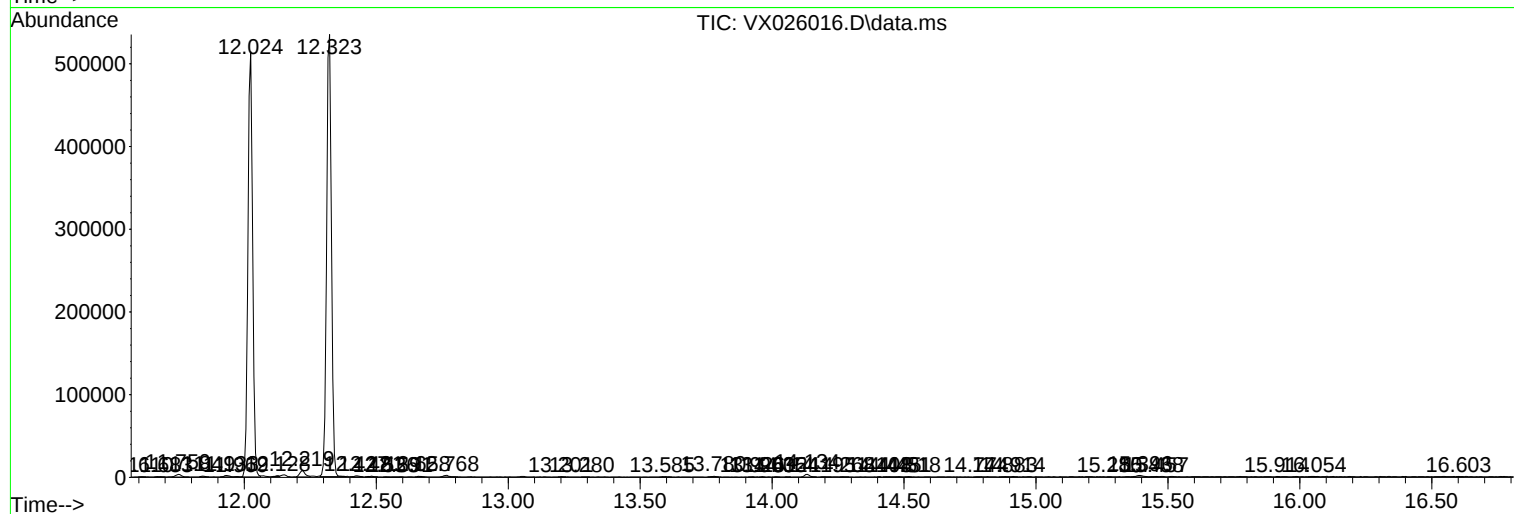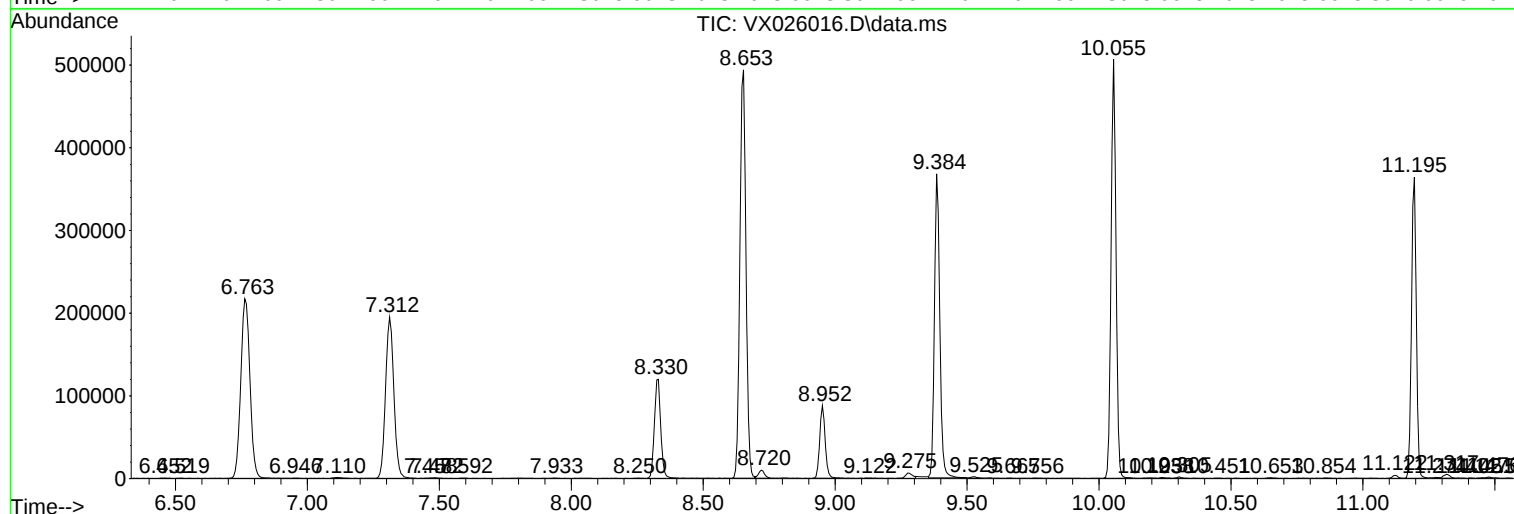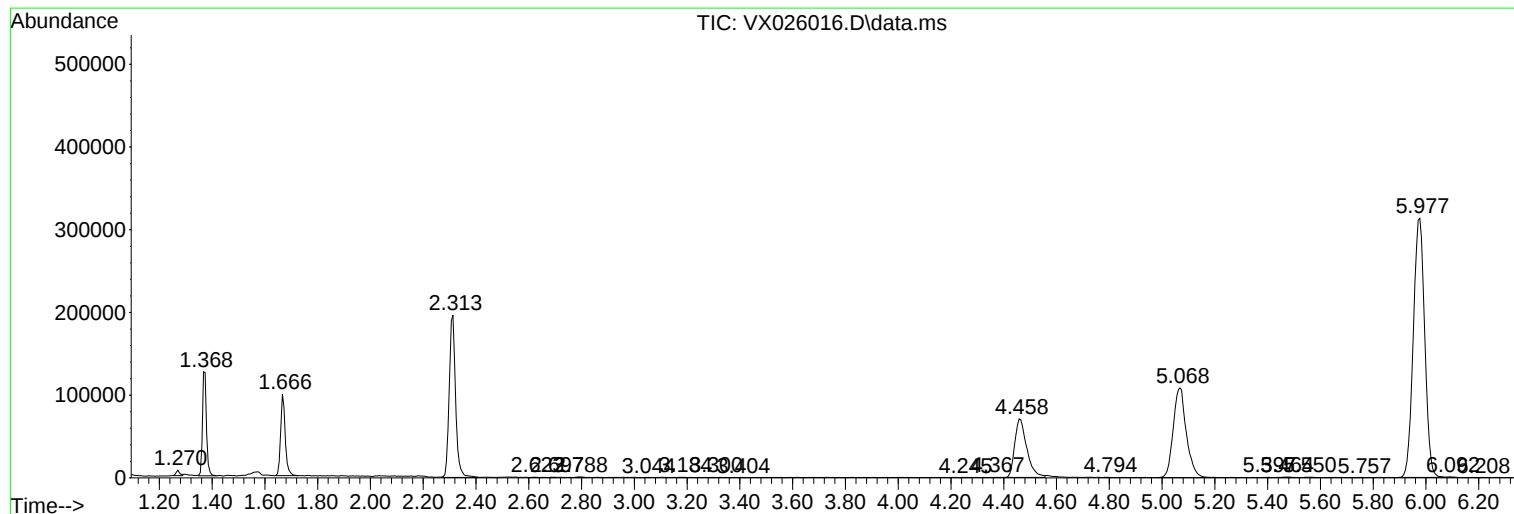

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122421\
Data File : VX026016.D
Acq On : 24 Dec 2021 15:46
Operator : JC/MD
Sample : M5126-17
Misc : 5.00mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J19

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122421\
Data File : VX026016.D
Acq On : 24 Dec 2021 15:46
Operator : JC/MD
Sample : M5126-17
Misc : 5.00mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J19

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------