

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122421\
 Data File : VX026017.D
 Acq On : 24 Dec 2021 16:09
 Operator : JC/MD
 Sample : M5126-18
 Misc : 5.00mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J27

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis

Signal : TIC: VX026017.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	56	rVB	123857	126157	13.44%	1.778%
2	1.666	91	95	104	rBV	96720	120800	12.87%	1.702%
3	2.312	194	201	211	rBV	190044	321191	34.23%	4.526%
4	2.703	262	265	272	rVB3	467	1016	0.11%	0.014%
5	2.794	272	280	284	rBV3	749	1659	0.18%	0.023%
6	3.111	330	332	335	rBV2	203	296	0.03%	0.004%
7	3.294	360	362	364	rVB2	307	277	0.03%	0.004%
8	3.611	412	414	416	rBV	233	198	0.02%	0.003%
9	3.757	435	438	440	rBB2	305	293	0.03%	0.004%
10	4.135	499	500	503	rBV2	328	208	0.02%	0.003%
11	4.233	511	516	518	rBV2	273	397	0.04%	0.006%
12	4.318	528	530	533	rVB2	184	215	0.02%	0.003%
13	4.349	533	535	538	rBV2	227	349	0.04%	0.005%
14	4.458	544	553	572	rBV2	72290	230723	24.59%	3.251%
15	4.660	584	586	590	rVB2	319	459	0.05%	0.006%
16	5.062	640	652	675	rBV2	108044	370580	39.49%	5.222%
17	5.294	688	690	693	rVB	198	201	0.02%	0.003%
18	5.385	703	705	706	rVV	281	232	0.02%	0.003%
19	5.403	706	708	709	rVV	445	265	0.03%	0.004%
20	5.544	729	731	732	rBV	248	222	0.02%	0.003%
21	5.623	741	744	746	rBV	198	244	0.03%	0.003%
22	5.976	789	802	818	rBV2	316338	938388	100.00%	13.222%
23	6.153	829	831	835	rVB2	232	212	0.02%	0.003%
24	6.220	841	842	846	rBV2	264	269	0.03%	0.004%
25	6.373	866	867	870	rBV2	176	199	0.02%	0.003%
26	6.421	873	875	878	rVB2	206	231	0.02%	0.003%
27	6.464	878	882	883	rBV2	208	254	0.03%	0.004%
28	6.604	902	905	906	rBV	249	245	0.03%	0.003%
29	6.763	920	931	946	rBV	225737	540677	57.62%	7.618%
30	7.110	984	988	995	rVB3	1084	2278	0.24%	0.032%
31	7.202	1001	1003	1007	rVB2	242	215	0.02%	0.003%
32	7.232	1007	1008	1011	rBV3	189	225	0.02%	0.003%
33	7.312	1011	1021	1039	rVV	199617	429990	45.82%	6.059%
34	7.488	1045	1050	1054	rVB3	597	1110	0.12%	0.016%
35	7.811	1102	1103	1106	rVB	440	331	0.04%	0.005%
36	7.921	1118	1121	1122	rBV2	286	292	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122421\
 Data File : VX026017.D
 Acq On : 24 Dec 2021 16:09
 Operator : JC/MD
 Sample : M5126-18
 Misc : 5.00mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J27

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis

37	8.055	1139	1143	1146	rVB2	289	259	0.03%	0.004%
38	8.141	1155	1157	1160	rBV2	194	235	0.03%	0.003%
39	8.330	1181	1188	1200	rBV	119590	200080	21.32%	2.819%
40	8.476	1210	1212	1215	rBV2	331	442	0.05%	0.006%
41	8.586	1227	1230	1233	rBV3	396	538	0.06%	0.008%
42	8.653	1233	1241	1248	rBV	477237	762065	81.21%	10.738%
43	8.720	1248	1252	1259	rVV	8059	13115	1.40%	0.185%
44	8.775	1259	1261	1263	rVB2	365	274	0.03%	0.004%
45	8.805	1263	1266	1268	rBV2	505	575	0.06%	0.008%
46	8.951	1284	1290	1301	rBV	82946	120560	12.85%	1.699%
47	9.061	1306	1308	1314	rVB2	312	260	0.03%	0.004%
48	9.110	1314	1316	1317	rBV2	217	206	0.02%	0.003%
49	9.214	1330	1333	1335	rVB	244	241	0.03%	0.003%
50	9.281	1338	1344	1349	rBV	6352	11607	1.24%	0.164%
51	9.384	1356	1361	1379	rVB	349886	499181	53.20%	7.034%
52	9.634	1401	1402	1406	rVB2	401	318	0.03%	0.004%
53	9.671	1406	1408	1409	rBV	246	193	0.02%	0.003%
54	9.848	1434	1437	1439	rBV2	193	281	0.03%	0.004%
55	9.982	1458	1459	1462	rBV	371	230	0.02%	0.003%
56	10.055	1465	1471	1481	rBV	473900	630269	67.17%	8.881%
57	10.195	1489	1494	1497	rBV3	634	904	0.10%	0.013%
58	10.250	1497	1503	1505	rVB3	710	1090	0.12%	0.015%
59	10.299	1505	1511	1517	rBV4	1456	2163	0.23%	0.030%
60	10.470	1537	1539	1542	rVB	267	249	0.03%	0.004%
61	10.640	1562	1567	1573	rVB4	657	1425	0.15%	0.020%
62	10.957	1617	1619	1626	rVB2	328	562	0.06%	0.008%
63	11.122	1642	1646	1651	rBV2	3228	4429	0.47%	0.062%
64	11.195	1652	1658	1667	rBV	351081	450868	48.05%	6.353%
65	11.317	1674	1678	1683	rVB	4778	7232	0.77%	0.102%
66	11.384	1686	1689	1691	rBV2	322	393	0.04%	0.006%
67	11.616	1726	1727	1730	rVV2	277	236	0.03%	0.003%
68	11.646	1730	1732	1734	rVB2	341	209	0.02%	0.003%
69	11.677	1734	1737	1739	rBV2	418	423	0.05%	0.006%
70	11.750	1745	1749	1754	rVB2	3207	4328	0.46%	0.061%
71	11.847	1761	1765	1767	rVB2	620	646	0.07%	0.009%
72	11.933	1775	1779	1783	rBV3	1592	2321	0.25%	0.033%
73	11.969	1784	1785	1789	rBV3	337	362	0.04%	0.005%
74	12.024	1789	1794	1807	rVB	508516	612352	65.26%	8.628%
75	12.128	1807	1811	1812	rBV3	1169	1299	0.14%	0.018%
76	12.219	1821	1826	1832	rBV	10018	14811	1.58%	0.209%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122421\
 Data File : VX026017.D
 Acq On : 24 Dec 2021 16:09
 Operator : JC/MD
 Sample : M5126-18
 Misc : 5.00mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J27

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
 Title : VOC Analysis

77	12.323	1836	1843	1850	rBV	519207	642553	68.47%	9.054%
78	12.475	1865	1868	1870	rBV2	1060	1028	0.11%	0.014%
79	12.573	1882	1884	1887	rVB2	240	215	0.02%	0.003%
80	12.609	1887	1890	1891	rBV2	308	279	0.03%	0.004%
81	12.628	1891	1893	1894	rVV	407	250	0.03%	0.004%
82	12.768	1909	1916	1920	rVB2	2100	3059	0.33%	0.043%
83	12.859	1929	1931	1934	rBV2	450	514	0.05%	0.007%
84	13.054	1958	1963	1966	rVB4	674	892	0.10%	0.013%
85	13.213	1987	1989	1991	rBV	249	306	0.03%	0.004%
86	13.414	2020	2022	2024	rBV2	243	225	0.02%	0.003%
87	13.438	2024	2026	2030	rVV	214	214	0.02%	0.003%
88	13.597	2049	2052	2053	rBV2	548	513	0.05%	0.007%
89	13.780	2079	2082	2084	rVV2	666	655	0.07%	0.009%
90	13.920	2104	2105	2107	rBV2	229	243	0.03%	0.003%
91	14.103	2130	2135	2136	rBV2	225	335	0.04%	0.005%
92	14.133	2136	2140	2143	rVB2	2363	3111	0.33%	0.044%
93	14.201	2148	2151	2156	rVV	246	345	0.04%	0.005%
94	14.865	2259	2260	2261	rBV	332	197	0.02%	0.003%
95	15.109	2298	2300	2303	rBV2	457	590	0.06%	0.008%
96	15.389	2343	2346	2350	rBV2	1613	2080	0.22%	0.029%
97	15.523	2366	2368	2370	rBV2	481	354	0.04%	0.005%
98	15.700	2396	2397	2400	rVB2	457	431	0.05%	0.006%
99	15.731	2400	2402	2404	rBV2	343	311	0.03%	0.004%
100	16.090	2460	2461	2465	rVB2	384	301	0.03%	0.004%


Sum of corrected areas: 7097130

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122421\
Data File : VX026017.D
Acq On : 24 Dec 2021 16:09
Operator : JC/MD
Sample : M5126-18
Misc : 5.00mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

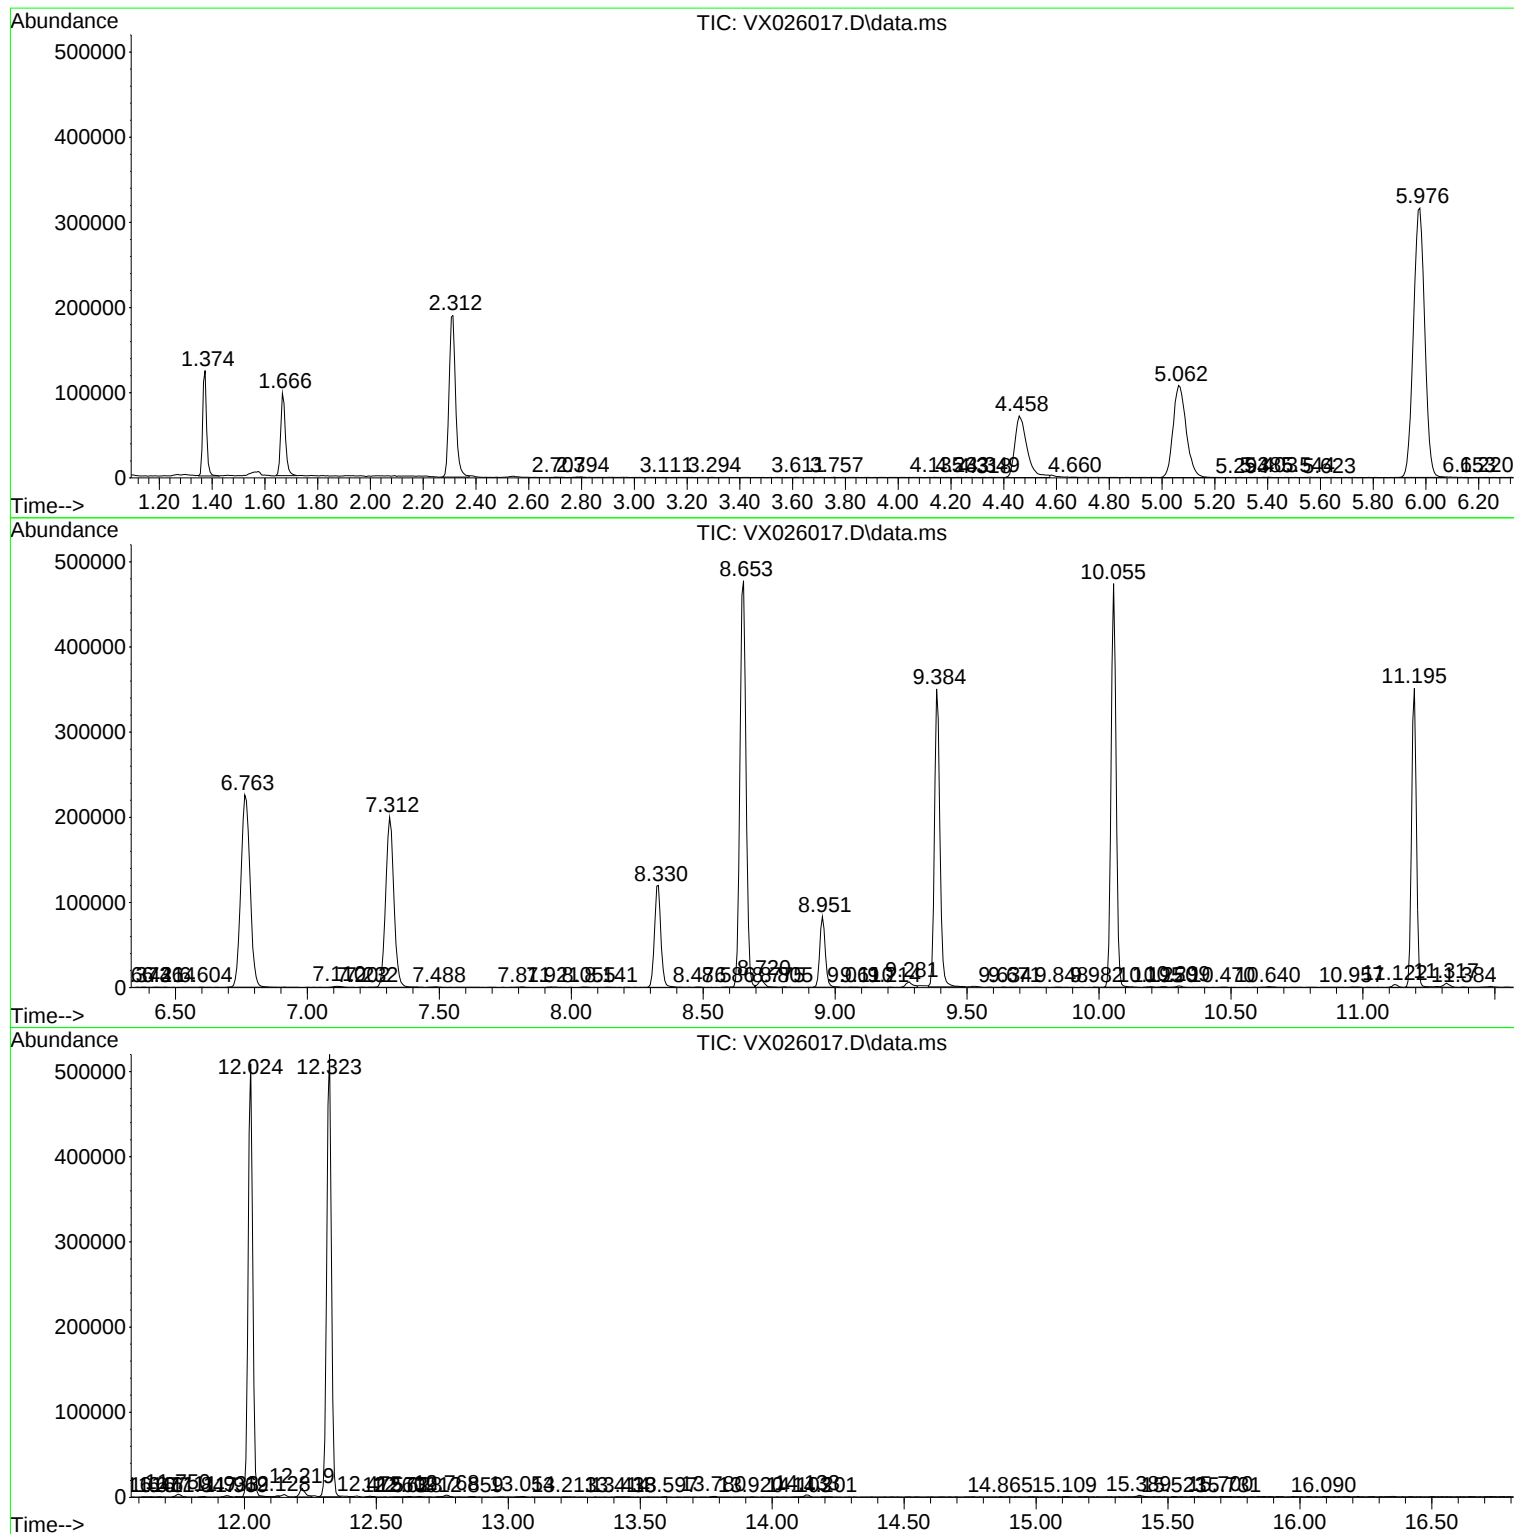

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122421\
Data File : VX026017.D
Acq On : 24 Dec 2021 16:09
Operator : JC/MD
Sample : M5126-18
Misc : 5.00mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122421\
Data File : VX026017.D
Acq On : 24 Dec 2021 16:09
Operator : JC/MD
Sample : M5126-18
Misc : 5.00mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
