

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122421\
 Data File : VX026023.D
 Acq On : 24 Dec 2021 18:29
 Operator : JC/MD
 Sample : M5150-15DL 20X
 Misc : 5.00mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBX3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
 Title : VOC Analysis

Signal : TIC: VX026023.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	24	27	32	rBV	11241	11482	1.20%	0.153%
2	1.374	43	47	55	rVB	124973	124501	13.05%	1.657%
3	1.666	91	95	106	rVB	92398	121181	12.70%	1.613%
4	2.312	194	201	210	rBV	192050	313297	32.84%	4.169%
5	2.794	276	280	288	rVB3	2516	3959	0.41%	0.053%
6	2.904	296	298	299	rBV2	285	216	0.02%	0.003%
7	2.928	299	302	304	rBV	136	177	0.02%	0.002%
8	3.007	311	315	316	rBV	303	277	0.03%	0.004%
9	3.099	328	330	332	rBV	195	209	0.02%	0.003%
10	3.123	332	334	336	rVV	275	183	0.02%	0.002%
11	3.190	343	345	347	rBV	321	235	0.02%	0.003%
12	3.513	397	398	399	rBV	335	164	0.02%	0.002%
13	3.769	438	440	442	rVV	225	204	0.02%	0.003%
14	3.897	457	461	464	rBV2	210	321	0.03%	0.004%
15	4.001	476	478	479	rBV	295	176	0.02%	0.002%
16	4.141	497	501	502	rBV2	224	220	0.02%	0.003%
17	4.379	538	540	543	rBV2	184	241	0.03%	0.003%
18	4.458	543	553	566	rBV	74716	224495	23.53%	2.987%
19	4.696	590	592	593	rBV2	246	157	0.02%	0.002%
20	4.910	625	627	628	rBV	236	166	0.02%	0.002%
21	4.977	636	638	639	rVB	275	170	0.02%	0.002%
22	5.068	639	653	671	rBV2	121962	377122	39.53%	5.018%
23	5.251	682	683	686	rBV2	251	255	0.03%	0.003%
24	5.348	697	699	702	rVB2	186	196	0.02%	0.003%
25	5.598	738	740	743	rVB2	293	212	0.02%	0.003%
26	5.629	743	745	748	rBV2	185	173	0.02%	0.002%
27	5.696	755	756	758	rBV	234	167	0.02%	0.002%
28	5.976	784	802	818	rBV2	319163	954134	100.00%	12.697%
29	6.123	825	826	829	rVB3	321	238	0.02%	0.003%
30	6.171	833	834	838	rVB	273	220	0.02%	0.003%
31	6.220	840	842	843	rVB	353	180	0.02%	0.002%
32	6.299	853	855	857	rVB2	194	169	0.02%	0.002%
33	6.324	857	859	860	rBV2	201	179	0.02%	0.002%
34	6.373	865	867	869	rBV2	203	204	0.02%	0.003%
35	6.421	873	875	878	rBV2	153	180	0.02%	0.002%
36	6.525	888	892	893	rBV	230	285	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122421\
 Data File : VX026023.D
 Acq On : 24 Dec 2021 18:29
 Operator : JC/MD
 Sample : M5150-15DL 20X
 Misc : 5.00mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBX3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis

37	6.556	893	897	899	rVB	203	265	0.03%	0.004%
38	6.580	899	901	904	rBV2	179	200	0.02%	0.003%
39	6.763	922	931	945	rBV	219233	519823	54.48%	6.917%
40	7.019	970	973	974	rBV	273	218	0.02%	0.003%
41	7.074	980	982	983	rBV	293	255	0.03%	0.003%
42	7.129	983	991	1001	rBV	157032	344041	36.06%	4.578%
43	7.312	1010	1021	1034	rBV	198128	432144	45.29%	5.751%
44	7.458	1042	1045	1047	rBV2	243	352	0.04%	0.005%
45	7.482	1047	1049	1054	rVV3	655	746	0.08%	0.010%
46	7.769	1093	1096	1099	rVB2	173	186	0.02%	0.002%
47	7.805	1099	1102	1106	rBV3	574	734	0.08%	0.010%
48	7.842	1106	1108	1110	rVB	361	245	0.03%	0.003%
49	7.915	1118	1120	1121	rBV2	299	268	0.03%	0.004%
50	8.055	1139	1143	1147	rVV2	234	331	0.03%	0.004%
51	8.202	1166	1167	1170	rBV2	235	229	0.02%	0.003%
52	8.330	1181	1188	1198	rBV	118320	196702	20.62%	2.618%
53	8.476	1210	1212	1213	rBV	327	238	0.02%	0.003%
54	8.567	1224	1227	1234	rBV3	526	863	0.09%	0.011%
55	8.653	1234	1241	1248	rBV	486908	752502	78.87%	10.014%
56	8.720	1248	1252	1259	rVB2	7400	11816	1.24%	0.157%
57	8.951	1284	1290	1297	rBV	81897	119526	12.53%	1.591%
58	9.281	1337	1344	1348	rBV3	6435	12264	1.29%	0.163%
59	9.384	1356	1361	1378	rVB	354601	497264	52.12%	6.617%
60	9.774	1423	1425	1428	rBV	314	234	0.02%	0.003%
61	9.945	1449	1453	1454	rVB2	344	255	0.03%	0.003%
62	10.055	1465	1471	1484	rBV	481142	638397	66.91%	8.495%
63	10.177	1489	1491	1492	rVV	332	245	0.03%	0.003%
64	10.201	1492	1495	1498	rVB	1383	1539	0.16%	0.020%
65	10.232	1498	1500	1501	rBV2	271	231	0.02%	0.003%
66	10.305	1507	1512	1517	rVB2	3268	5024	0.53%	0.067%
67	10.500	1542	1544	1547	rVV2	318	284	0.03%	0.004%
68	10.530	1547	1549	1552	rVV2	223	198	0.02%	0.003%
69	10.640	1564	1567	1569	rBV3	1074	1445	0.15%	0.019%
70	10.744	1580	1584	1586	rBV2	456	582	0.06%	0.008%
71	10.762	1586	1587	1590	rVV2	423	286	0.03%	0.004%
72	10.817	1593	1596	1598	rVB2	312	306	0.03%	0.004%
73	10.890	1607	1608	1612	rVB2	250	256	0.03%	0.003%
74	10.963	1618	1620	1623	rBV	937	886	0.09%	0.012%
75	10.988	1623	1624	1627	rVB	359	247	0.03%	0.003%
76	11.043	1630	1633	1635	rBV2	439	529	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122421\
 Data File : VX026023.D
 Acq On : 24 Dec 2021 18:29
 Operator : JC/MD
 Sample : M5150-15DL 20X
 Misc : 5.00mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBX3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
 Title : VOC Analysis

77	11.122	1635	1646	1650	rBV2	3407	5678	0.60%	0.076%
78	11.195	1652	1658	1667	rBV	351313	457251	47.92%	6.085%
79	11.317	1675	1678	1685	rVB3	5842	9155	0.96%	0.122%
80	11.384	1685	1689	1695	rBV5	1333	2411	0.25%	0.032%
81	11.481	1697	1705	1712	rBV10	2163	5944	0.62%	0.079%
82	11.616	1724	1727	1731	rVB4	653	980	0.10%	0.013%
83	11.677	1735	1737	1741	rVV4	727	928	0.10%	0.012%
84	11.719	1741	1744	1745	rVV2	709	698	0.07%	0.009%
85	11.750	1745	1749	1754	rVB3	5269	6917	0.72%	0.092%
86	11.823	1760	1761	1762	rBV	341	177	0.02%	0.002%
87	11.841	1762	1764	1766	rVV2	895	731	0.08%	0.010%
88	11.896	1771	1773	1775	rBV3	470	358	0.04%	0.005%
89	11.933	1776	1779	1783	rVB3	1670	1943	0.20%	0.026%
90	11.975	1783	1786	1788	rBV3	442	559	0.06%	0.007%
91	12.024	1788	1794	1802	rBV	521437	629074	65.93%	8.371%
92	12.146	1812	1814	1819	rVB3	2315	2827	0.30%	0.038%
93	12.274	1826	1835	1836	rBV5	1180	3422	0.36%	0.046%
94	12.323	1837	1843	1851	rVB	497755	656612	68.82%	8.738%
95	13.048	1960	1962	1965	rBV3	1449	1786	0.19%	0.024%
96	13.780	2078	2082	2086	rVB	11213	15443	1.62%	0.206%
97	14.133	2137	2140	2144	rVB	4979	5726	0.60%	0.076%
98	14.639	2220	2223	2232	rVB3	10919	19652	2.06%	0.262%
99	15.481	2358	2361	2367	rVB7	4311	7479	0.78%	0.100%
100	16.645	2550	2552	2553	rBV	1269	874	0.09%	0.012%




Sum of corrected areas: 7514726

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122421\
Data File : VX026023.D
Acq On : 24 Dec 2021 18:29
Operator : JC/MD
Sample : M5150-15DL 20X
Misc : 5.00mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBX3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

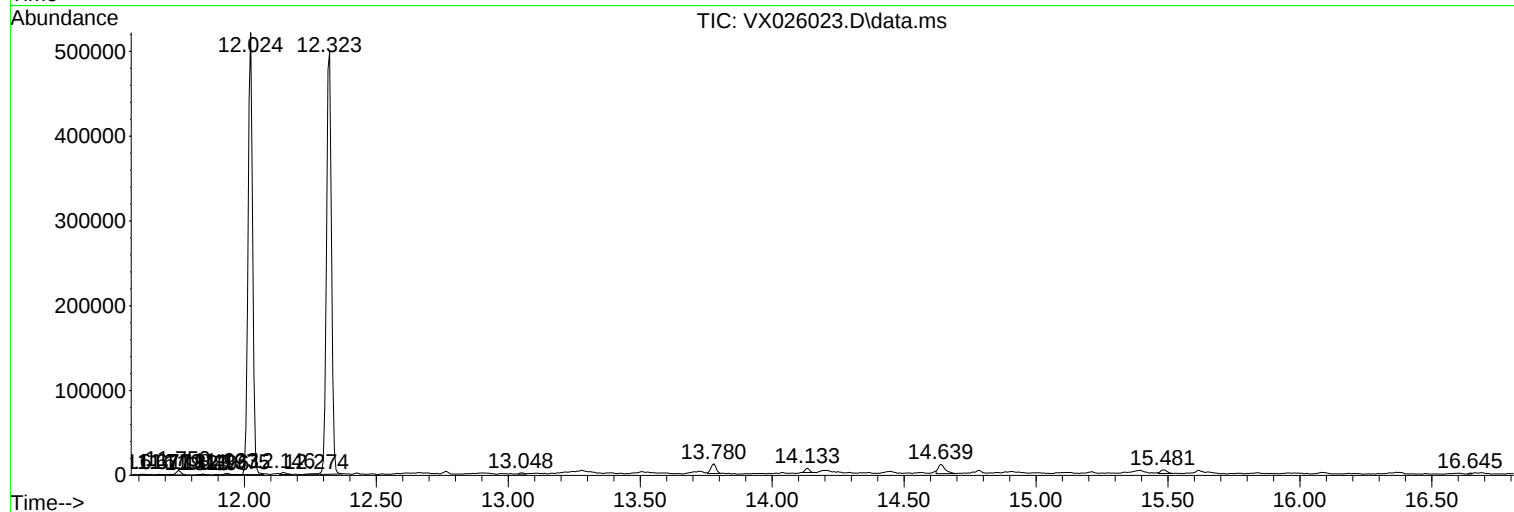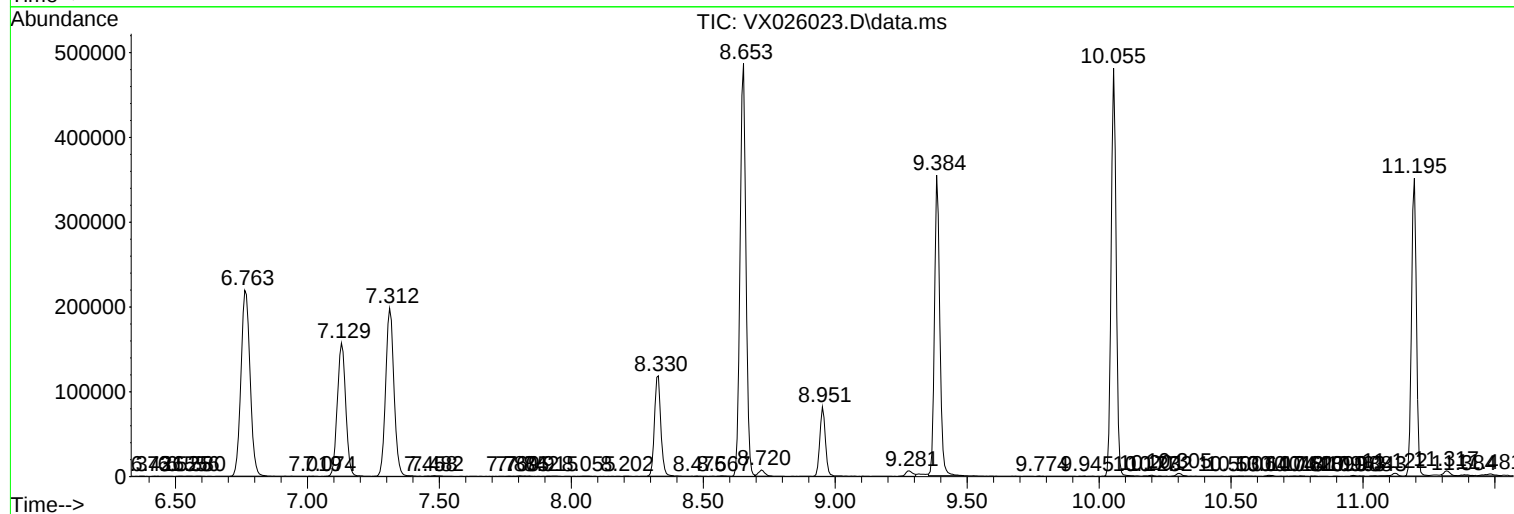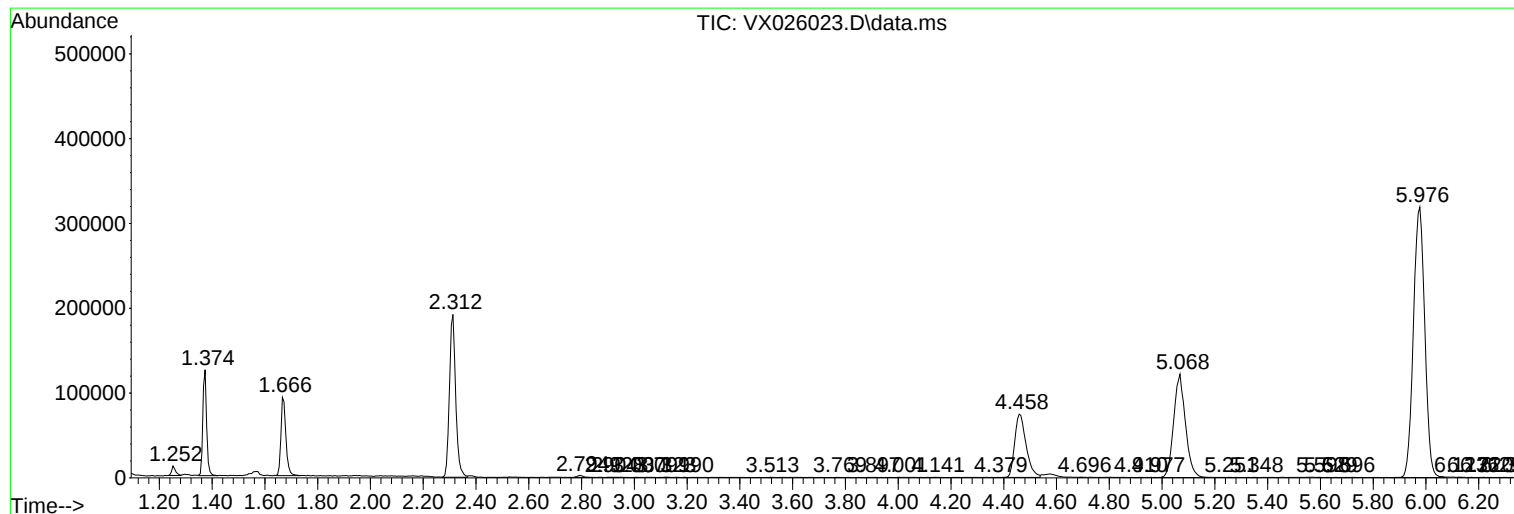

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122421\
Data File : VX026023.D
Acq On : 24 Dec 2021 18:29
Operator : JC/MD
Sample : M5150-15DL 20X
Misc : 5.00mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBX3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122421\
Data File : VX026023.D
Acq On : 24 Dec 2021 18:29
Operator : JC/MD
Sample : M5150-15DL 20X
Misc : 5.00mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBX3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc