

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122421\
 Data File : VX026024.D
 Acq On : 24 Dec 2021 18:52
 Operator : JC/MD
 Sample : M5150-21DL 40X
 Misc : 5.00mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBX9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M

Title : VOC Analysis

Signal : TIC: VX026024.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	25	27	32	rBV	6478	6137	0.66%	0.079%
2	1.374	43	47	54	rVB	131334	130860	14.14%	1.694%
3	1.666	91	95	105	rVB	92123	113641	12.28%	1.471%
4	2.313	194	201	211	rBV	186676	316305	34.18%	4.095%
5	2.514	230	234	237	rBV2	537	1096	0.12%	0.014%
6	2.544	237	239	242	rVB	830	761	0.08%	0.010%
7	2.709	263	266	270	rBV2	328	483	0.05%	0.006%
8	2.794	276	280	287	rVB5	2143	3480	0.38%	0.045%
9	3.001	313	314	318	rBV	294	338	0.04%	0.004%
10	3.093	324	329	335	rVV4	2334	4304	0.47%	0.056%
11	3.209	344	348	350	rBV2	177	270	0.03%	0.003%
12	3.257	354	356	358	rBV	230	259	0.03%	0.003%
13	3.507	395	397	400	rBV	354	264	0.03%	0.003%
14	3.550	400	404	407	rBB	233	324	0.04%	0.004%
15	3.709	426	430	431	rBV2	243	251	0.03%	0.003%
16	3.806	442	446	448	rBV	182	308	0.03%	0.004%
17	4.184	507	508	512	rVB2	269	274	0.03%	0.004%
18	4.239	515	517	520	rBV2	243	274	0.03%	0.004%
19	4.489	545	558	570	rBV3	133585	521654	56.38%	6.753%
20	4.745	598	600	603	rVB2	428	432	0.05%	0.006%
21	4.928	628	630	633	rBV2	207	265	0.03%	0.003%
22	4.971	633	637	639	rVV2	144	222	0.02%	0.003%
23	5.062	639	652	670	rVV	109184	368087	39.78%	4.765%
24	5.202	673	675	678	rVB2	391	286	0.03%	0.004%
25	5.495	719	723	727	rVB2	307	549	0.06%	0.007%
26	5.544	727	731	733	rBV2	417	681	0.07%	0.009%
27	5.733	757	762	764	rBV	266	322	0.03%	0.004%
28	5.788	767	771	774	rVB2	273	366	0.04%	0.005%
29	5.818	774	776	780	rBV2	238	283	0.03%	0.004%
30	5.977	788	802	819	rBV2	312307	925317	100.00%	11.979%
31	6.245	844	846	850	rBV	208	266	0.03%	0.003%
32	6.446	877	879	882	rBV	282	286	0.03%	0.004%
33	6.483	882	885	888	rBV2	247	276	0.03%	0.004%
34	6.763	921	931	947	rBV	218272	521864	56.40%	6.756%
35	7.019	970	973	976	rVB2	224	236	0.03%	0.003%
36	7.129	982	991	1007	rVB	173534	377893	40.84%	4.892%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122421\
 Data File : VX026024.D
 Acq On : 24 Dec 2021 18:52
 Operator : JC/MD
 Sample : M5150-21DL 40X
 Misc : 5.00mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBX9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
 Title : VOC Analysis

37	7.238	1007	1009	1011	rVB2	312	255	0.03%	0.003%
38	7.312	1011	1021	1033	rBV	191318	424742	45.90%	5.499%
39	7.458	1042	1045	1046	rBV2	288	272	0.03%	0.004%
40	7.799	1097	1101	1102	rBV	439	571	0.06%	0.007%
41	7.927	1120	1122	1126	rVV2	398	456	0.05%	0.006%
42	8.147	1157	1158	1161	rBV	267	245	0.03%	0.003%
43	8.257	1172	1176	1178	rBV	231	274	0.03%	0.004%
44	8.324	1181	1187	1196	rBV	113891	189956	20.53%	2.459%
45	8.476	1207	1212	1218	rVB3	429	716	0.08%	0.009%
46	8.580	1225	1229	1234	rVV2	394	611	0.07%	0.008%
47	8.653	1234	1241	1249	rVV	467894	751364	81.20%	9.727%
48	8.720	1249	1252	1261	rVB2	6564	10389	1.12%	0.134%
49	8.872	1276	1277	1280	rVB2	347	271	0.03%	0.004%
50	8.952	1284	1290	1303	rBV	80288	118131	12.77%	1.529%
51	9.202	1330	1331	1333	rVB	352	224	0.02%	0.003%
52	9.281	1338	1344	1348	rBV2	6344	11721	1.27%	0.152%
53	9.384	1356	1361	1379	rVB	353275	493925	53.38%	6.394%
54	9.592	1394	1395	1397	rBV	372	242	0.03%	0.003%
55	9.610	1397	1398	1401	rVV2	267	233	0.03%	0.003%
56	9.732	1413	1418	1421	rVB3	262	422	0.05%	0.005%
57	9.842	1435	1436	1441	rVV2	226	233	0.03%	0.003%
58	9.951	1451	1454	1458	rVB2	241	291	0.03%	0.004%
59	9.994	1458	1461	1462	rBV2	265	269	0.03%	0.003%
60	10.055	1465	1471	1487	rVV	488006	645248	69.73%	8.353%
61	10.165	1487	1489	1491	rVV2	256	235	0.03%	0.003%
62	10.201	1493	1495	1499	rVB3	863	865	0.09%	0.011%
63	10.305	1505	1512	1518	rBV4	1961	3149	0.34%	0.041%
64	10.646	1565	1568	1572	rBV4	572	815	0.09%	0.011%
65	10.805	1591	1594	1596	rBV2	148	228	0.02%	0.003%
66	10.963	1617	1620	1624	rVB2	437	614	0.07%	0.008%
67	11.012	1624	1628	1630	rBV2	364	356	0.04%	0.005%
68	11.122	1642	1646	1652	rVB3	2694	3974	0.43%	0.051%
69	11.195	1652	1658	1664	rBV	354515	445732	48.17%	5.771%
70	11.317	1674	1678	1684	rVB3	4444	7320	0.79%	0.095%
71	11.384	1684	1689	1690	rBV2	680	705	0.08%	0.009%
72	11.451	1699	1700	1702	rBV2	583	444	0.05%	0.006%
73	11.482	1702	1705	1708	rVV3	985	1129	0.12%	0.015%
74	11.549	1713	1716	1719	rVB2	420	383	0.04%	0.005%
75	11.677	1735	1737	1740	rVB2	510	414	0.04%	0.005%
76	11.713	1740	1743	1745	rVV3	387	598	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122421\
 Data File : VX026024.D
 Acq On : 24 Dec 2021 18:52
 Operator : JC/MD
 Sample : M5150-21DL 40X
 Misc : 5.00mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBX9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis

77	11.750	1745	1749	1757	rVB3	3924	5590	0.60%	0.072%
78	11.847	1763	1765	1768	rVB3	623	802	0.09%	0.010%
79	11.933	1776	1779	1783	rBV2	1534	1800	0.19%	0.023%
80	12.024	1788	1794	1800	rBV	520116	629041	67.98%	8.144%
81	12.152	1812	1815	1818	rVB3	2070	2179	0.24%	0.028%
82	12.256	1829	1832	1836	rBV4	454	733	0.08%	0.009%
83	12.323	1837	1843	1850	rVV	498265	638938	69.05%	8.272%
84	12.427	1857	1860	1864	rVB3	1313	1660	0.18%	0.021%
85	12.481	1864	1869	1876	rVV3	654	1105	0.12%	0.014%
86	12.536	1876	1878	1879	rVB	418	240	0.03%	0.003%
87	12.573	1881	1884	1885	rBV2	265	242	0.03%	0.003%
88	12.664	1895	1899	1901	rBV4	693	1064	0.11%	0.014%
89	12.762	1911	1915	1920	rBV2	2472	3748	0.41%	0.049%
90	13.055	1959	1963	1966	rBV4	640	1069	0.12%	0.014%
91	13.176	1981	1983	1987	rBV3	300	425	0.05%	0.006%
92	13.311	2003	2005	2009	rVB3	425	346	0.04%	0.004%
93	13.378	2013	2016	2020	rVB2	291	532	0.06%	0.007%
94	13.451	2024	2028	2029	rBV	258	239	0.03%	0.003%
95	13.524	2038	2040	2046	rVB4	538	746	0.08%	0.010%
96	13.682	2062	2066	2067	rBV	428	354	0.04%	0.005%
97	13.707	2068	2070	2072	rVV4	341	279	0.03%	0.004%
98	13.780	2078	2082	2086	rVB2	3363	4392	0.47%	0.057%
99	14.127	2136	2139	2144	rBV2	4216	6293	0.68%	0.081%
100	14.640	2218	2223	2230	rVB5	3202	5547	0.60%	0.072%

Sum of corrected areas: 7724300




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122421\
Data File : VX026024.D
Acq On : 24 Dec 2021 18:52
Operator : JC/MD
Sample : M5150-21DL 40X
Misc : 5.00mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBX9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

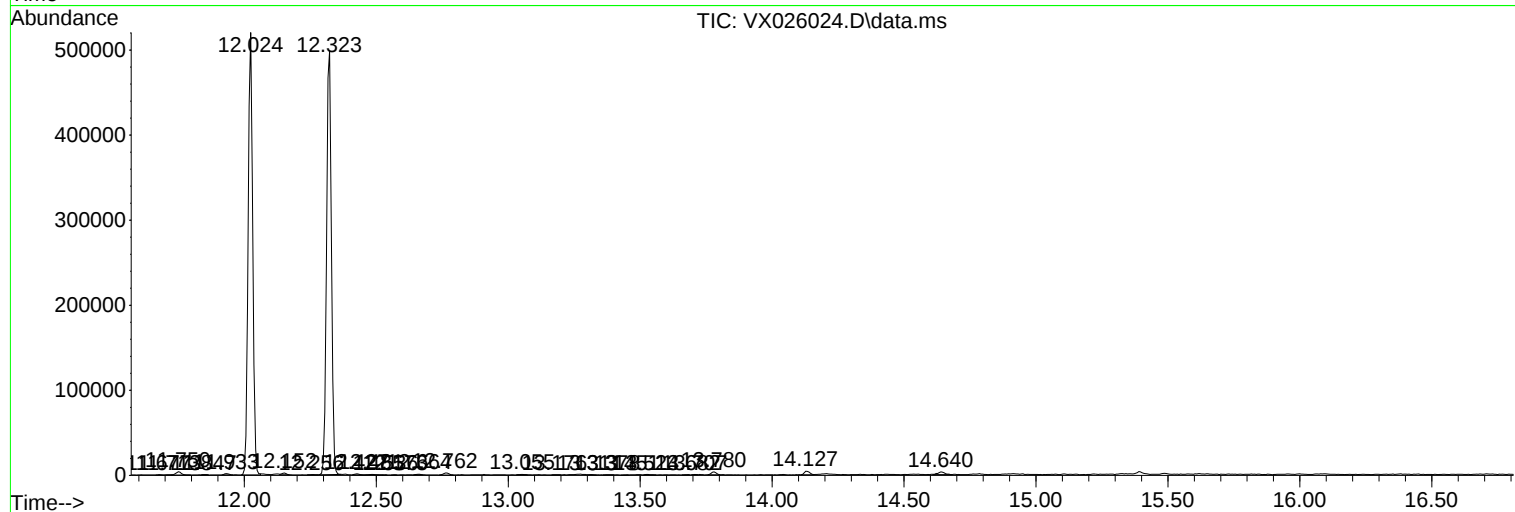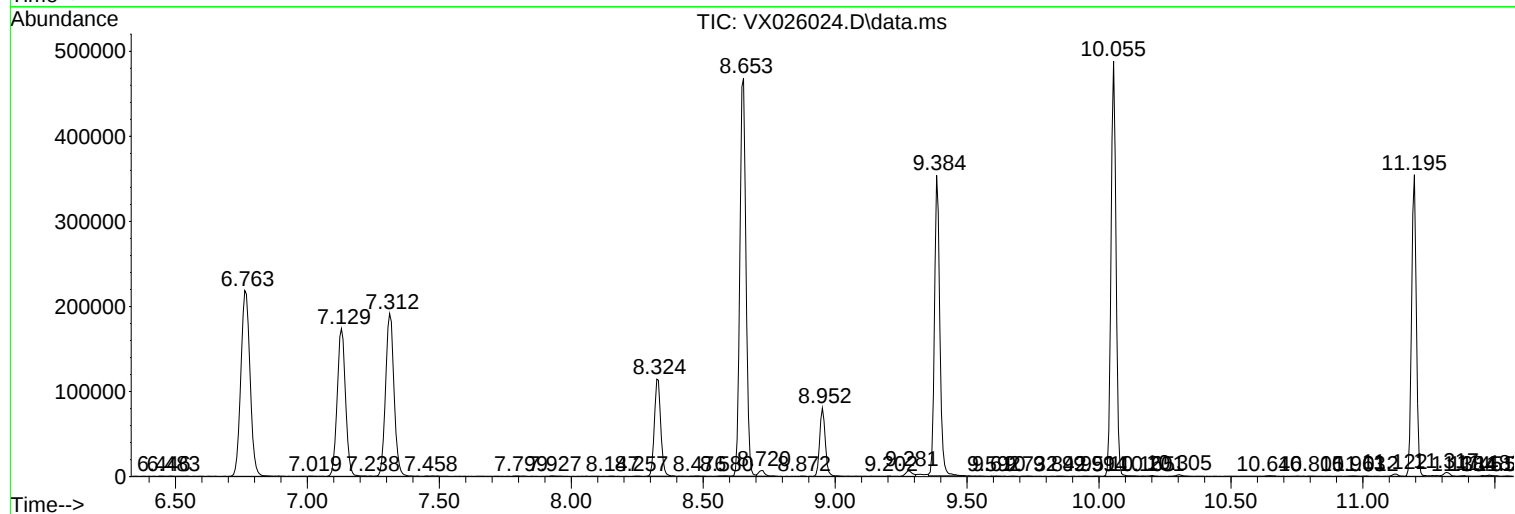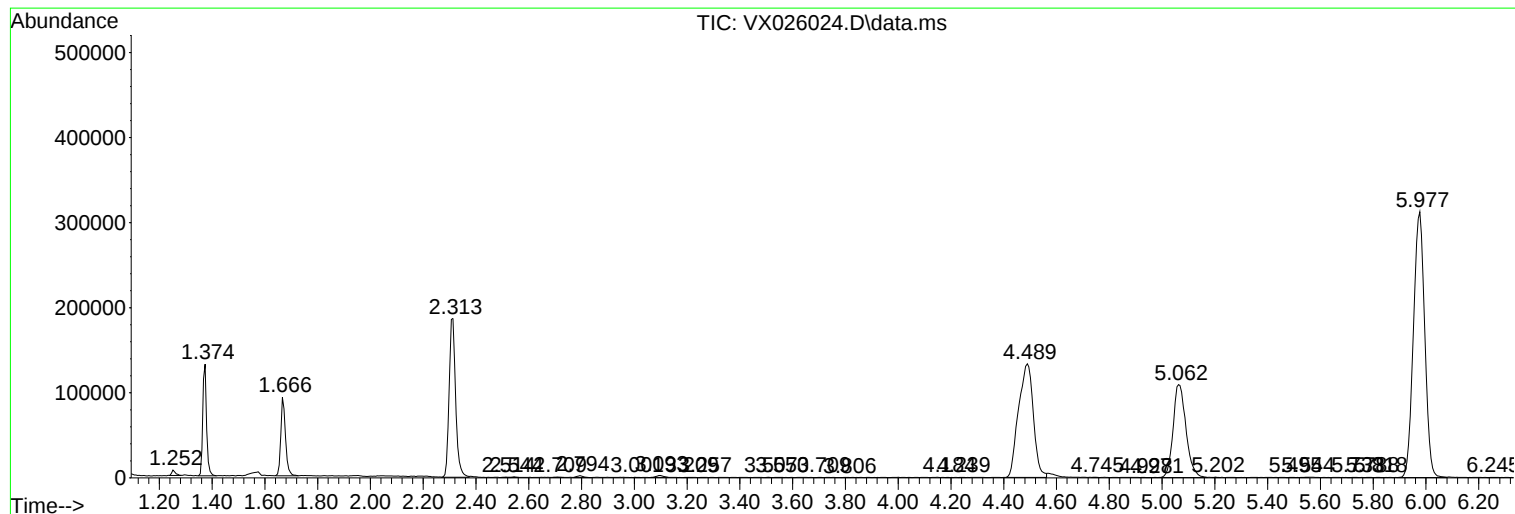

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122421\
Data File : VX026024.D
Acq On : 24 Dec 2021 18:52
Operator : JC/MD
Sample : M5150-21DL 40X
Misc : 5.00mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBX9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122421\
Data File : VX026024.D
Acq On : 24 Dec 2021 18:52
Operator : JC/MD
Sample : M5150-21DL 40X
Misc : 5.00mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBX9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------