

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122421\
 Data File : VX026026.D
 Acq On : 24 Dec 2021 19:39
 Operator : JC/MD
 Sample : M5126-10
 Misc : 5.00mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J14

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis

Signal : TIC: VX026026.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	53	rVB	108989	111721	12.80%	1.640%
2	1.666	91	95	105	rVB	87096	112595	12.90%	1.653%
3	2.313	194	201	210	rBV	186706	309966	35.52%	4.551%
4	2.502	231	232	233	rBV	449	249	0.03%	0.004%
5	2.532	235	237	246	rVB2	1192	2185	0.25%	0.032%
6	2.697	262	264	269	rBV2	400	480	0.06%	0.007%
7	2.794	276	280	284	rBV3	827	1440	0.17%	0.021%
8	2.959	302	307	310	rBV2	337	490	0.06%	0.007%
9	3.404	378	380	383	rVB2	219	233	0.03%	0.003%
10	3.495	394	395	398	rBV2	288	298	0.03%	0.004%
11	3.562	400	406	409	rBV2	187	312	0.04%	0.005%
12	3.611	409	414	422	rVB3	1800	3603	0.41%	0.053%
13	3.788	440	443	447	rVB	238	266	0.03%	0.004%
14	3.910	459	463	464	rVB2	189	241	0.03%	0.004%
15	4.007	475	479	482	rVB2	192	286	0.03%	0.004%
16	4.459	543	553	567	rBV	71149	212473	24.35%	3.119%
17	4.861	617	619	622	rBV2	169	218	0.02%	0.003%
18	5.062	640	652	669	rBV	114894	356781	40.89%	5.238%
19	5.397	697	707	716	rVB4	3846	10926	1.25%	0.160%
20	5.824	776	777	780	rBV2	208	224	0.03%	0.003%
21	5.977	789	802	818	rBV2	293773	872637	100.00%	12.812%
22	6.086	818	820	821	rBV2	586	380	0.04%	0.006%
23	6.452	878	880	882	rBV2	248	220	0.03%	0.003%
24	6.763	921	931	944	rBV	217333	517392	59.29%	7.596%
25	6.903	951	954	955	rVB3	245	255	0.03%	0.004%
26	7.013	970	972	975	rBV2	201	211	0.02%	0.003%
27	7.129	980	991	1001	rBV2	41491	91239	10.46%	1.340%
28	7.312	1012	1021	1034	rBV	182925	400346	45.88%	5.878%
29	7.434	1035	1041	1054	rVB2	11148	23543	2.70%	0.346%
30	7.806	1100	1102	1103	rBV2	336	310	0.04%	0.005%
31	7.927	1119	1122	1126	rBV4	602	1048	0.12%	0.015%
32	8.324	1179	1187	1198	rBV	107600	179805	20.60%	2.640%
33	8.470	1209	1211	1213	rBV2	425	483	0.06%	0.007%
34	8.537	1220	1222	1223	rBV2	235	229	0.03%	0.003%
35	8.653	1234	1241	1248	rBV	436561	691400	79.23%	10.151%
36	8.720	1249	1252	1263	rVB2	6460	10517	1.21%	0.154%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122421\
 Data File : VX026026.D
 Acq On : 24 Dec 2021 19:39
 Operator : JC/MD
 Sample : M5126-10
 Misc : 5.00mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J14

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis

37	8.952	1284	1290	1299	rBV	74967	109086	12.50%	1.602%
38	9.275	1338	1343	1349	rBV2	11622	19911	2.28%	0.292%
39	9.384	1356	1361	1372	rVB	329061	458264	52.51%	6.728%
40	9.519	1381	1383	1390	rVB4	1084	1837	0.21%	0.027%
41	9.836	1433	1435	1437	rBV2	222	219	0.03%	0.003%
42	9.903	1444	1446	1450	rBV2	290	308	0.04%	0.005%
43	10.006	1459	1463	1465	rBV2	258	335	0.04%	0.005%
44	10.055	1465	1471	1480	rVV	459855	621681	71.24%	9.127%
45	10.195	1492	1494	1498	rVB	422	457	0.05%	0.007%
46	10.244	1498	1502	1505	rVB2	986	1095	0.13%	0.016%
47	10.305	1508	1512	1515	rBV2	1586	1764	0.20%	0.026%
48	10.409	1528	1529	1532	rBV	289	248	0.03%	0.004%
49	10.500	1543	1544	1546	rBV2	262	235	0.03%	0.003%
50	10.646	1560	1568	1573	rBV5	607	1260	0.14%	0.018%
51	10.756	1583	1586	1588	rVB	300	243	0.03%	0.004%
52	10.774	1588	1589	1592	rBV2	209	258	0.03%	0.004%
53	10.878	1605	1606	1610	rVB	311	234	0.03%	0.003%
54	10.963	1618	1620	1623	rVB3	499	437	0.05%	0.006%
55	11.122	1642	1646	1650	rVB2	2308	2853	0.33%	0.042%
56	11.195	1652	1658	1667	rBV	328625	433570	49.69%	6.366%
57	11.317	1674	1678	1684	rVB2	6724	9765	1.12%	0.143%
58	11.457	1697	1701	1702	rBV4	495	660	0.08%	0.010%
59	11.476	1702	1704	1708	rVB3	843	1043	0.12%	0.015%
60	11.750	1745	1749	1753	rVB3	2578	3387	0.39%	0.050%
61	11.841	1762	1764	1767	rBV2	543	589	0.07%	0.009%
62	11.933	1775	1779	1782	rVB4	1193	1594	0.18%	0.023%
63	11.975	1782	1786	1788	rVB2	341	466	0.05%	0.007%
64	12.024	1788	1794	1806	rBV	473141	580763	66.55%	8.527%
65	12.219	1822	1826	1831	rVV2	5910	8395	0.96%	0.123%
66	12.323	1837	1843	1852	rVB	480199	609540	69.85%	8.949%
67	12.421	1857	1859	1865	rVB4	628	1037	0.12%	0.015%
68	12.475	1867	1868	1873	rVB4	531	587	0.07%	0.009%
69	12.597	1883	1888	1889	rBV2	443	514	0.06%	0.008%
70	12.664	1896	1899	1902	rVB2	437	424	0.05%	0.006%
71	12.768	1909	1916	1920	rBV	2958	4470	0.51%	0.066%
72	12.823	1923	1925	1927	rBV2	296	344	0.04%	0.005%
73	12.872	1929	1933	1936	rBV2	370	517	0.06%	0.008%
74	12.914	1939	1940	1942	rBV	321	205	0.02%	0.003%
75	13.055	1960	1963	1965	rBV3	616	604	0.07%	0.009%
76	13.201	1984	1987	1988	rBV2	283	253	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122421\
 Data File : VX026026.D
 Acq On : 24 Dec 2021 19:39
 Operator : JC/MD
 Sample : M5126-10
 Misc : 5.00mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J14

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
 Title : VOC Analysis

77	13.292	1999	2002	2004	rBV2	375	412	0.05%	0.006%
78	13.500	2035	2036	2040	rBV2	171	214	0.02%	0.003%
79	13.567	2045	2047	2052	rBV2	200	318	0.04%	0.005%
80	13.652	2059	2061	2065	rVV2	296	296	0.03%	0.004%
81	13.780	2078	2082	2089	rVB2	1252	1831	0.21%	0.027%
82	13.932	2105	2107	2108	rVB	490	330	0.04%	0.005%
83	13.963	2110	2112	2115	rVB2	347	298	0.03%	0.004%
84	13.993	2115	2117	2119	rBV2	289	285	0.03%	0.004%
85	14.134	2136	2140	2145	rVB	3458	4790	0.55%	0.070%
86	14.189	2148	2149	2152	rVB2	286	211	0.02%	0.003%
87	14.298	2164	2167	2168	rBV2	288	212	0.02%	0.003%
88	14.530	2201	2205	2206	rBV2	224	320	0.04%	0.005%
89	14.554	2208	2209	2212	rVV2	464	396	0.05%	0.006%
90	14.585	2212	2214	2216	rVV	426	267	0.03%	0.004%
91	14.640	2221	2223	2228	rVB3	877	1010	0.12%	0.015%
92	14.755	2241	2242	2244	rVB2	442	246	0.03%	0.004%
93	15.121	2301	2302	2306	rBV2	416	373	0.04%	0.005%
94	15.158	2306	2308	2309	rBV	348	281	0.03%	0.004%
95	15.298	2329	2331	2332	rBV2	534	391	0.04%	0.006%
96	15.396	2343	2347	2350	rBV2	1869	2609	0.30%	0.038%
97	15.457	2354	2357	2360	rBV3	495	626	0.07%	0.009%
98	15.700	2395	2397	2399	rBV	362	275	0.03%	0.004%
99	16.078	2456	2459	2461	rBV2	470	504	0.06%	0.007%
100	16.255	2487	2488	2489	rBV	466	242	0.03%	0.004%


Sum of corrected areas: 6811191

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122421\
Data File : VX026026.D
Acq On : 24 Dec 2021 19:39
Operator : JC/MD
Sample : M5126-10
Misc : 5.00mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J14

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

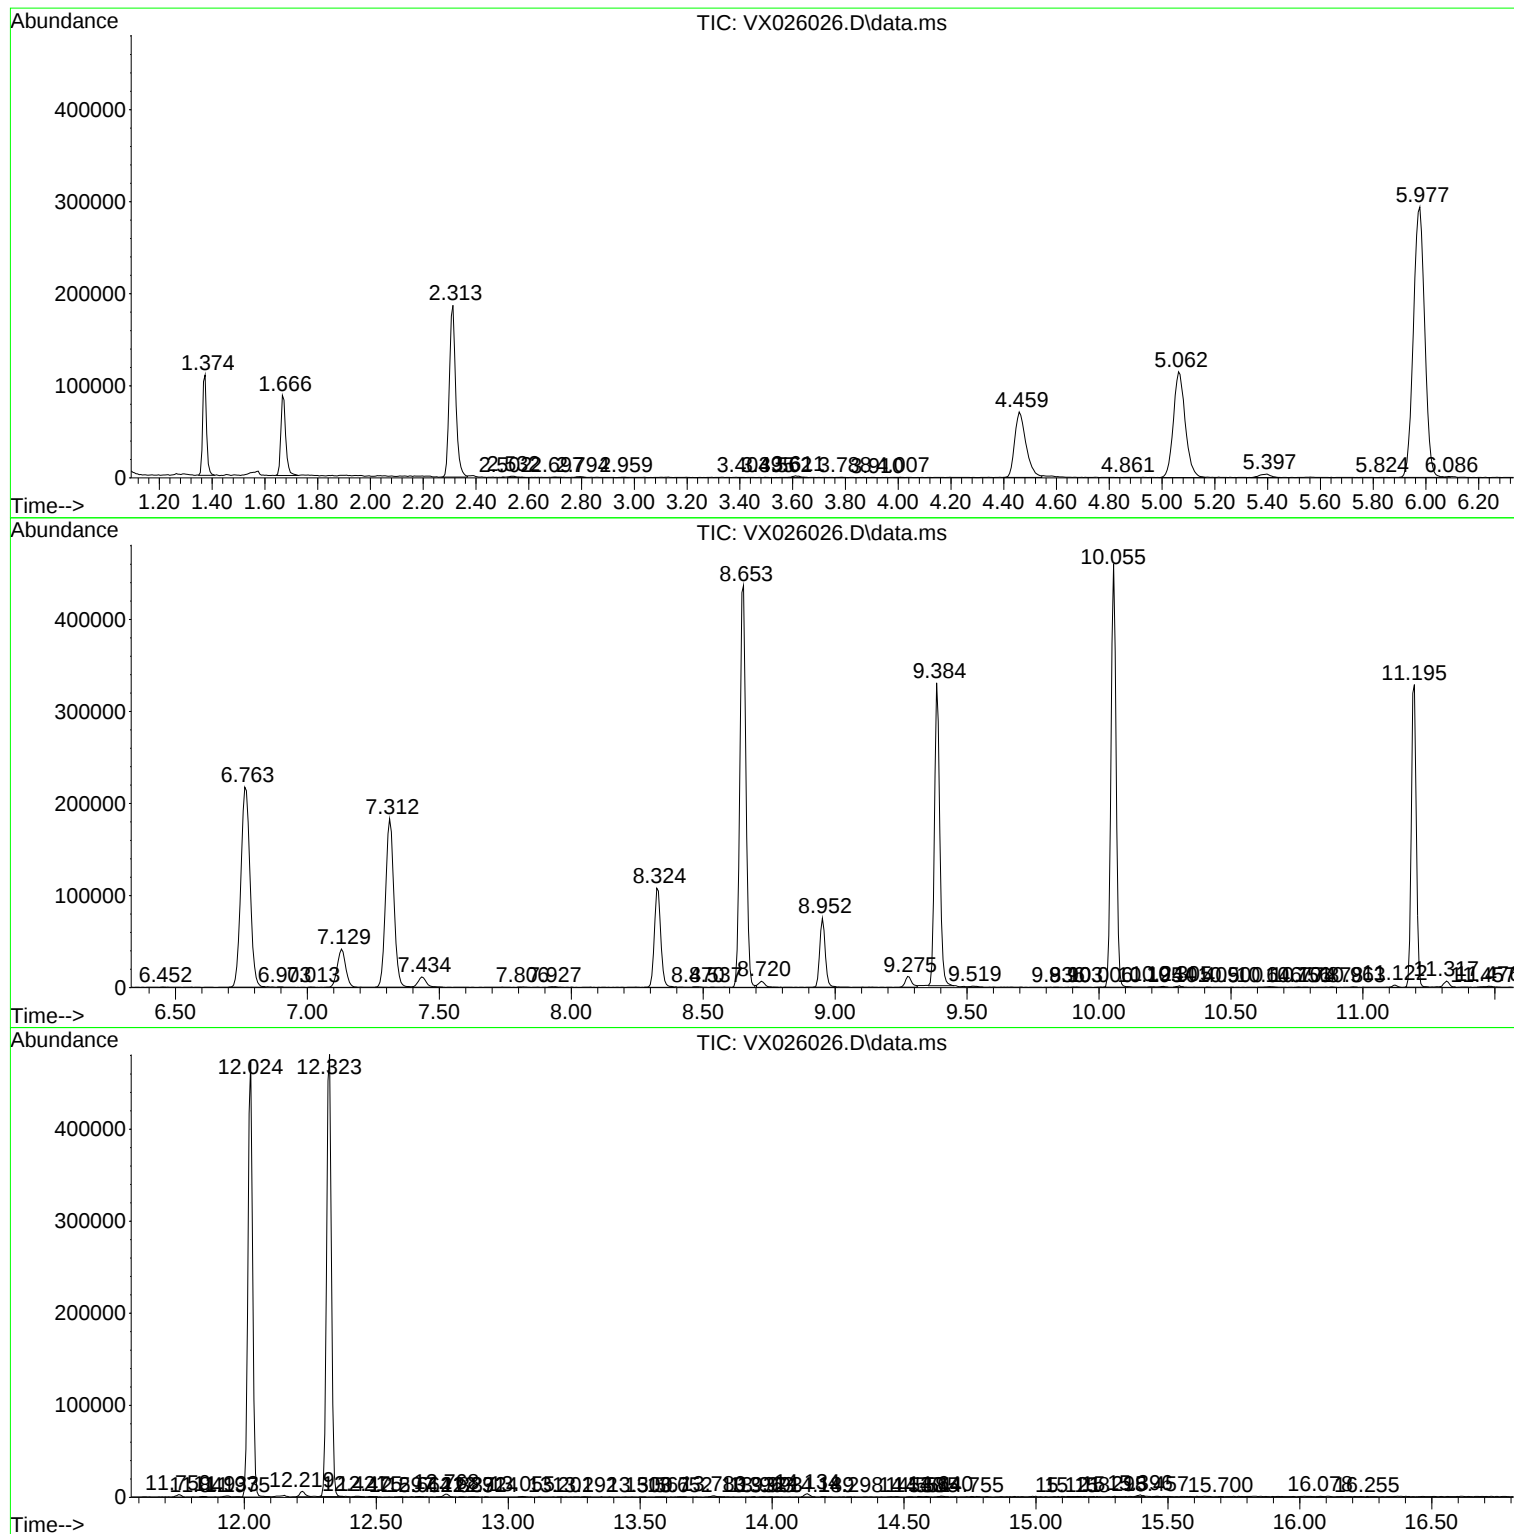

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122421\
Data File : VX026026.D
Acq On : 24 Dec 2021 19:39
Operator : JC/MD
Sample : M5126-10
Misc : 5.00mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J14

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122421\
Data File : VX026026.D
Acq On : 24 Dec 2021 19:39
Operator : JC/MD
Sample : M5126-10
Misc : 5.00mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J14

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------