


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122421\
 Data File : VX026007.D
 Acq On : 24 Dec 2021 09:41
 Operator : JC/MD
 Sample : BFB629
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB629

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis
 Last Update : Tue Dec 28 02:17:03 2021

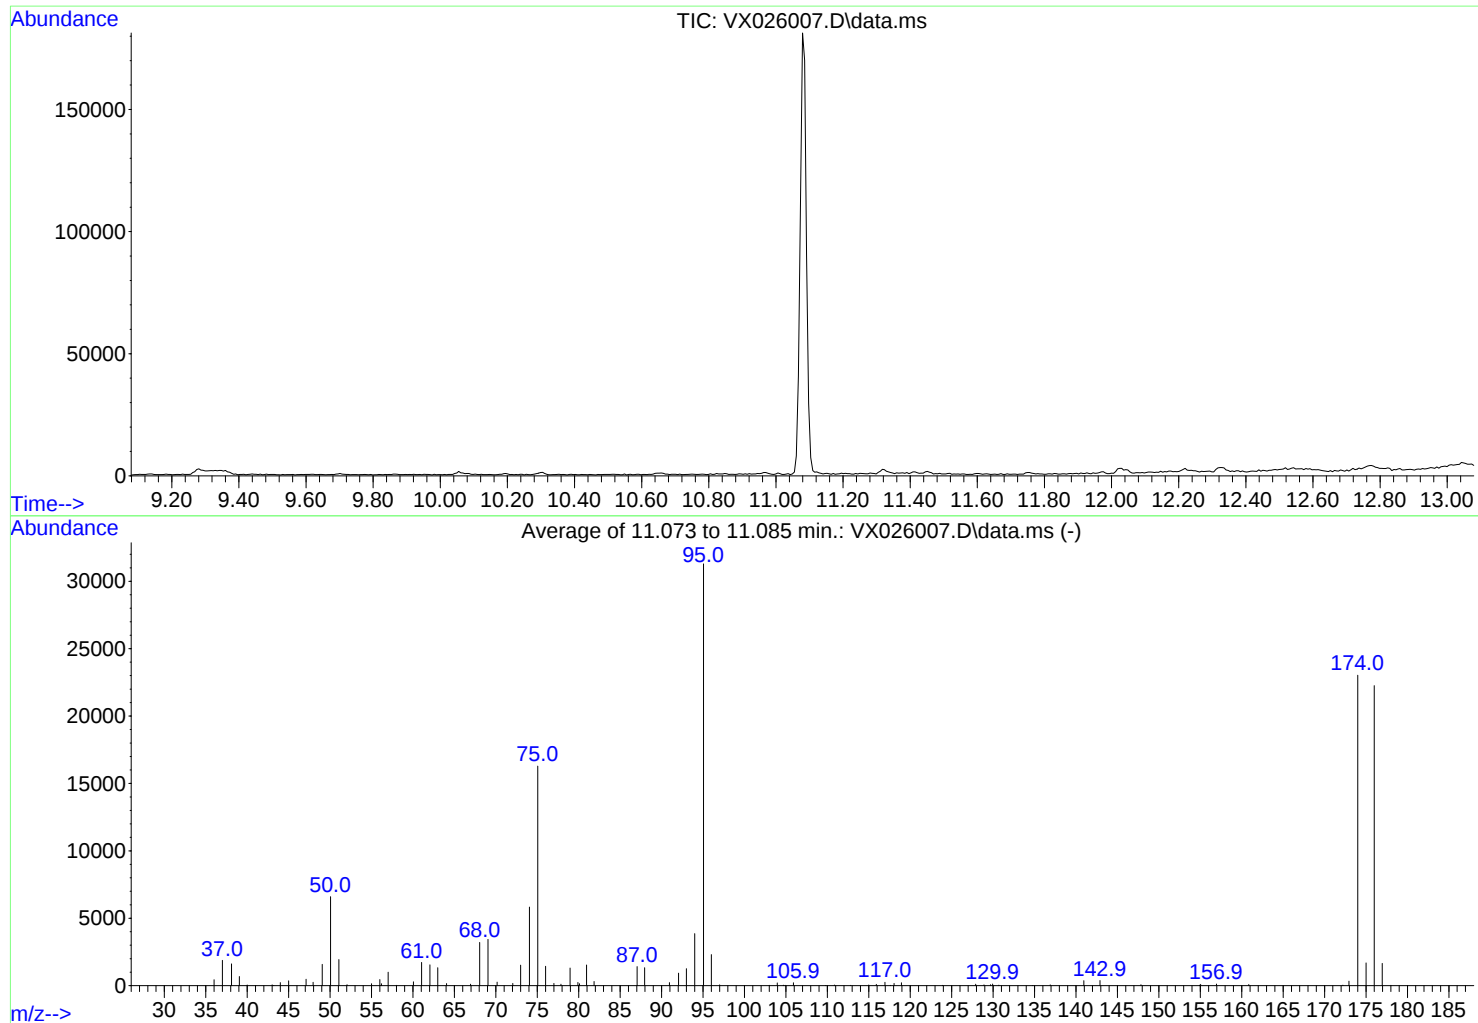

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	6602	PASS
75	95	30	80	52.0	16286	PASS
95	95	100	100	100.0	31293	PASS
96	95	5	9	7.4	2303	PASS
173	174	0.00	2	1.4	330	PASS
174	95	50	120	73.6	23032	PASS
175	174	5	9	7.3	1687	PASS
176	174	95	101	96.6	22256	PASS
177	176	5	9	7.4	1655	PASS

m/z	Abundance
40.00	323.0
44.00	199.0

Instrument :
MSVOA_X
ClientSampleId :
BFB629

m/z	Abundance
35.90	443.0
37.00	1873.0
38.10	1574.0
39.00	596.0
40.10	352.0
41.00	52.0
43.00	95.0
44.00	504.0
44.90	441.0
47.20	403.0
48.00	248.0
49.10	1617.0
50.00	6905.0
51.10	1748.0
52.10	56.0
55.00	122.0
56.20	440.0
57.00	956.0
60.00	251.0
61.00	1916.0
62.10	1736.0
63.00	1298.0
64.10	145.0
66.90	121.0
68.10	3377.0
69.10	3288.0
70.10	239.0
72.10	154.0
73.00	1464.0
74.10	5870.0
75.00	16736.0
76.00	1492.0
77.00	209.0
77.90	126.0
79.00	1403.0
80.10	426.0
81.00	1584.0
81.90	280.0
87.10	1457.0
87.90	1482.0
91.00	241.0
92.10	959.0
93.00	1494.0
94.00	4269.0
95.00	33512.0
96.00	2484.0
97.00	102.0
103.00	67.0
103.90	215.0
104.90	75.0
105.90	222.0
110.80	95.0
112.80	63.0
115.00	70.0
115.90	128.0
116.90	310.0
117.60	77.0
118.10	158.0
119.00	295.0
123.90	64.0
128.00	127.0
128.90	78.0
129.90	215.0
130.70	57.0
136.90	111.0
140.90	396.0
142.90	366.0
147.90	110.0
155.00	157.0
157.00	115.0
160.90	103.0
173.00	460.0
174.00	28520.0
175.00	2158.0
176.00	26936.0
177.00	1787.0

Instrument :
MSVOA_X
ClientSampleId :
BFB629

m/z	Abundance
36.00	344.0
37.00	1593.0
38.10	1300.0
39.10	641.0
40.00	413.0
43.00	75.0
44.00	348.0
45.10	267.0
47.00	475.0
47.90	228.0
49.00	1388.0
50.10	5136.0
51.10	1852.0
52.00	67.0
55.00	118.0
56.00	537.0
57.00	877.0
60.00	217.0
61.10	1305.0
62.00	1094.0
63.00	967.0
64.00	149.0
67.10	71.0
68.00	2426.0
69.00	2869.0
70.20	189.0
72.00	140.0
73.00	1208.0
74.00	4641.0
75.00	12753.0
76.00	1156.0
77.00	161.0
77.80	67.0
78.90	981.0
79.90	290.0
80.90	1202.0
81.90	287.0
87.00	1072.0
88.00	1067.0
90.90	205.0
92.10	601.0
93.00	974.0
94.00	2746.0
95.10	23552.0
96.00	1602.0
104.10	147.0
105.90	144.0
117.00	179.0
118.10	110.0
119.10	133.0
127.80	70.0
130.00	139.0
134.80	54.0
136.90	64.0
141.00	289.0
142.90	270.0
154.90	124.0
157.00	82.0
160.90	80.0
173.00	198.0
174.00	14089.0
175.00	1029.0
176.00	13721.0
177.00	1087.0

Instrument :
MSVOA_X
ClientSampleId :
BFB629

m/z	Abundance
36.10	524.0
37.00	2160.0
38.10	1977.0
39.10	811.0
40.00	334.0
43.20	54.0
44.00	432.0
45.00	371.0
47.10	553.0
48.00	278.0
49.10	1750.0
50.00	7765.0
51.00	2212.0
52.00	85.0
55.00	206.0
56.00	827.0
57.00	1177.0
58.00	64.0
60.10	390.0
61.00	1939.0
62.00	1786.0
63.00	1738.0
64.00	168.0
66.90	134.0
68.00	3816.0
69.00	4149.0
70.10	359.0
72.00	214.0
73.00	1894.0
74.00	6972.0
75.10	19368.0
76.00	1677.0
77.00	145.0
77.90	122.0
78.90	1522.0
79.90	409.0
80.90	1816.0
81.80	353.0
87.00	1706.0
87.90	1423.0
91.00	232.0
92.00	1208.0
93.00	1326.0
94.00	4566.0
95.00	36816.0
96.00	2822.0
97.00	68.0
103.90	247.0
104.70	97.0
105.90	289.0
109.80	56.0
111.00	56.0
115.00	56.0
115.90	156.0
117.00	252.0
118.00	218.0
118.90	228.0
127.90	114.0
128.90	103.0
129.70	197.0
130.70	56.0
141.00	418.0
142.90	507.0
147.80	101.0
155.10	132.0
156.90	151.0
160.80	62.0
172.20	99.0
172.90	333.0
174.00	26488.0
175.00	1874.0
176.00	26112.0
176.90	2092.0
178.00	83.0

Instrument :
MSVOA_X
ClientSampleId :
BFB629