
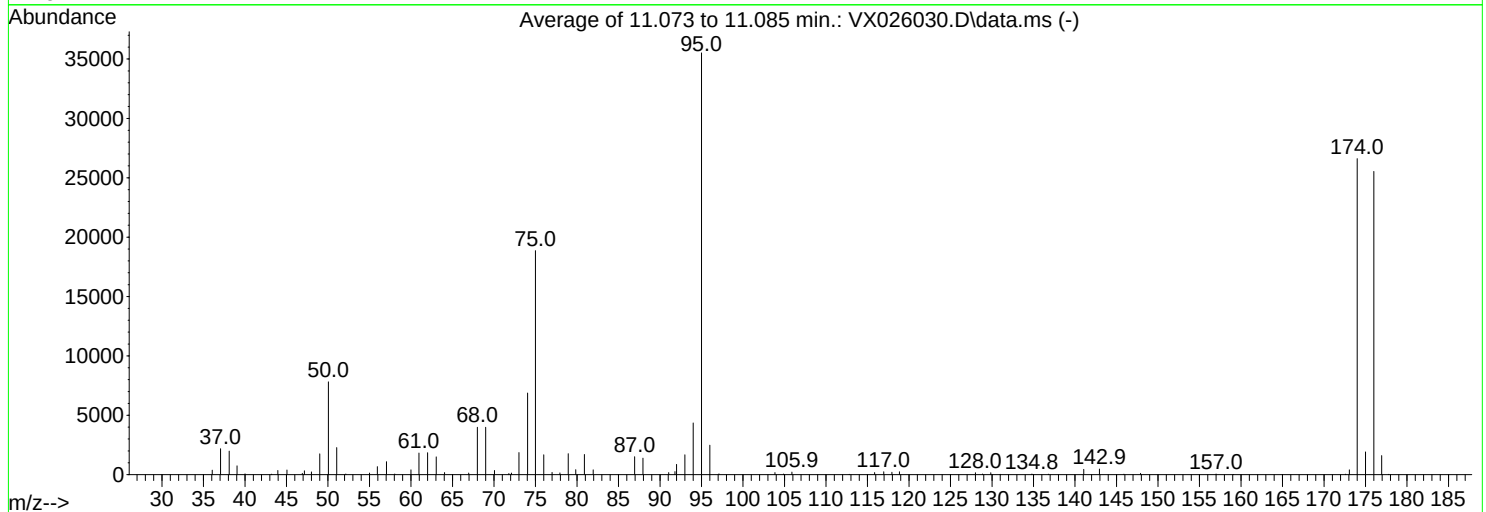


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122521\
 Data File : VX026030.D
 Acq On : 25 Dec 2021 10:52
 Operator : JC/MD
 Sample : BFB630
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB630

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis
 Last Update : Tue Dec 28 02:17:03 2021

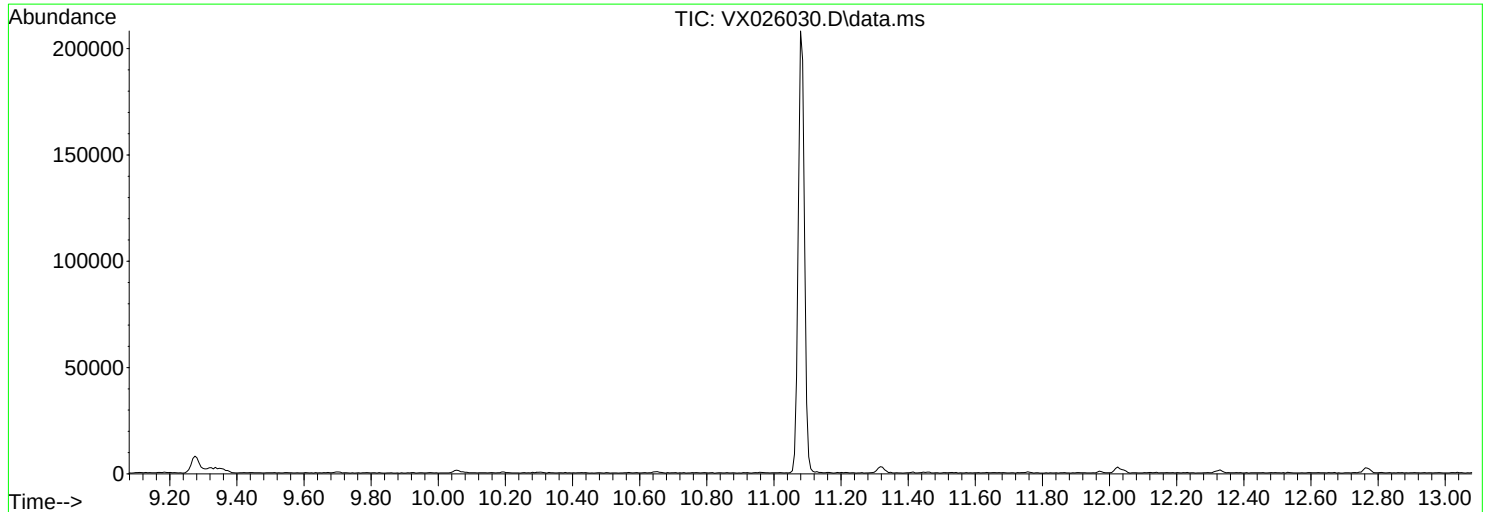

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.0	7811	PASS
75	95	30	80	53.1	18862	PASS
95	95	100	100	100.0	35520	PASS
96	95	5	9	7.0	2481	PASS
173	174	0.00	2	1.5	402	PASS
174	95	50	120	74.9	26613	PASS
175	174	5	9	7.2	1914	PASS
176	174	95	101	96.0	25541	PASS
177	176	5	9	6.3	1598	PASS

m/z	Abundance
40.00	316.0
43.80	164.0

Instrument :
MSVOA_X
ClientSampleId :
BFB630

m/z	Abundance
36.10	285.0
37.10	1639.0
38.10	1756.0
39.00	621.0
40.10	379.0
44.00	446.0
45.00	298.0
46.90	320.0
48.10	209.0
49.00	1515.0
50.00	6350.0
51.10	1781.0
55.00	83.0
56.00	503.0
57.00	964.0
58.10	59.0
60.00	347.0
61.00	1463.0
62.00	1496.0
63.10	1101.0
64.00	152.0
67.00	115.0
68.00	2971.0
69.00	3280.0
70.00	240.0
72.20	179.0
73.00	1415.0
74.10	5190.0
75.00	14793.0
76.00	1318.0
76.90	148.0
78.00	142.0
79.00	1201.0
79.90	294.0
80.90	1252.0
81.90	329.0
86.90	1394.0
87.90	907.0
91.10	94.0
91.80	770.0
93.00	1134.0
94.00	3261.0
95.00	26736.0
96.00	1729.0
97.10	67.0
104.00	66.0
105.90	155.0
115.90	137.0
117.10	176.0
117.90	102.0
118.90	172.0
128.00	93.0
128.80	81.0
129.80	140.0
141.00	310.0
142.90	355.0
172.60	109.0
173.10	232.0
174.00	16656.0
175.00	1249.0
176.00	15696.0
177.00	1060.0

Instrument :
MSVOA_X
ClientSampleId :
BFB630

m/z	Abundance
36.10	503.0
37.00	2647.0
38.10	2244.0
39.10	758.0
40.10	418.0
43.20	72.0
44.00	668.0
45.10	499.0
47.20	596.0
48.00	259.0
49.00	2041.0
50.00	9587.0
51.10	2951.0
52.20	84.0
55.00	207.0
55.90	792.0
57.10	1116.0
58.00	53.0
60.10	507.0
61.00	2109.0
62.00	2073.0
63.00	1839.0
64.00	212.0
66.90	144.0
68.00	4985.0
69.00	4676.0
70.00	394.0
72.00	221.0
73.00	2153.0
74.00	8182.0
75.00	22096.0
76.00	1969.0
77.00	263.0
78.00	163.0
78.90	2157.0
79.90	553.0
80.90	1981.0
82.00	479.0
87.00	1758.0
88.00	1598.0
91.00	245.0
92.00	1354.0
93.00	2050.0
94.00	5112.0
95.00	42032.0
96.00	3020.0
97.10	77.0
103.90	287.0
104.90	83.0
105.90	264.0
112.80	70.0
115.90	223.0
116.90	214.0
118.00	246.0
118.80	272.0
128.00	239.0
128.90	90.0
129.90	174.0
134.80	91.0
141.10	469.0
143.00	591.0
145.90	62.0
147.90	166.0
157.00	64.0
159.10	52.0
173.00	513.0
174.00	30560.0
175.00	2181.0
176.00	29488.0
176.90	1912.0
177.80	86.0

Instrument :
MSVOA_X
ClientSampleId :
BFB630

m/z	Abundance
36.00	359.0
37.00	2272.0
38.10	1937.0
39.00	835.0
40.00	362.0
43.20	56.0
44.00	442.0
45.00	362.0
47.10	368.0
47.90	224.0
49.00	1698.0
50.10	7497.0
51.00	2111.0
52.10	96.0
55.00	105.0
56.00	737.0
57.00	1211.0
58.00	64.0
59.90	358.0
60.90	1870.0
62.00	1956.0
63.00	1534.0
64.10	169.0
67.00	144.0
68.00	4000.0
69.00	4000.0
70.10	420.0
71.80	271.0
73.00	1994.0
74.00	7229.0
75.00	19696.0
76.00	1710.0
77.10	172.0
77.80	141.0
78.90	1958.0
79.80	403.0
80.90	1846.0
81.90	414.0
87.00	1374.0
88.00	1669.0
91.00	175.0
92.00	1230.0
93.00	1845.0
94.00	4672.0
95.00	37792.0
96.00	2693.0
97.10	74.0
103.80	171.0
104.90	64.0
105.90	229.0
115.80	166.0
116.90	350.0
117.90	248.0
118.90	284.0
128.00	151.0
129.90	163.0
131.00	70.0
134.80	79.0
136.80	116.0
141.00	541.0
142.90	454.0
145.90	72.0
147.90	156.0
157.00	94.0
173.00	460.0
174.00	32624.0
175.00	2311.0
176.00	31440.0
177.00	1822.0

Instrument :
MSVOA_X
ClientSampleId :
BFB630