

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122624\
 Data File : VX044495.D
 Acq On : 26 Dec 2024 09:21
 Operator : JC/MD
 Sample : VX1226MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Dec 27 03:38:14 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 27 03:37:01 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.751	114	232749	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.049	117	208160	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.018	152	94501	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	91620	43.015	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	86.040%
7) Chloroethane-d5	1.648	69	66605	40.368	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	80.740%
11) 1,1-Dichloroethene-d2	2.300	65	38338	42.088	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	84.180%
21) 2-Butanone-d5	4.452	46	95931	73.564	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	73.560%
24) Chloroform-d	5.044	84	159721	39.495	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	79.000%
26) 1,2-Dichloroethane-d4	5.946	65	110586	38.668	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	77.340%
32) Benzene-d6	5.964	84	311660	43.331	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.660%
36) 1,2-Dichloropropane-d6	7.299	67	96014	42.991	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	85.980%
41) Toluene-d8	8.641	98	287666	43.255	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	86.520%
43) trans-1,3-Dichloroprop...	8.946	79	40284	37.534	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	75.060%
47) 2-Hexanone-d5	9.384	63	63432	72.843	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	72.840%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	122186	40.801	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	81.600%
66) 1,2-Dichlorobenzene-d4	12.317	152	94880	43.091	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	86.180%
Target Compounds						
44) trans-1,3-Dichloropropene	8.952	75	2721	1.080	ug/L	Qvalue # 69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122624\
Data File : VX044495.D
Acq On : 26 Dec 2024 09:21
Operator : JC/MD
Sample : VX1226MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Dec 27 03:38:14 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 27 03:37:01 2024
Response via : Initial Calibration

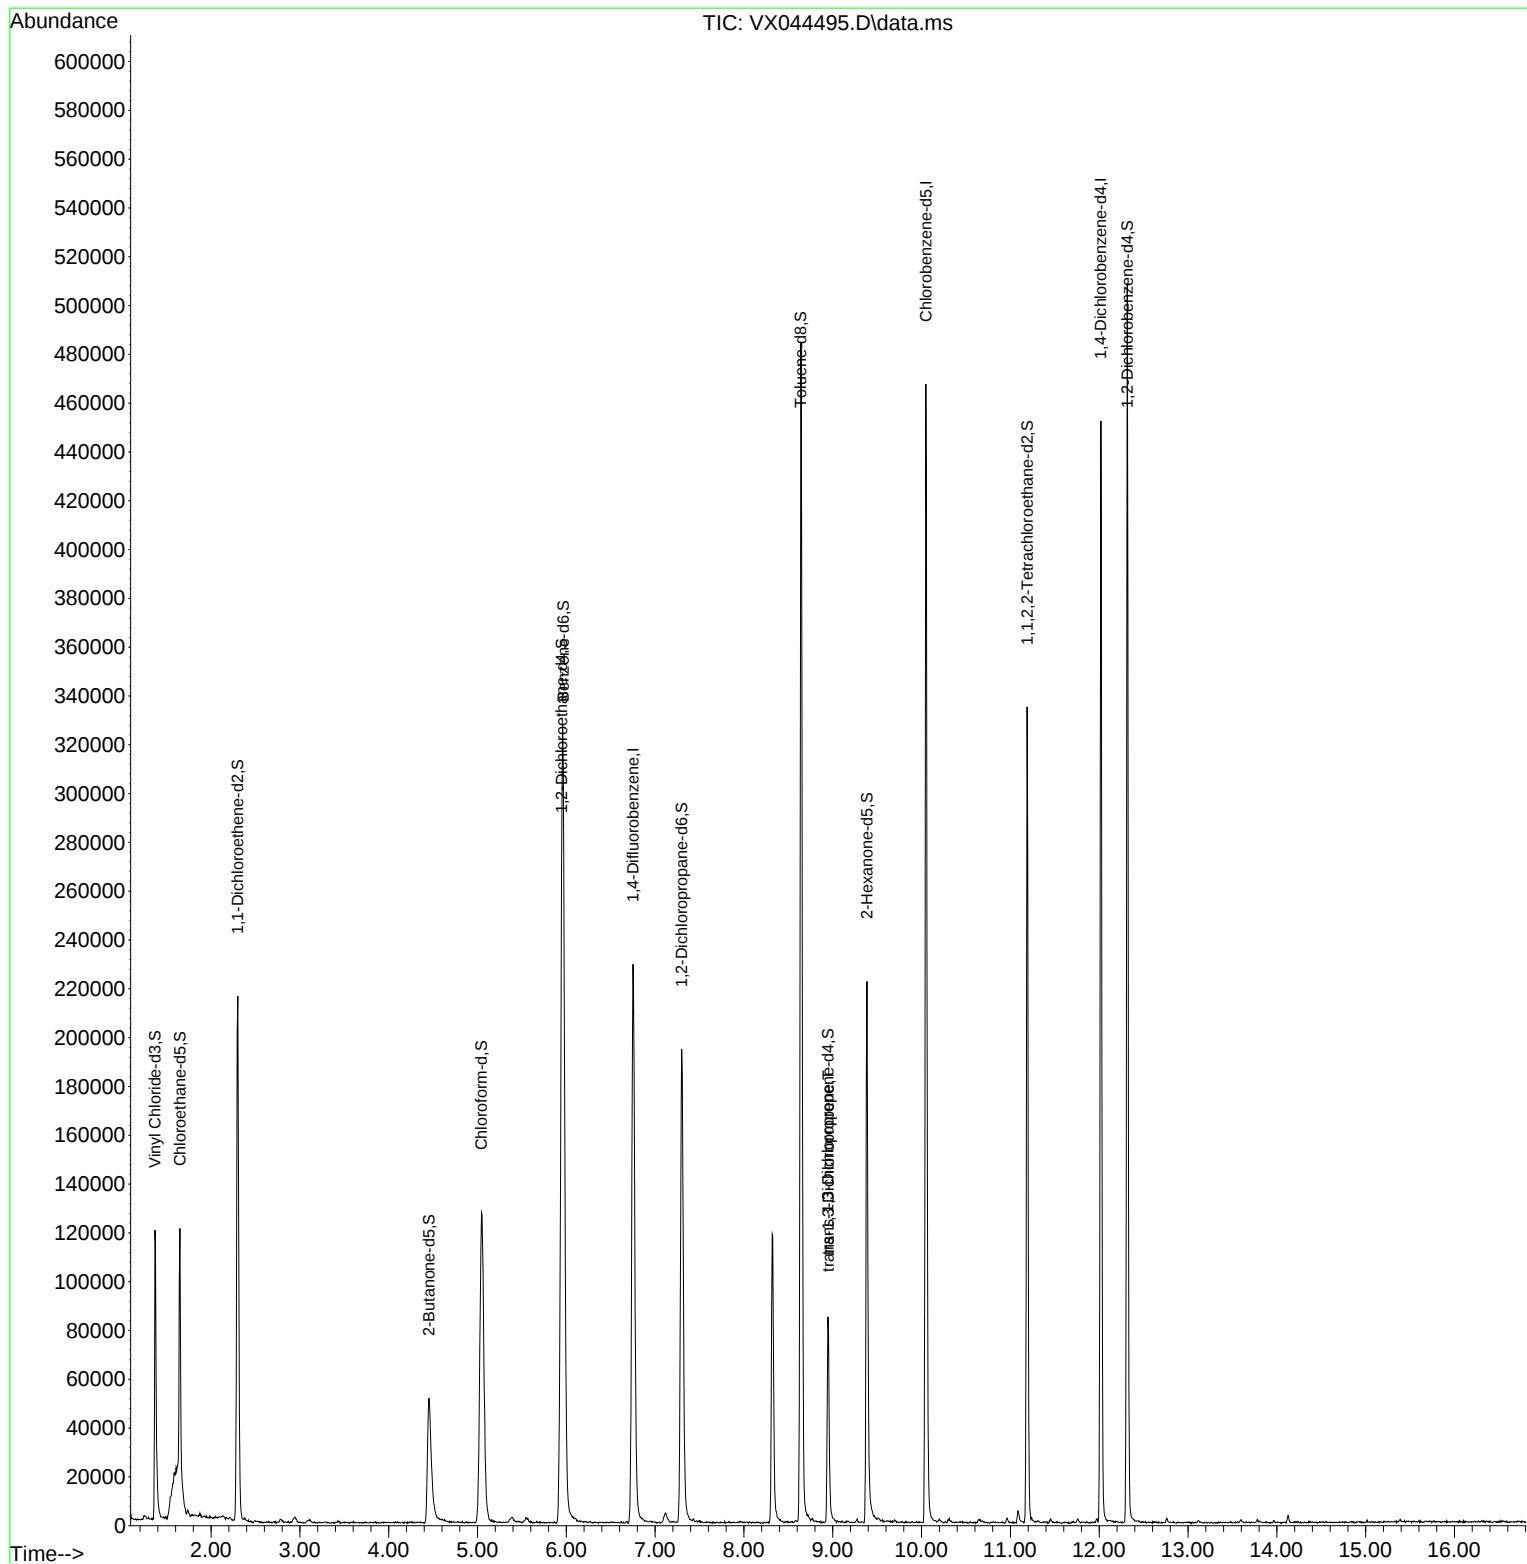

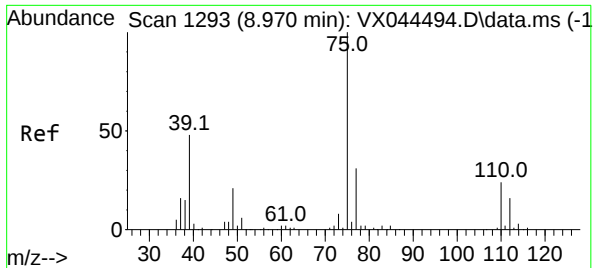

#44

trans-1,3-Dichloropropene

Concen: 1.080 ug/L

RT: 8.952 min Scan# 11

Delta R.T. -0.018 min


Lab File: VX044495.D

Acq: 26 Dec 2024 09:21

Instrument :

MSVOA_X

ClientSampleId :

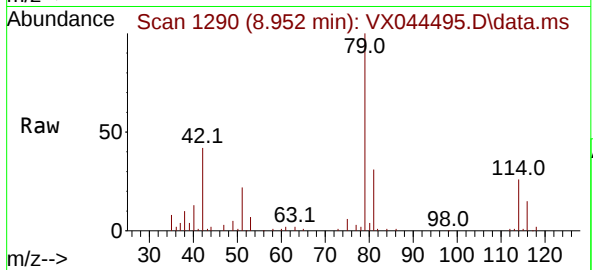

Tgt Ion: 75 Resp: 2721

Ion Ratio Lower Upper

75 100

77 48.2 21.8 40.6#

