

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122624\
 Data File : VX044497.D
 Acq On : 26 Dec 2024 10:21
 Operator : JC/MD
 Sample : P5302-09ME
 Misc : 6.33g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Dec 27 03:38:44 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 27 03:37:01 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.751	114	326097	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.049	117	288784	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.018	152	131481	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	84034	28.160	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	56.320%#
7) Chloroethane-d5	1.648	69	19286	8.343	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	16.680%#
11) 1,1-Dichloroethene-d2	2.288	65	31864	24.967	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	49.940%#
21) 2-Butanone-d5	4.660	46	137	0.075	ug/L	0.20
Spiked Amount	100.000	Range	40 - 130	Recovery	=	0.070%#
24) Chloroform-d	5.044	84	136254	24.048	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	48.100%#
26) 1,2-Dichloroethane-d4	5.946	65	96485	24.080	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	48.160%#
32) Benzene-d6	5.958	84	287704	28.833	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	57.660%#
36) 1,2-Dichloropropane-d6	7.299	67	85600	27.627	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	55.260%#
41) Toluene-d8	8.641	98	257081	27.864	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	55.720%#
43) trans-1,3-Dichloroprop...	8.945	79	33525	22.516	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	45.040%#
47) 2-Hexanone-d5	9.390	63	53008	43.878	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	43.880%#
56) 1,1,2,2-Tetrachloroeth...	11.189	84	103765	24.976	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	49.960%#
66) 1,2-Dichlorobenzene-d4	12.317	152	91320	29.810	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	59.620%#
Target Compounds						
37) 1,2-Dichloropropane	7.299	63	10249	4.352	ug/L	Qvalue # 86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122624\
Data File : VX044497.D
Acq On : 26 Dec 2024 10:21
Operator : JC/MD
Sample : P5302-09ME
Misc : 6.33g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Dec 27 03:38:44 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 27 03:37:01 2024
Response via : Initial Calibration

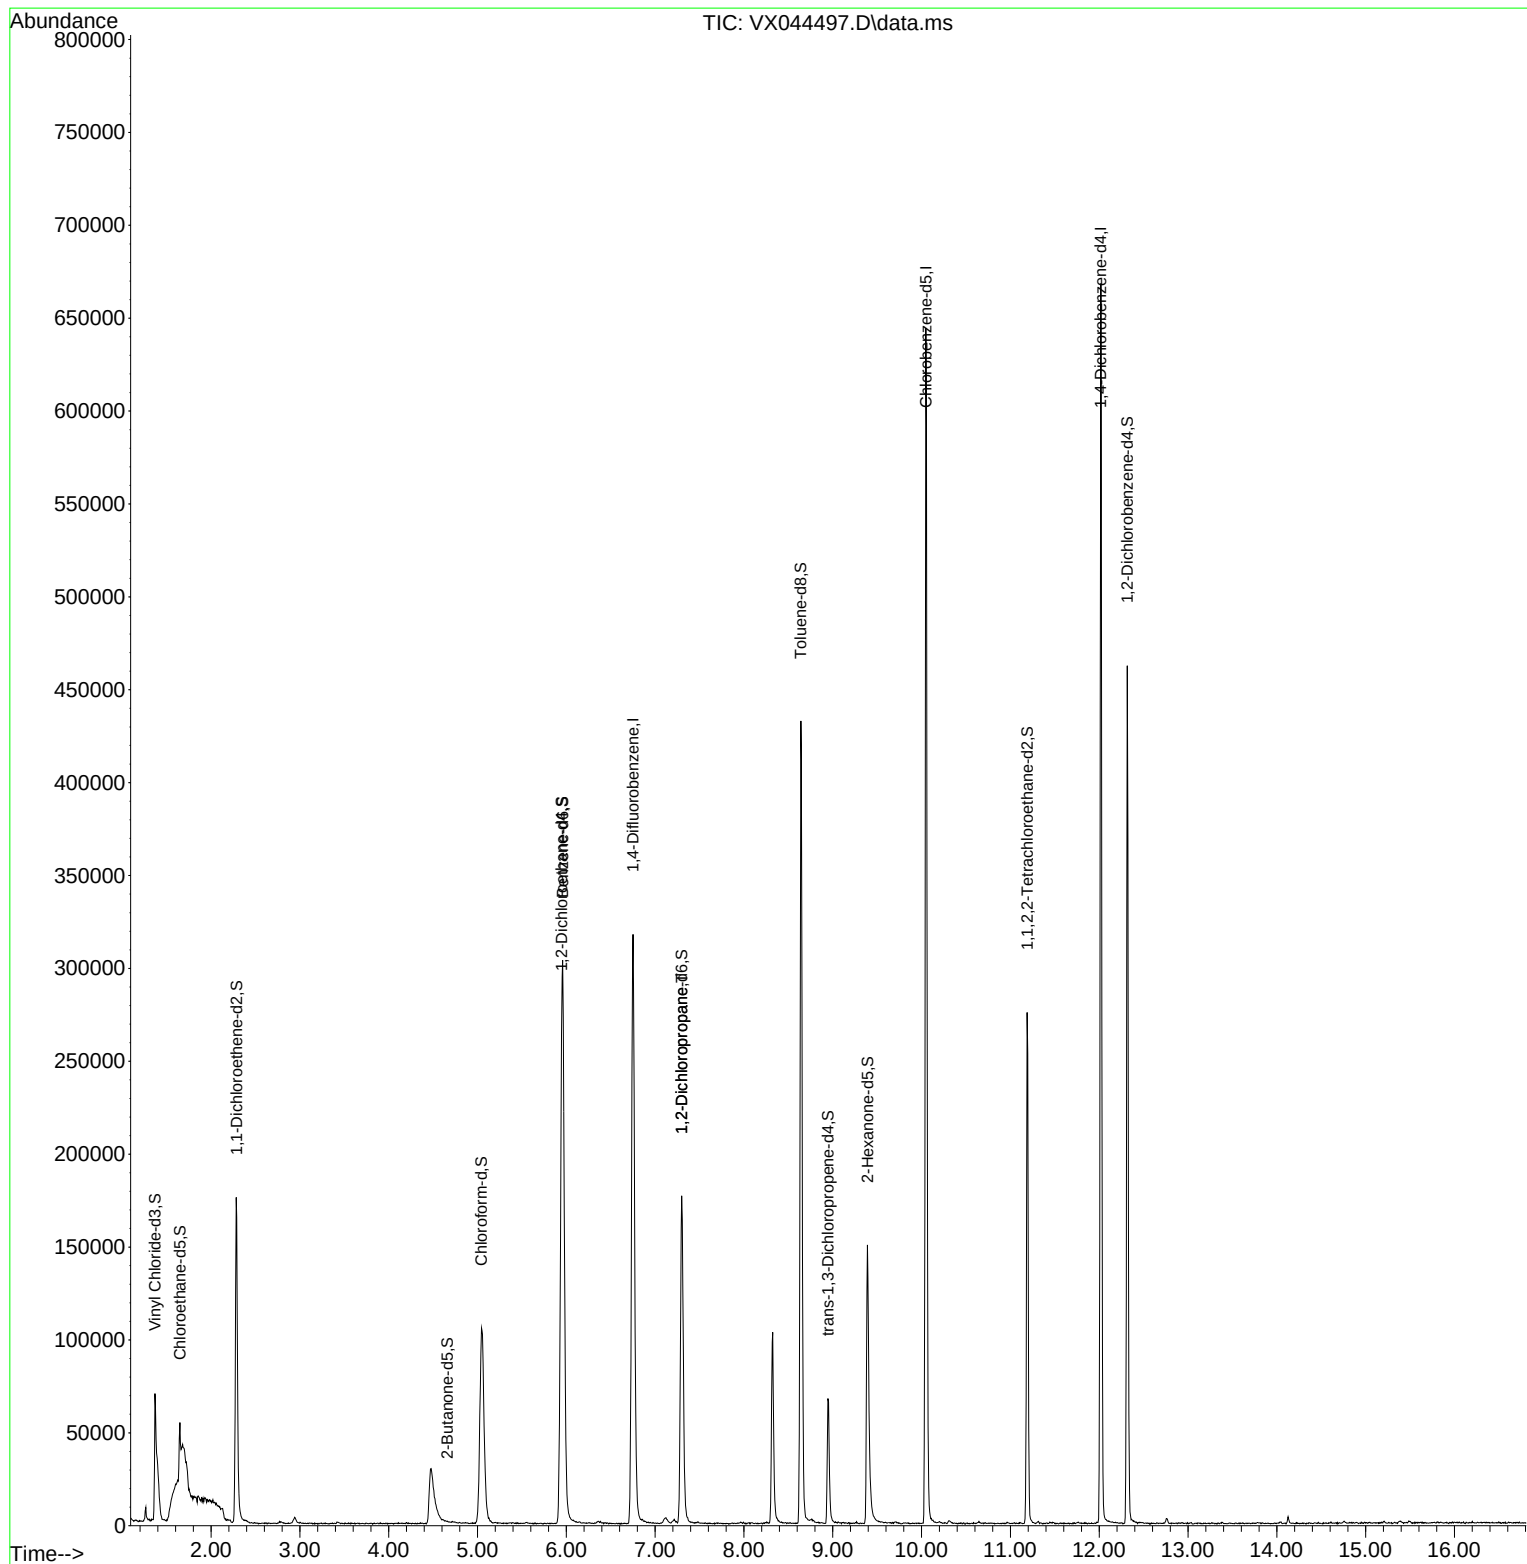

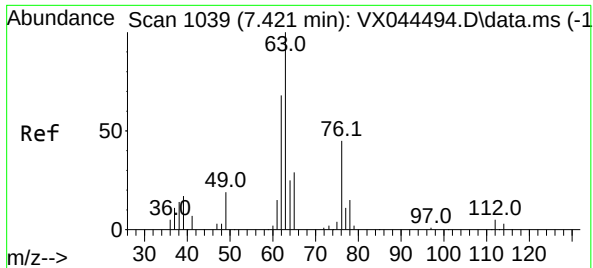

#37
 1,2-Dichloropropane
 Concen: 4.352 ug/L
 RT: 7.299 min Scan# 10
 Delta R.T. -0.122 min
 Lab File: VX044497.D
 Acq: 26 Dec 2024 10:21

Instrument :
 MSVOA_X
 ClientSampleId :

Tgt Ion: 63 Resp: 10249
 Ion Ratio Lower Upper
 63 100
 112 0.0 3.6 5.4#

