

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122624\
 Data File : VX044505.D
 Acq On : 26 Dec 2024 13:24
 Operator : JC/MD
 Sample : P5351-03ME
 Misc : 12.13g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E2925ME

Quant Time: Dec 27 03:40:49 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 27 03:37:01 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	254406	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	227176	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.018	152	111909	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	89652	38.508	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	77.020%		
7) Chloroethane-d5	1.648	69	57467	31.865	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	63.720%#		
11) 1,1-Dichloroethene-d2	2.288	65	36684	36.844	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	73.680%		
21) 2-Butanone-d5	4.465	46	90055	63.179	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	63.180%		
24) Chloroform-d	5.050	84	153691	34.769	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	69.540%#		
26) 1,2-Dichloroethane-d4	5.946	65	107838	34.497	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	69.000%#		
32) Benzene-d6	5.964	84	317496	40.447	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	80.900%		
36) 1,2-Dichloropropane-d6	7.306	67	94949	38.955	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	77.920%		
41) Toluene-d8	8.647	98	294628	40.594	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	81.180%		
43) trans-1,3-Dichloroprop...	8.946	79	37977	32.423	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	64.840%		
47) 2-Hexanone-d5	9.391	63	62188	65.437	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	65.440%		
56) 1,1,2,2-Tetrachloroeth...	11.189	84	116525	35.654	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	71.300%		
66) 1,2-Dichlorobenzene-d4	12.317	152	106664	40.908	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	81.820%		
Target Compounds					Qvalue	
15) Methyl Acetate	2.709	43	13932	6.774	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122624\
Data File : VX044505.D
Acq On : 26 Dec 2024 13:24
Operator : JC/MD
Sample : P5351-03ME
Misc : 12.13g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E2925ME


Quant Time: Dec 27 03:40:49 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 27 03:37:01 2024
Response via : Initial Calibration

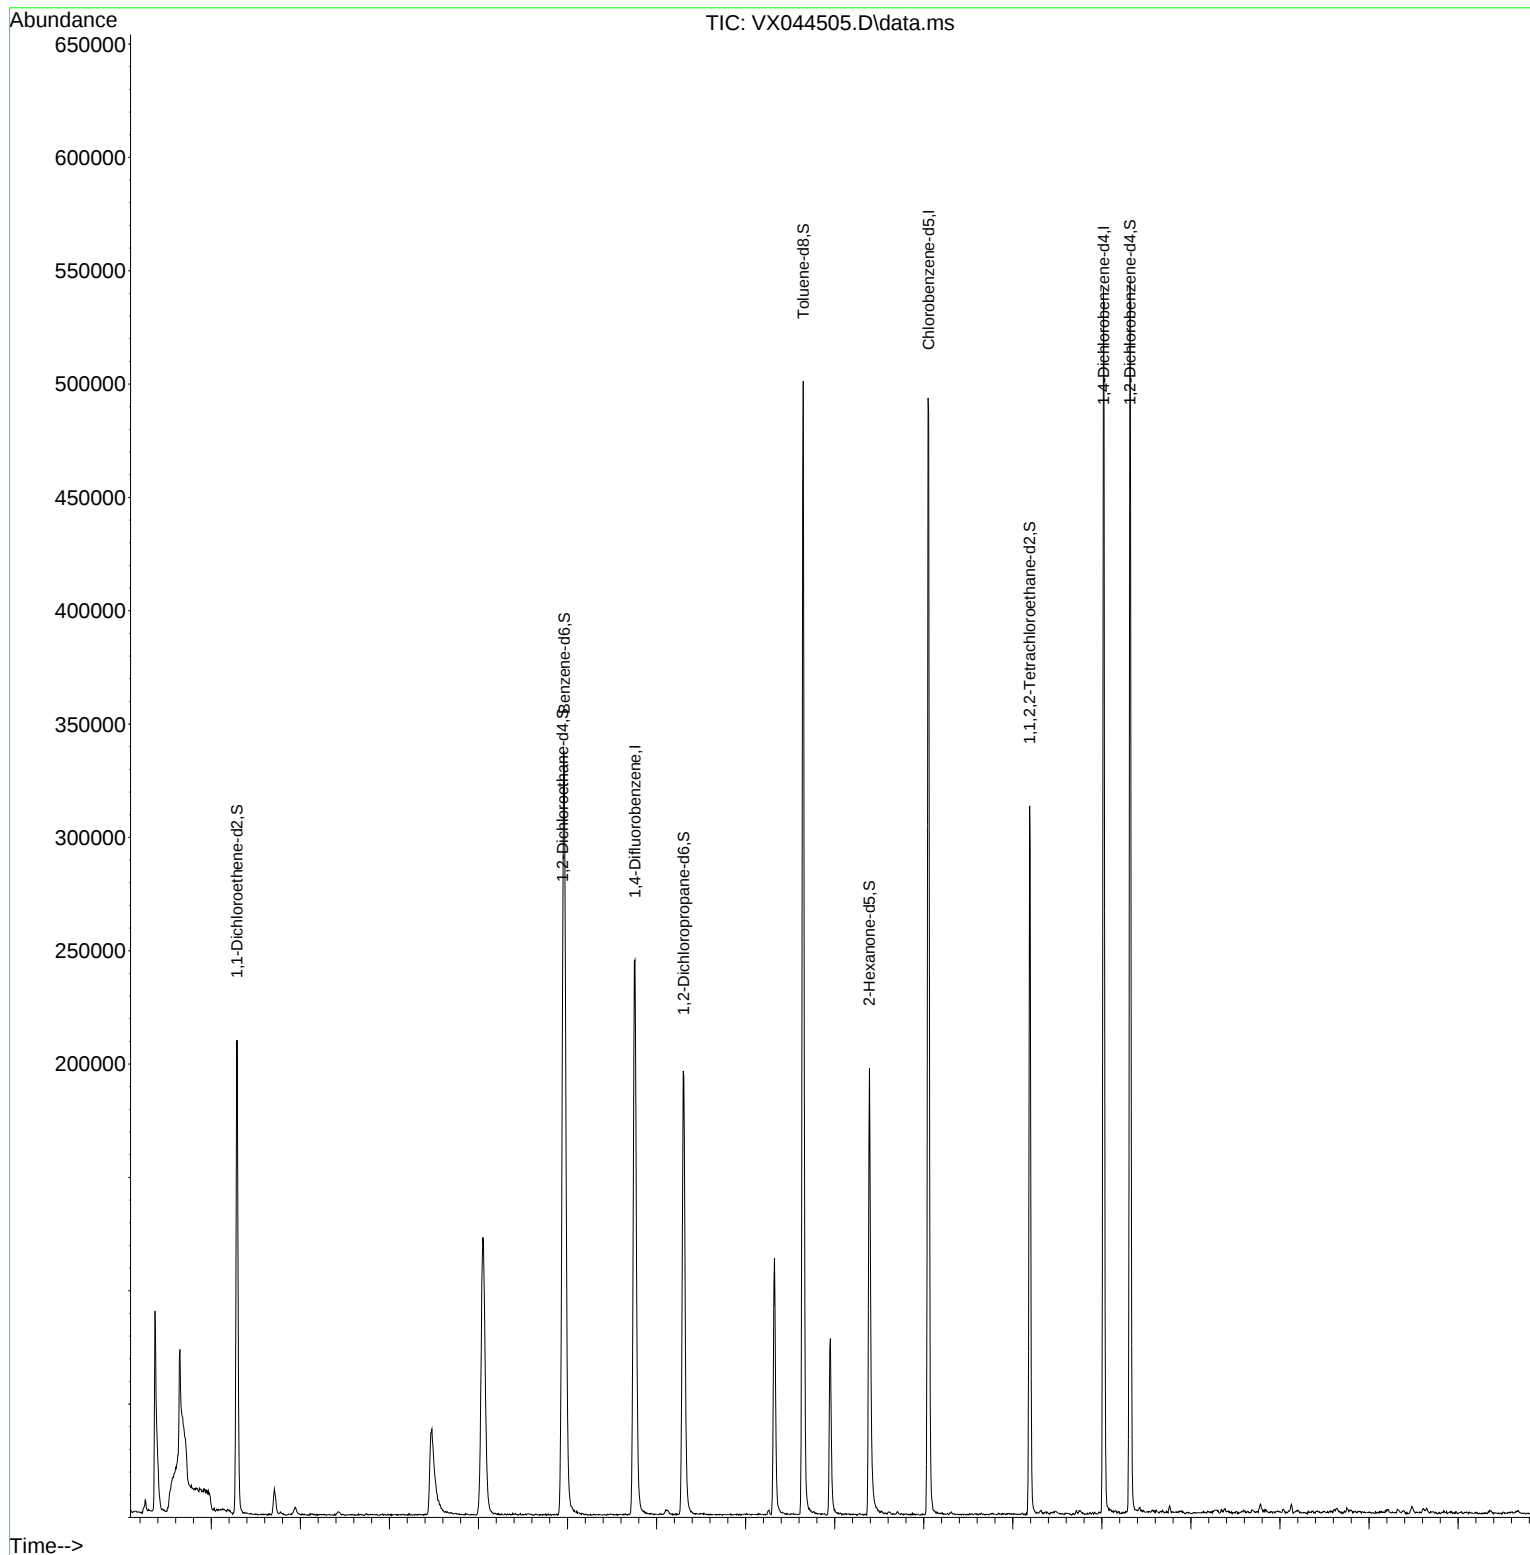

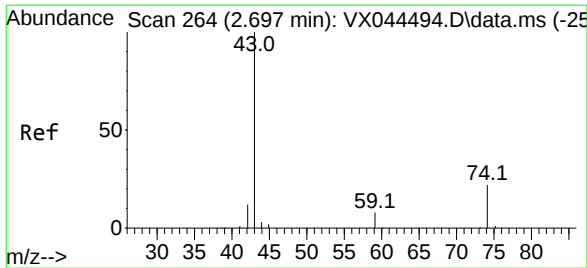

#15
Methyl Acetate
Concen: 6.774 ug/L
RT: 2.709 min Scan# 26
Delta R.T. 0.012 min
Lab File: VX044505.D
Acq: 26 Dec 2024 13:24

Instrument :
MSVOA_X
ClientSampleId :
E2925ME

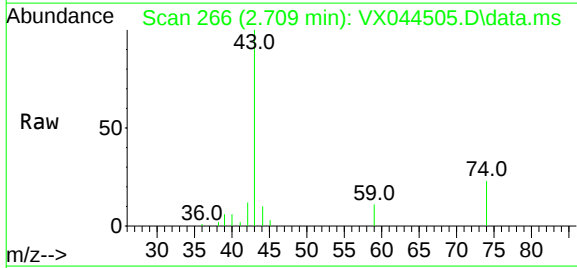

Tgt Ion: 43 Resp: 13932
Ion Ratio Lower Upper
43 100
74 24.7 19.4 29.2

