

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122624\
 Data File : VX044496.D
 Acq On : 26 Dec 2024 09:49
 Operator : JC/MD
 Sample : VX1226WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK745

Integration Parameters: LSCINT.P

Integrator: RTE

Smothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

Signal : TIC: VX044496.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	32	rBV4	2532	5554	0.58%	0.082%
2	1.368	43	46	58	rVB	112349	141374	14.67%	2.088%
3	1.648	89	92	103	rVB	104412	143453	14.88%	2.119%
4	2.300	192	199	210	rVB	200835	329446	34.17%	4.865%
5	2.739	269	271	274	rBV3	526	716	0.07%	0.011%
6	2.788	274	279	285	rVB5	1416	2911	0.30%	0.043%
7	2.849	287	289	292	rVB4	418	478	0.05%	0.007%
8	2.947	296	305	311	rBV3	3859	9612	1.00%	0.142%
9	3.221	347	350	352	rVB3	504	574	0.06%	0.008%
10	3.245	352	354	356	rBV2	710	699	0.07%	0.010%
11	3.605	409	413	416	rVB3	713	1230	0.13%	0.018%
12	3.721	431	432	436	rBV3	401	458	0.05%	0.007%
13	3.782	440	442	444	rBV2	515	632	0.07%	0.009%
14	3.867	454	456	458	rBV2	444	439	0.05%	0.006%
15	3.928	463	466	471	rVV4	452	608	0.06%	0.009%
16	3.995	474	477	478	rBV3	525	506	0.05%	0.007%
17	4.081	488	491	493	rBV3	561	474	0.05%	0.007%
18	4.117	493	497	499	rBV3	532	587	0.06%	0.009%
19	4.306	525	528	530	rVB3	496	473	0.05%	0.007%
20	4.452	545	552	569	rBV	51756	166519	17.27%	2.459%
21	4.721	594	596	597	rBV	671	478	0.05%	0.007%
22	4.806	608	610	612	rVB3	580	445	0.05%	0.007%
23	5.050	639	650	666	rVB	122360	389606	40.41%	5.754%
24	5.227	677	679	681	rBV3	531	447	0.05%	0.007%
25	5.282	687	688	690	rBV2	989	596	0.06%	0.009%
26	5.355	699	700	701	rBV	652	432	0.04%	0.006%
27	5.714	756	759	762	rBV2	530	802	0.08%	0.012%
28	5.958	787	799	820	rBV2	314573	964022	100.00%	14.237%
29	6.544	893	895	898	rVB3	696	777	0.08%	0.011%
30	6.678	915	917	918	rVB	808	550	0.06%	0.008%
31	6.751	920	929	946	rBV	219135	523612	54.32%	7.733%
32	7.056	978	979	982	rBV3	731	625	0.06%	0.009%
33	7.117	982	989	995	rBV7	4076	10152	1.05%	0.150%
34	7.300	1011	1019	1036	rBV	191942	432607	44.88%	6.389%
35	7.641	1072	1075	1076	rVB2	684	550	0.06%	0.008%
36	7.738	1088	1091	1093	rBV3	472	573	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122624\
 Data File : VX044496.D
 Acq On : 26 Dec 2024 09:49
 Operator : JC/MD
 Sample : VX1226WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK745

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

37	7.818	1101	1104	1110	rVV4	477	948	0.10%	0.014%
38	8.123	1153	1154	1158	rBV3	694	818	0.08%	0.012%
39	8.184	1161	1164	1167	rBV3	526	783	0.08%	0.012%
40	8.263	1175	1177	1179	rBV2	543	472	0.05%	0.007%
41	8.318	1180	1186	1201	rBV	121666	206255	21.40%	3.046%
42	8.549	1222	1224	1225	rBV2	631	459	0.05%	0.007%
43	8.580	1225	1229	1232	rBV5	906	1232	0.13%	0.018%
44	8.641	1233	1239	1250	rBV	449341	735214	76.27%	10.858%
45	8.946	1284	1289	1297	rBV	79951	126819	13.16%	1.873%
46	9.165	1324	1325	1327	rVB2	1033	503	0.05%	0.007%
47	9.250	1336	1339	1340	rBV2	702	777	0.08%	0.011%
48	9.275	1340	1343	1345	rVB4	1281	1362	0.14%	0.020%
49	9.385	1356	1361	1375	rBV	223618	343409	35.62%	5.072%
50	9.695	1408	1412	1415	rBV4	1070	1479	0.15%	0.022%
51	9.866	1436	1440	1443	rBV4	506	755	0.08%	0.011%
52	9.982	1458	1459	1462	rVB3	490	435	0.05%	0.006%
53	10.049	1465	1470	1485	rBV	438279	616436	63.94%	9.104%
54	10.269	1504	1506	1509	rBV2	569	583	0.06%	0.009%
55	10.311	1509	1513	1517	rVV3	1599	2255	0.23%	0.033%
56	10.378	1520	1524	1525	rBV3	558	756	0.08%	0.011%
57	10.659	1565	1570	1578	rVB8	1403	3504	0.36%	0.052%
58	10.756	1583	1586	1591	rBV4	494	994	0.10%	0.015%
59	10.890	1607	1608	1611	rBV	539	588	0.06%	0.009%
60	10.964	1617	1620	1626	rBV4	935	1647	0.17%	0.024%
61	11.189	1649	1657	1671	rBV	331398	426799	44.27%	6.303%
62	11.305	1674	1676	1680	rBV4	879	1265	0.13%	0.019%
63	11.427	1694	1696	1697	rBV	779	768	0.08%	0.011%
64	11.451	1698	1700	1703	rVV2	1602	1796	0.19%	0.027%
65	11.482	1703	1705	1709	rVB4	667	621	0.06%	0.009%
66	11.652	1730	1733	1735	rBV2	572	620	0.06%	0.009%
67	11.756	1745	1750	1754	rVB4	1402	2274	0.24%	0.034%
68	11.793	1754	1756	1760	rBV2	619	1020	0.11%	0.015%
69	11.976	1781	1786	1788	rBV4	1701	2719	0.28%	0.040%
70	12.018	1788	1793	1803	rVV	425265	531070	55.09%	7.843%
71	12.195	1820	1822	1824	rBV	836	630	0.07%	0.009%
72	12.317	1837	1842	1855	rBV	474318	596817	61.91%	8.814%
73	12.506	1871	1873	1877	rVB4	765	695	0.07%	0.010%
74	12.689	1902	1903	1907	rVB2	506	446	0.05%	0.007%
75	12.731	1907	1910	1911	rBV2	558	552	0.06%	0.008%
76	12.756	1912	1914	1918	rVB3	1982	2252	0.23%	0.033%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122624\
 Data File : VX044496.D
 Acq On : 26 Dec 2024 09:49
 Operator : JC/MD
 Sample : VX1226WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK745

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

77	12.902	1937	1938	1940	rBV	542	456	0.05%	0.007%
78	12.945	1944	1945	1948	rBV2	625	451	0.05%	0.007%
79	13.012	1952	1956	1960	rBV5	455	764	0.08%	0.011%
80	13.262	1993	1997	2000	rBV3	385	558	0.06%	0.008%
81	13.451	2026	2028	2031	rBV2	503	463	0.05%	0.007%
82	13.585	2049	2050	2051	rBV	783	548	0.06%	0.008%
83	13.725	2071	2073	2075	rBV2	622	444	0.05%	0.007%
84	13.750	2075	2077	2080	rBV3	699	708	0.07%	0.010%
85	13.786	2080	2083	2085	rBV3	1027	1281	0.13%	0.019%
86	13.932	2105	2107	2110	rBV	678	891	0.09%	0.013%
87	13.975	2112	2114	2115	rVB2	1136	682	0.07%	0.010%
88	13.993	2115	2117	2120	rVB3	413	431	0.04%	0.006%
89	14.128	2134	2139	2144	rVB	2664	3787	0.39%	0.056%
90	14.176	2144	2147	2150	rBV3	586	642	0.07%	0.009%
91	14.597	2214	2216	2218	rBV4	499	631	0.07%	0.009%
92	14.859	2258	2259	2262	rBV2	631	571	0.06%	0.008%
93	14.938	2271	2272	2276	rBV3	725	726	0.08%	0.011%
94	14.981	2278	2279	2281	rBV	824	697	0.07%	0.010%
95	15.091	2295	2297	2299	rBV3	725	576	0.06%	0.009%
96	15.377	2342	2344	2346	rBV2	1259	1279	0.13%	0.019%
97	15.737	2402	2403	2405	rBV	859	691	0.07%	0.010%
98	15.877	2424	2426	2427	rBV2	619	492	0.05%	0.007%
99	16.005	2445	2447	2449	rBV3	569	569	0.06%	0.008%
100	16.487	2521	2526	2527	rBV3	785	1159	0.12%	0.017%

Sum of corrected areas: 6771341




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122624\
Data File : VX044496.D
Acq On : 26 Dec 2024 09:49
Operator : JC/MD
Sample : VX1226WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK745

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

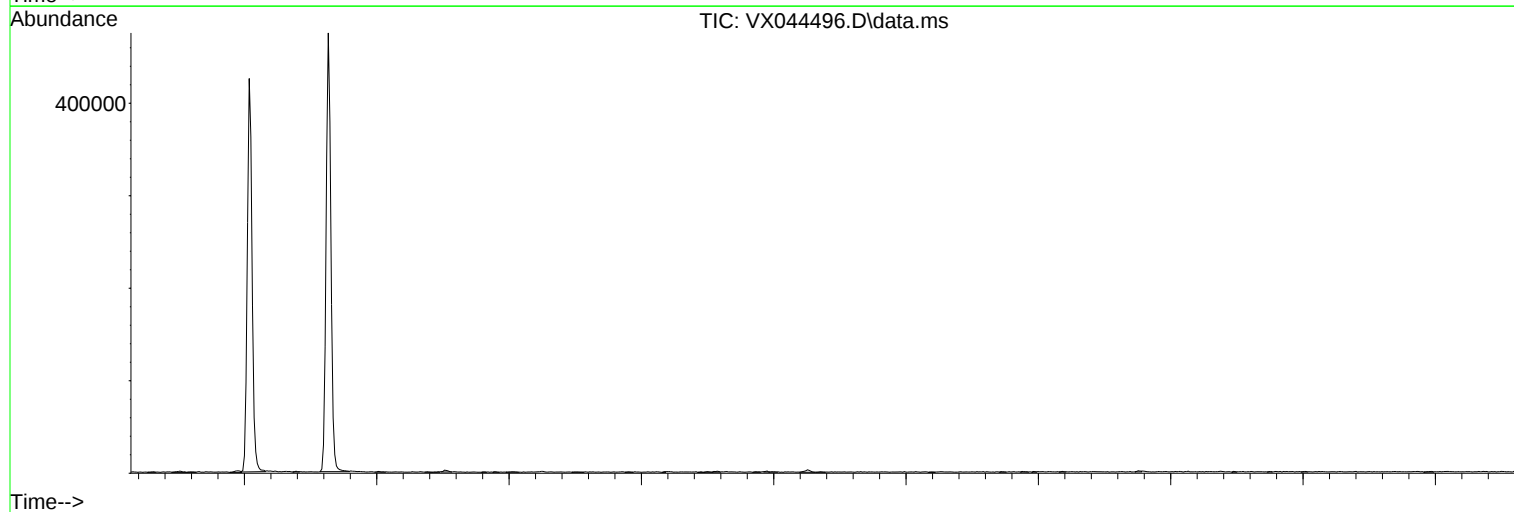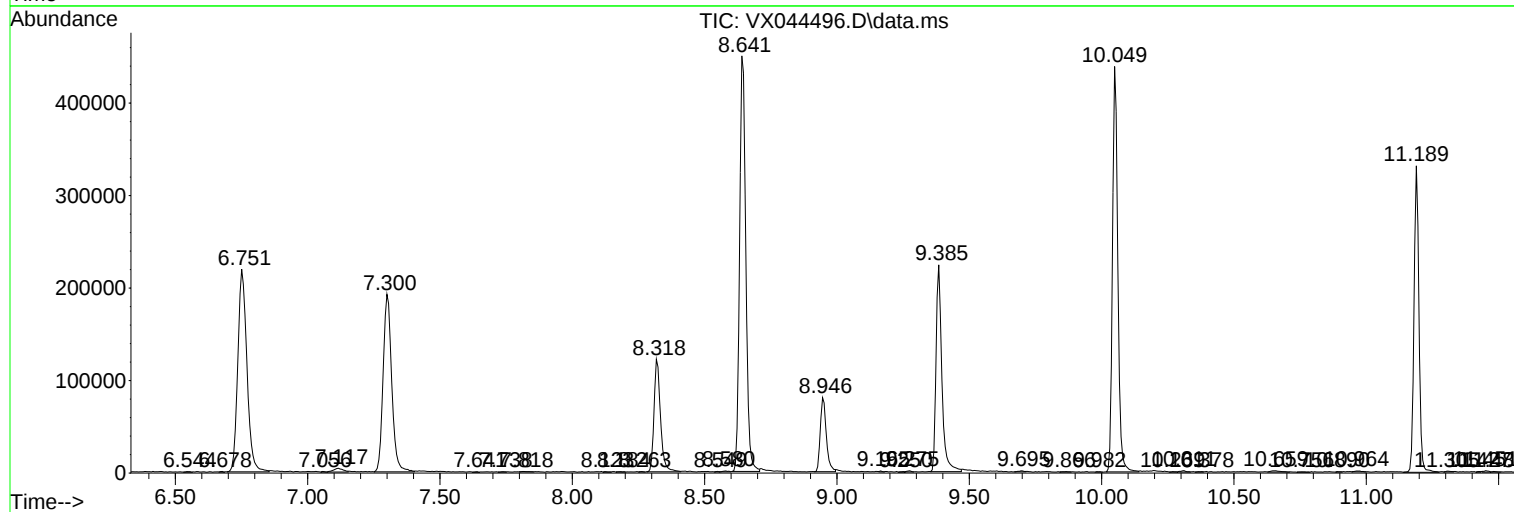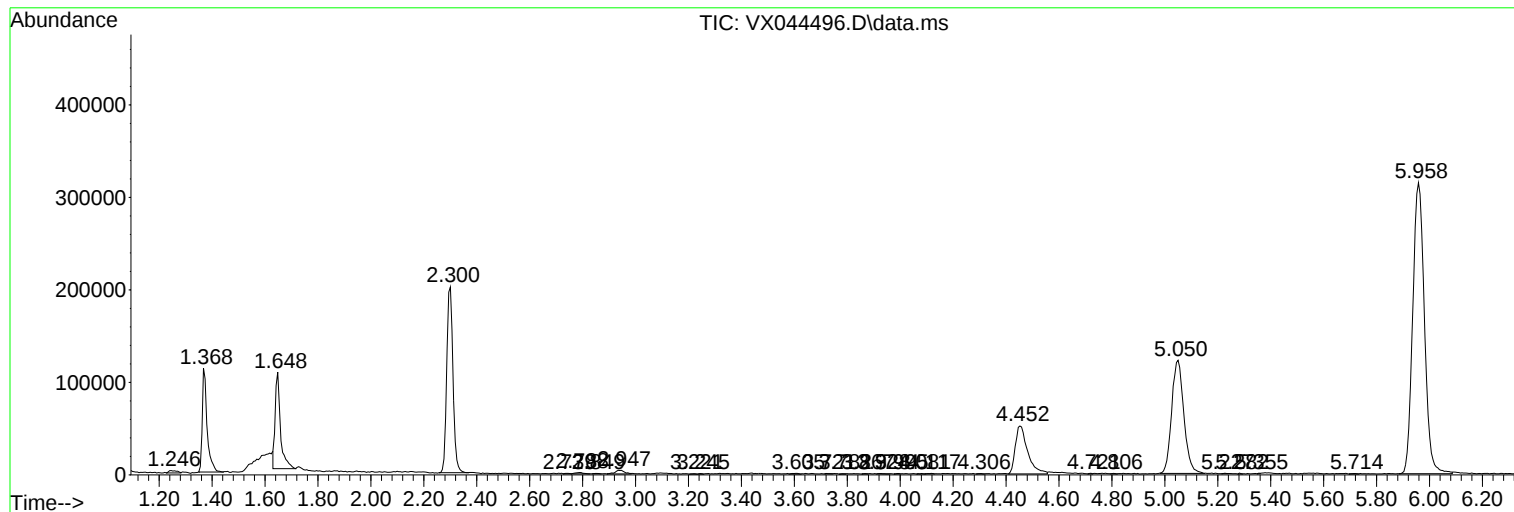

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122624\
Data File : VX044496.D
Acq On : 26 Dec 2024 09:49
Operator : JC/MD
Sample : VX1226WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK745

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122624\
Data File : VX044496.D
Acq On : 26 Dec 2024 09:49
Operator : JC/MD
Sample : VX1226WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK745

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc