
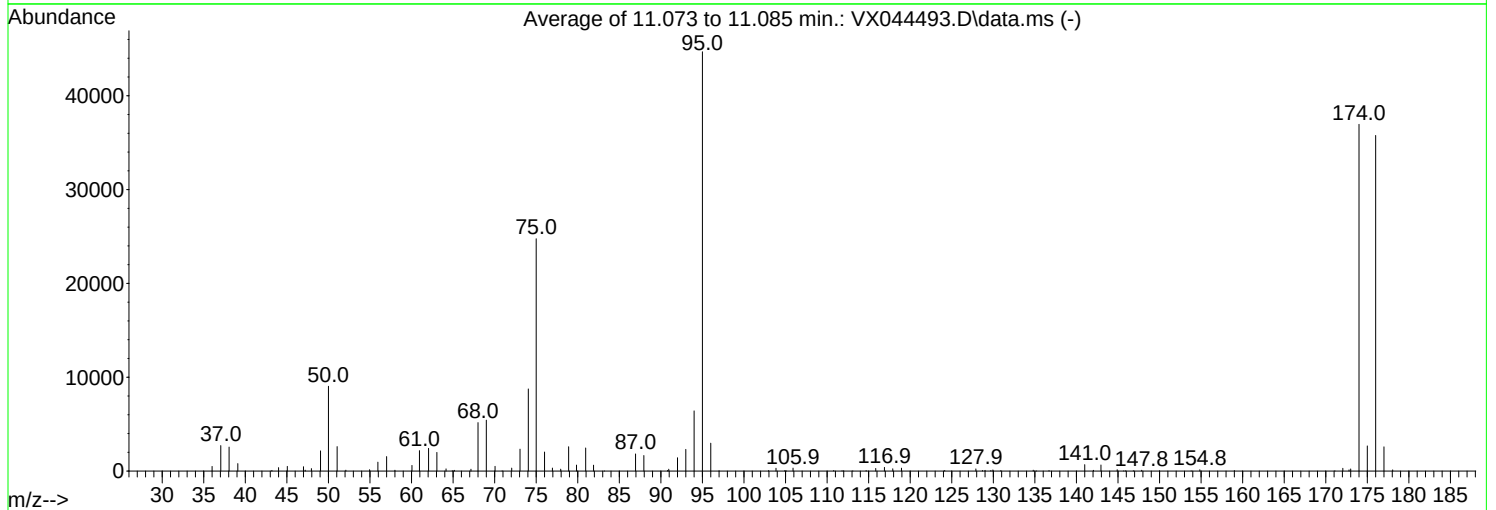


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122624\
Data File : VX044493.D
Acq On : 26 Dec 2024 07:47
Operator : JC/MD
Sample : BFB708
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB708

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
Title : VOC Analysis
Last Update : Fri Dec 27 22:07:46 2024

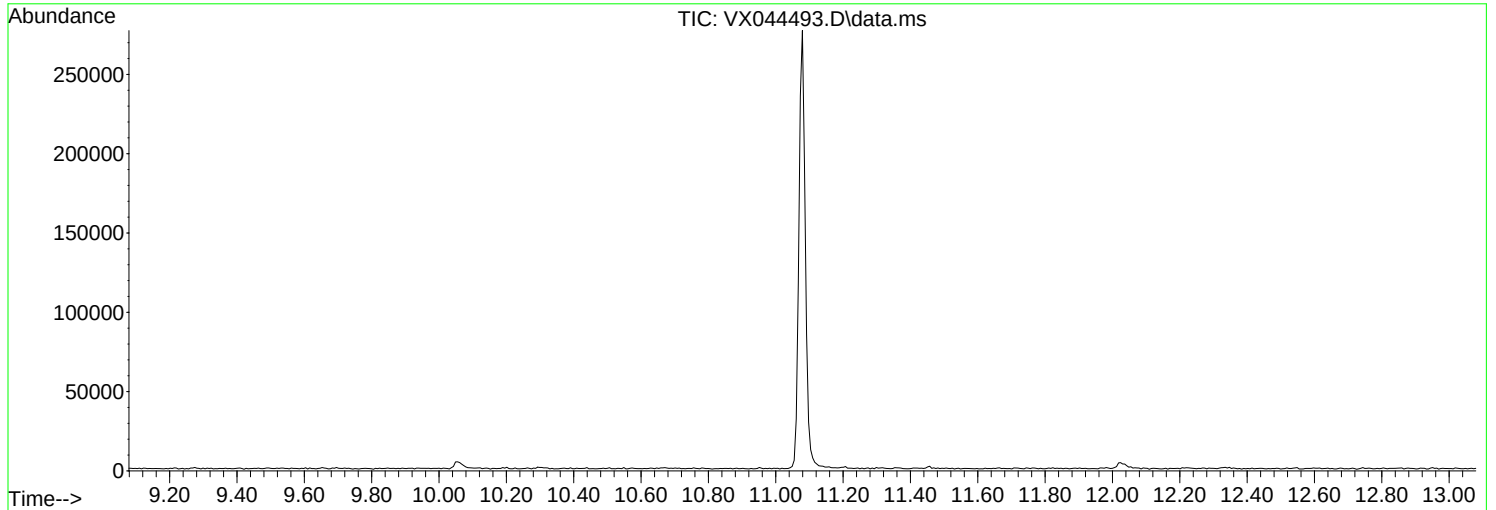

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	9039	PASS
75	95	30	80	55.4	24760	PASS
95	95	100	100	100.0	44691	PASS
96	95	5	9	6.7	2975	PASS
173	174	0.00	2	0.6	227	PASS
174	95	50	120	82.7	36957	PASS
175	174	5	9	7.3	2683	PASS
176	174	95	101	96.8	35771	PASS
177	176	5	9	7.2	2587	PASS

m/z	Abundance
38.10	118.0
39.20	549.0
40.10	564.0
44.00	283.0

Instrument :
MSVOA_X
ClientSampleId :
BFB708

m/z	Abundance
36.00	623.0
37.00	3011.0
38.00	3107.0
39.10	1572.0
40.10	495.0
43.20	122.0
44.00	522.0
45.00	559.0
47.00	491.0
47.90	303.0
49.00	2135.0
50.00	9659.0
51.10	3272.0
52.20	99.0
55.00	163.0
56.00	1021.0
57.00	1904.0
58.00	78.0
60.10	683.0
60.90	2005.0
62.00	2785.0
63.00	1900.0
64.10	208.0
65.10	120.0
67.10	312.0
68.00	5073.0
69.00	5851.0
70.10	458.0
70.90	55.0
72.00	435.0
73.00	2758.0
74.10	9646.0
75.00	26640.0
76.00	2043.0
77.00	432.0
78.00	218.0
78.90	2772.0
79.90	576.0
81.00	2743.0
81.90	772.0
83.20	52.0
87.00	2300.0
87.90	1922.0
90.80	191.0
92.00	1425.0
93.00	2542.0
94.00	6685.0
95.00	47904.0
96.00	3440.0
102.90	57.0
103.80	290.0
104.90	85.0
106.00	317.0
110.80	62.0
111.80	108.0
113.10	52.0
115.90	344.0
116.90	543.0
118.00	163.0
119.00	384.0
127.90	232.0
128.70	101.0
130.00	161.0
134.70	66.0
135.20	58.0
136.70	98.0
141.00	590.0
142.00	76.0
142.90	755.0
144.90	214.0
145.70	77.0
154.90	111.0
172.10	240.0
172.80	379.0
174.00	32016.0
175.00	2469.0
176.00	29856.0
177.00	2180.0
178.10	148.0

Instrument :
MSVOA_X
ClientSampleId :
BFB708

m/z	Abundance
36.00	537.0
37.10	3142.0
38.10	3104.0
39.10	1356.0
40.00	569.0
43.20	52.0
44.00	778.0
45.10	566.0
47.00	665.0
48.00	277.0
49.10	2650.0
50.00	11082.0
51.00	2874.0
52.10	83.0
54.90	196.0
55.90	1009.0
57.00	1708.0
58.00	194.0
60.00	585.0
61.00	2863.0
62.10	2495.0
63.00	2487.0
64.20	262.0
65.20	132.0
67.20	151.0
68.00	6525.0
69.00	6409.0
70.00	536.0
72.10	294.0
73.00	2417.0
74.00	10163.0
75.00	28232.0
76.00	2511.0
77.00	254.0
77.90	174.0
78.90	3187.0
79.90	765.0
80.90	2659.0
81.90	575.0
87.00	2297.0
88.00	1696.0
91.00	392.0
92.10	1910.0
93.00	2447.0
94.00	7416.0
95.00	52256.0
96.00	3079.0
97.00	86.0
103.00	79.0
103.90	364.0
104.90	56.0
105.90	363.0
110.80	133.0
112.00	81.0
114.70	111.0
115.90	280.0
116.90	346.0
117.90	342.0
118.90	301.0
124.20	112.0
128.00	212.0
128.70	87.0
129.00	84.0
129.90	211.0
130.90	71.0
134.80	102.0
136.70	91.0
141.00	716.0
142.10	176.0
143.00	723.0
144.90	78.0
145.90	77.0
146.90	57.0
147.90	196.0
150.00	61.0
154.80	189.0
159.00	80.0
171.10	77.0
172.00	278.0
173.00	360.0
174.00	44096.0
175.00	3048.0
176.00	44504.0
177.00	3225.0
178.00	146.0

Instrument :
MSVOA_X
ClientSampleId :
BFB708

m/z	Abundance
36.10	324.0
37.00	2000.0
38.00	1812.0
39.10	1122.0
40.00	601.0
43.10	52.0
44.10	656.0
45.00	390.0
46.90	236.0
47.20	288.0
47.90	218.0
49.00	1687.0
50.10	6375.0
51.00	1679.0
52.00	113.0
54.90	94.0
55.90	833.0
57.00	1023.0
60.00	546.0
61.00	1676.0
62.00	1976.0
63.10	1582.0
64.10	242.0
64.90	99.0
67.10	144.0
68.00	3901.0
69.00	4028.0
70.00	523.0
72.00	225.0
73.10	1842.0
74.00	6452.0
75.00	19408.0
76.00	1546.0
76.90	283.0
78.00	222.0
78.90	1823.0
79.80	578.0
80.90	1979.0
81.90	545.0
86.80	887.0
87.90	1358.0
90.90	204.0
91.90	927.0
93.00	1946.0
94.00	5149.0
95.00	33912.0
96.00	2405.0
103.80	259.0
105.10	57.0
105.80	272.0
114.70	57.0
115.70	220.0
116.90	295.0
117.80	233.0
118.90	254.0
124.10	72.0
127.80	254.0
129.00	144.0
129.70	193.0
130.90	61.0
134.90	121.0
141.00	761.0
143.00	469.0
144.90	155.0
146.80	71.0
147.80	71.0
153.80	68.0
154.90	136.0
159.00	61.0
172.00	379.0
173.00	322.0
174.00	34760.0
175.00	2533.0
176.00	32952.0
177.00	2356.0
178.00	85.0

Instrument :
MSVOA_X
ClientSampleId :
BFB708