


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX122719\
 Data File : VX014301.D
 Acq On : 27 Dec 2019 11:31
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X121319W.M
 Title : SW846 8260
 Last Update : Tue Dec 17 03:01:07 2019

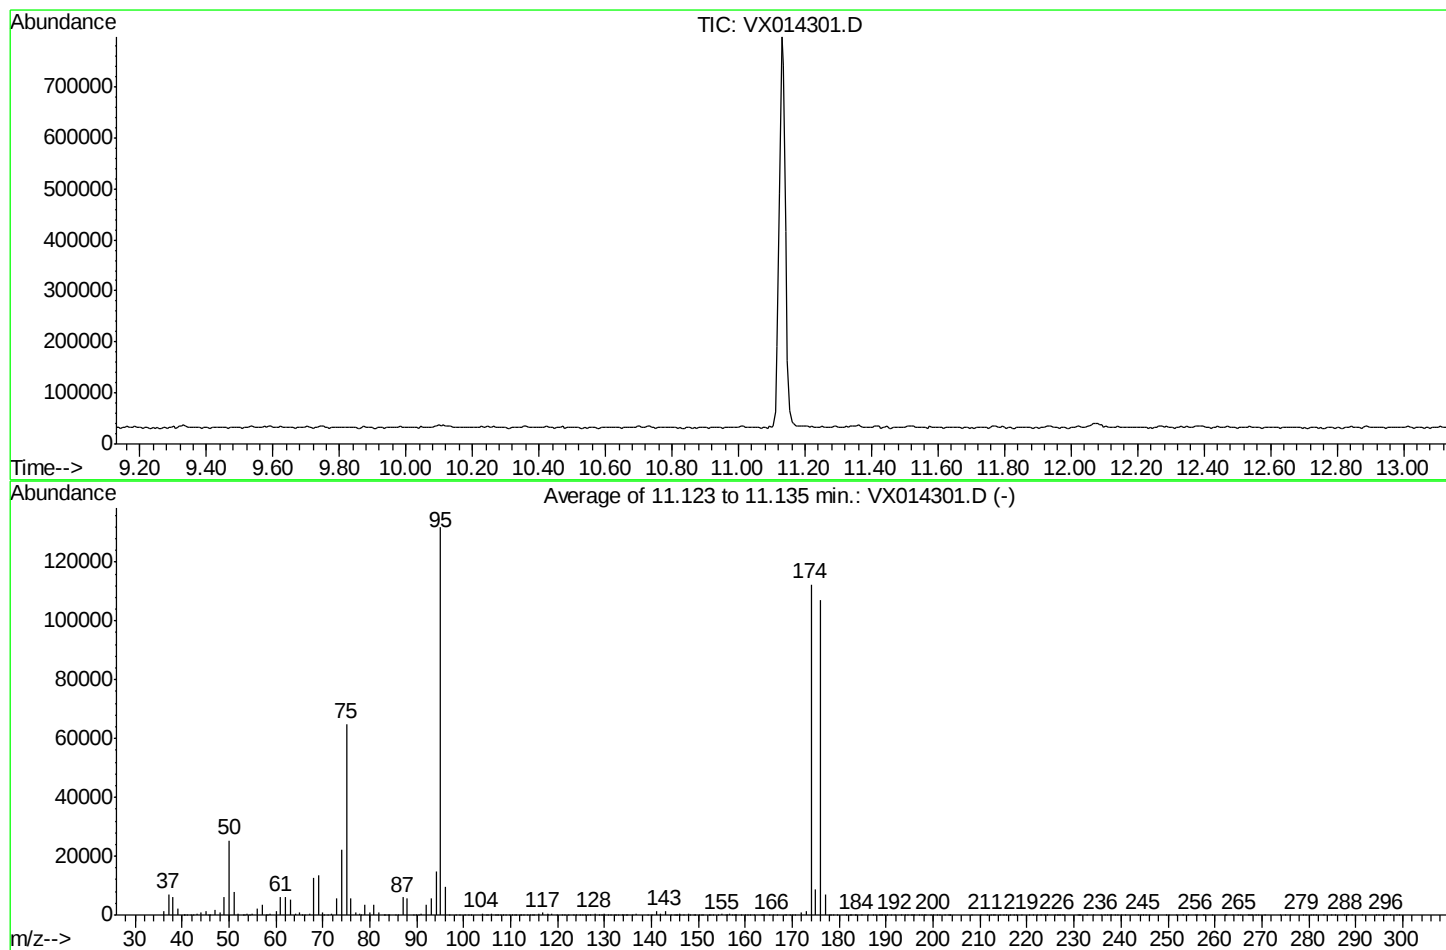

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1671

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	25313	PASS
75	95	30	60	49.3	65025	PASS
95	95	100	100	100.0	131828	PASS
96	95	5	9	7.1	9385	PASS
173	174	0.00	2	1.3	1513	PASS
174	95	50	100	85.3	112496	PASS
175	174	5	9	7.6	8575	PASS
176	174	95	101	95.2	107116	PASS
177	176	5	9	6.5	6928	PASS