


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX122719\
Data File : VX014329.D
Acq On : 27 Dec 2019 23:07
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X121319W.M
Title : SW846 8260
Last Update : Tue Dec 17 03:01:07 2019

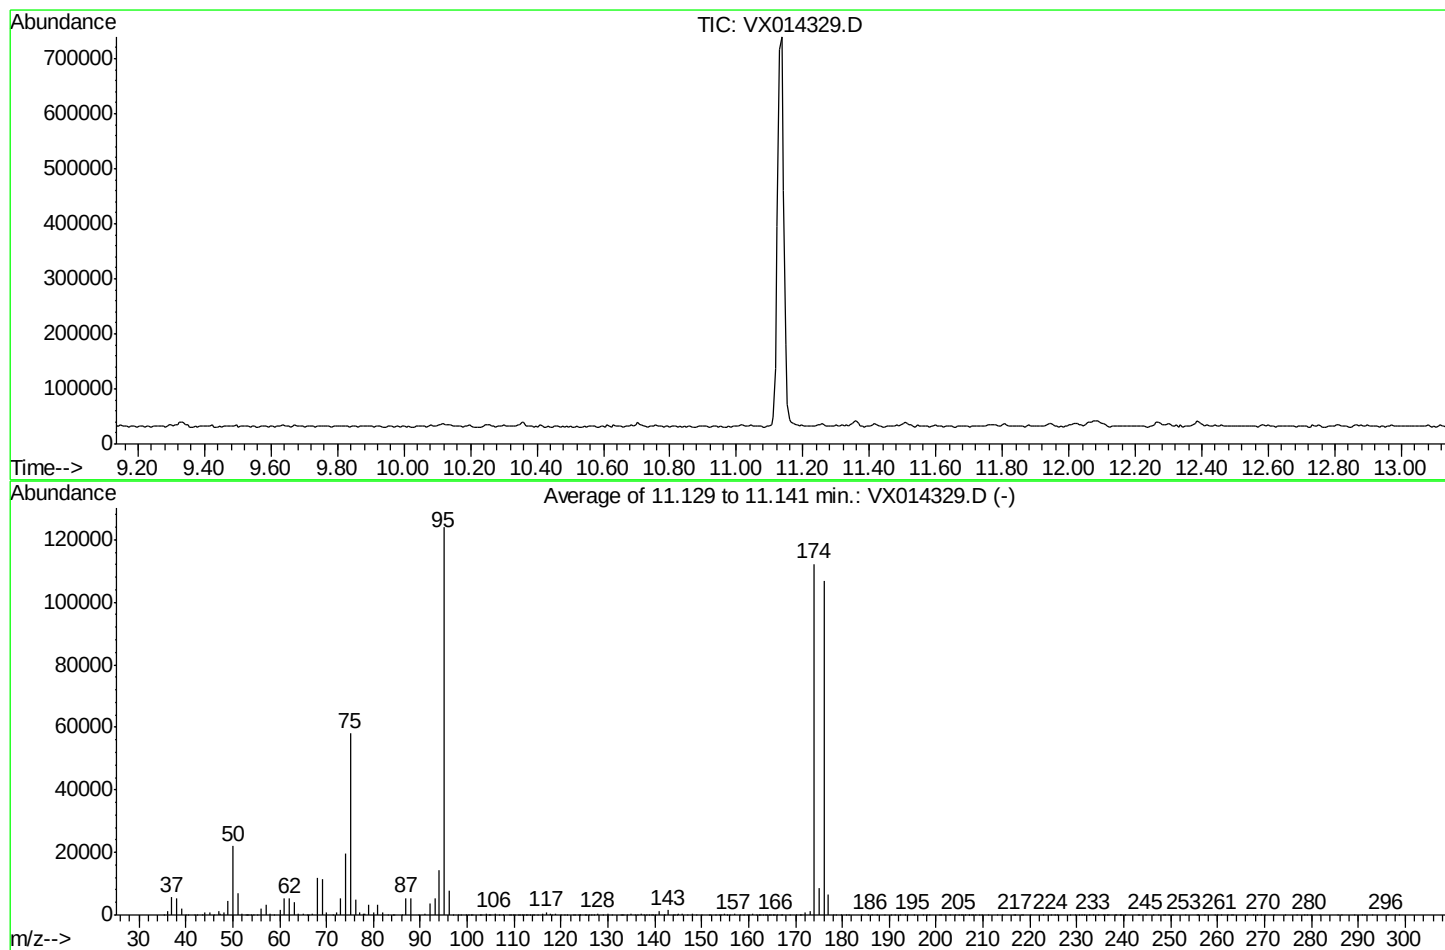

AutoFind: Scans 1680, 1681, 1682; Background Corrected with Scan 1672

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	22092	PASS
75	95	30	60	46.8	58052	PASS
95	95	100	100	100.0	123937	PASS
96	95	5	9	6.4	7993	PASS
173	174	0.00	2	1.3	1417	PASS
174	95	50	100	90.6	112266	PASS
175	174	5	9	7.6	8525	PASS
176	174	95	101	95.2	106826	PASS
177	176	5	9	6.3	6729	PASS