

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026057.D
 Acq On : 27 Dec 2021 13:27
 Operator : JC/MD
 Sample : M5213-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BGLD9

Quant Time: Dec 27 15:25:11 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Dec 23 21:00:32 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	198818	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	184524	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	88301	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.374	65	92698	65.748	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 131.500%			
7) Chloroethane-d5	1.672	69	69666	61.830	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 123.660%			
11) 1,1-Dichloroethene-d2	2.312	63	129679	46.414	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 92.820%			
21) 2-Butanone-d5	4.458	46	139354	114.004	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 114.000%			
24) Chloroform-d	5.068	84	156005	55.292	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 110.580%			
26) 1,2-Dichloroethane-d4	5.958	65	107232	56.134	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 112.260%			
32) Benzene-d6	5.976	84	326406	61.456	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 122.920%			
36) 1,2-Dichloropropane-d6	7.312	67	101422	61.432	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 122.860%#			
41) Toluene-d8	8.653	98	294914	59.470	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 118.940%			
43) trans-1,3-Dichloroprop...	8.951	79	40320	56.133	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 112.260%			
47) 2-Hexanone-d5	9.384	63	102231	119.980	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 119.980%			
56) 1,1,2,2-Tetrachloroeth...	11.195	84	131191	53.890	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 107.780%			
66) 1,2-Dichlorobenzene-d4	12.323	152	102121	61.201	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 122.400%#			
Target Compounds					Qvalue	
13) Acetone	2.386	43	4795	7.175	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026057.D
Acq On : 27 Dec 2021 13:27
Operator : JC/MD
Sample : M5213-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BGLD9

Quant Time: Dec 27 15:25:11 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Dec 23 21:00:32 2021
Response via : Initial Calibration

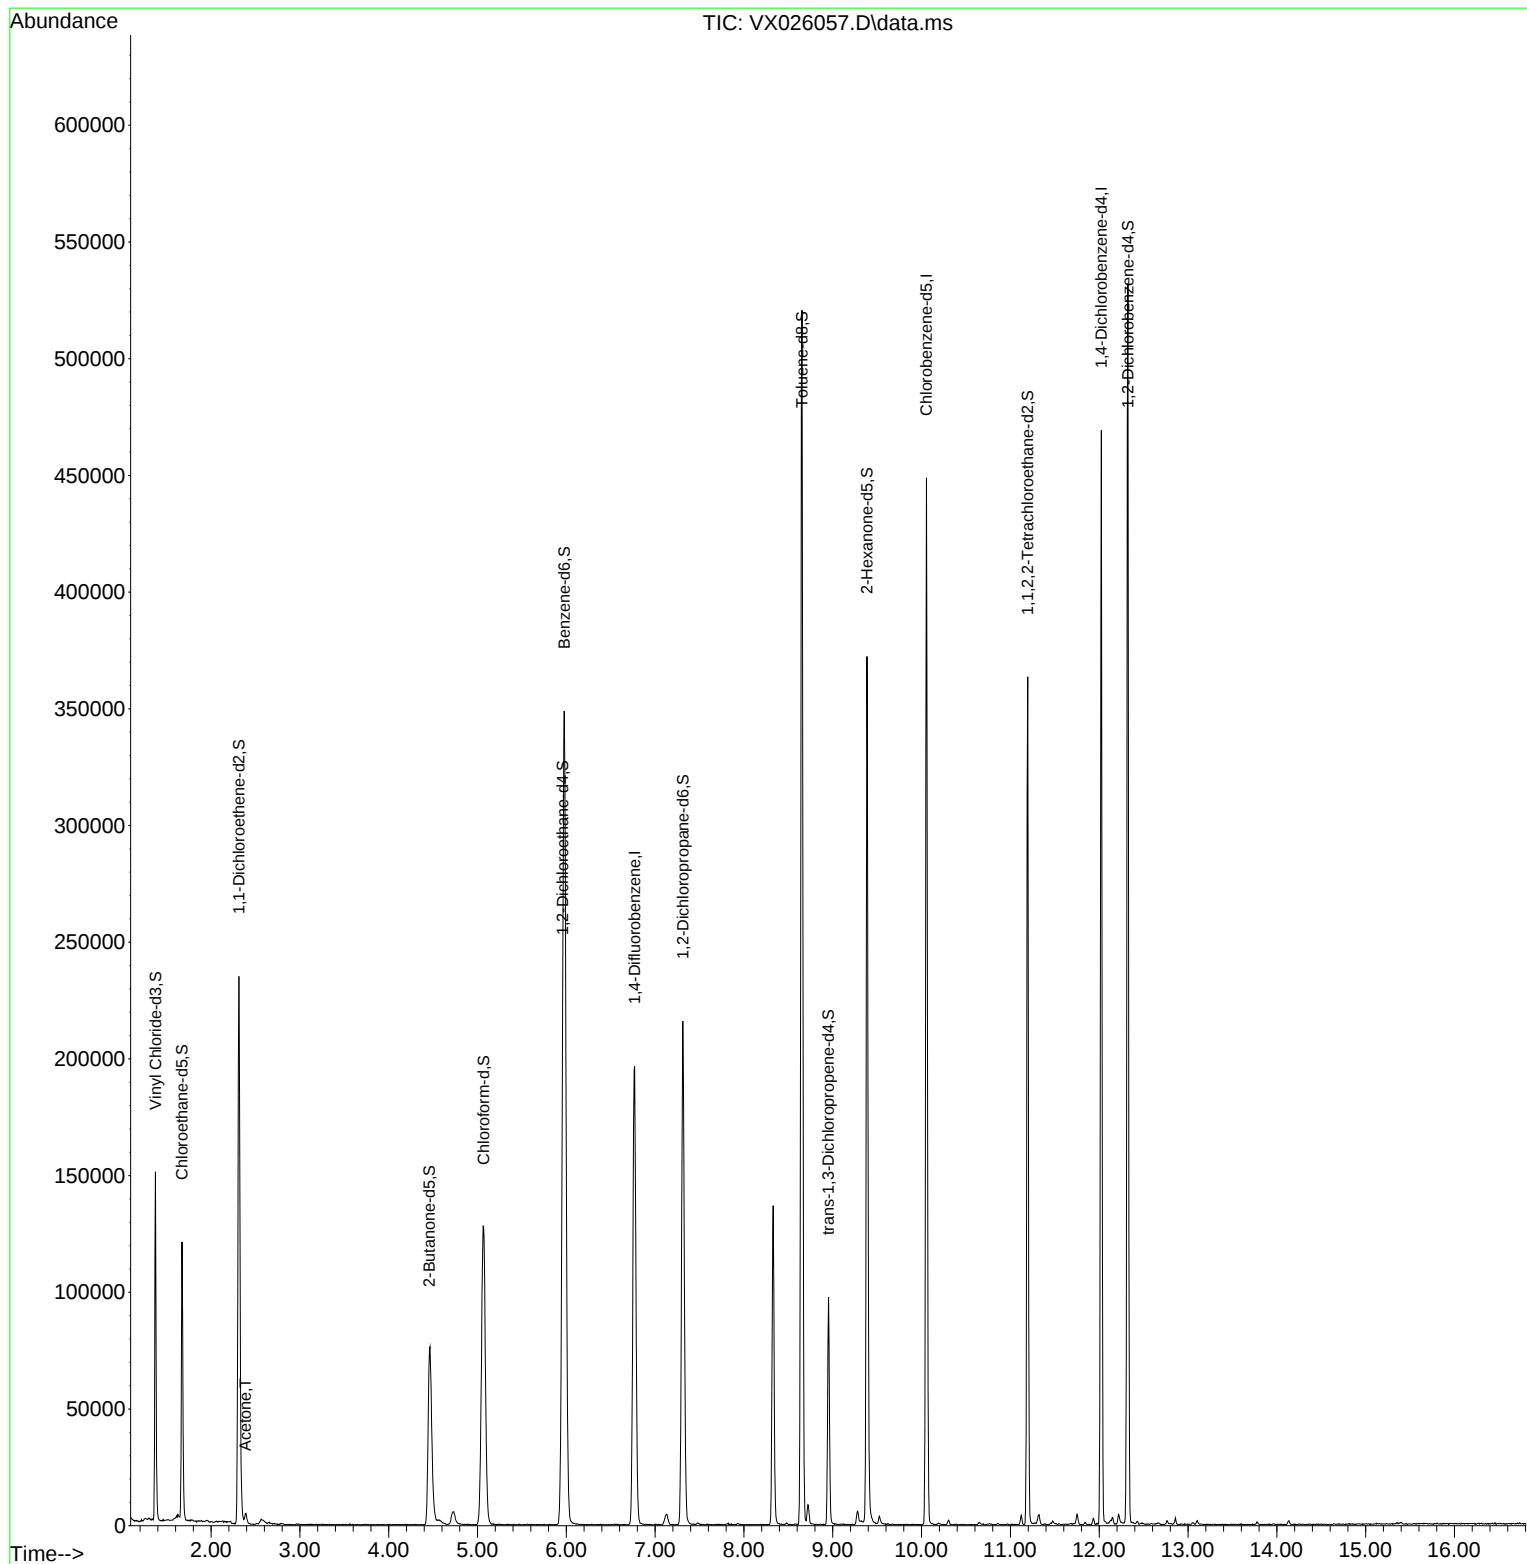

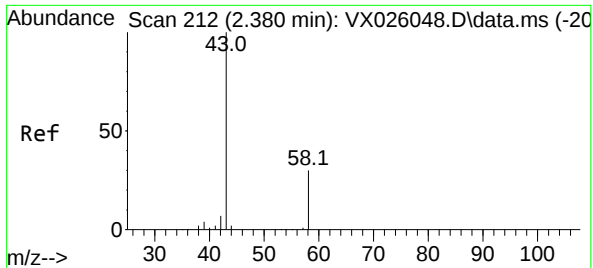

#13
 Acetone
 Concen: 7.175 ug/L
 RT: 2.386 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: VX026057.D
 Acq: 27 Dec 2021 13:27

Instrument :
 MSVOA_X
 ClientSampleId :
 BGLD9

Tgt Ion: 43 Resp: 4795
 Ion Ratio Lower Upper
 43 100
 58 29.2 0.0 65.6

