

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026062.D
 Acq On : 27 Dec 2021 15:22
 Operator : JC/MD
 Sample : M5126-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J23

Quant Time: Dec 28 01:31:32 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Dec 23 21:00:32 2021
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	200545	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	182637	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	86948	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.374	65	90048	63.319	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	= 126.640%		
7) Chloroethane-d5	1.672	69	68160	59.972	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	= 119.940%		
11) 1,1-Dichloroethene-d2	2.313	63	125048	44.371	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	= 88.740%		
21) 2-Butanone-d5	4.458	46	130780	106.068	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	= 106.070%		
24) Chloroform-d	5.068	84	155313	54.573	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 109.140%		
26) 1,2-Dichloroethane-d4	5.964	65	105840	54.928	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 109.860%		
32) Benzene-d6	5.976	84	318945	60.671	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 121.340%		
36) 1,2-Dichloropropane-d6	7.312	67	99592	60.946	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	= 121.900%#		
41) Toluene-d8	8.653	98	287548	58.584	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	= 117.160%		
43) trans-1,3-Dichloroprop...	8.952	79	39112	55.014	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	= 110.020%		
47) 2-Hexanone-d5	9.384	63	92835	110.079	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	= 110.080%		
56) 1,1,2,2-Tetrachloroeth...	11.195	84	128068	53.151	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	= 106.300%		
66) 1,2-Dichlorobenzene-d4	12.323	152	98827	60.149	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	= 120.300%#		
Target Compounds						
13) Acetone	2.386	43	4605	6.832	ug/L	Qvalue 87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026062.D
Acq On : 27 Dec 2021 15:22
Operator : JC/MD
Sample : M5126-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J23

Quant Time: Dec 28 01:31:32 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Dec 23 21:00:32 2021
Response via : Initial Calibration

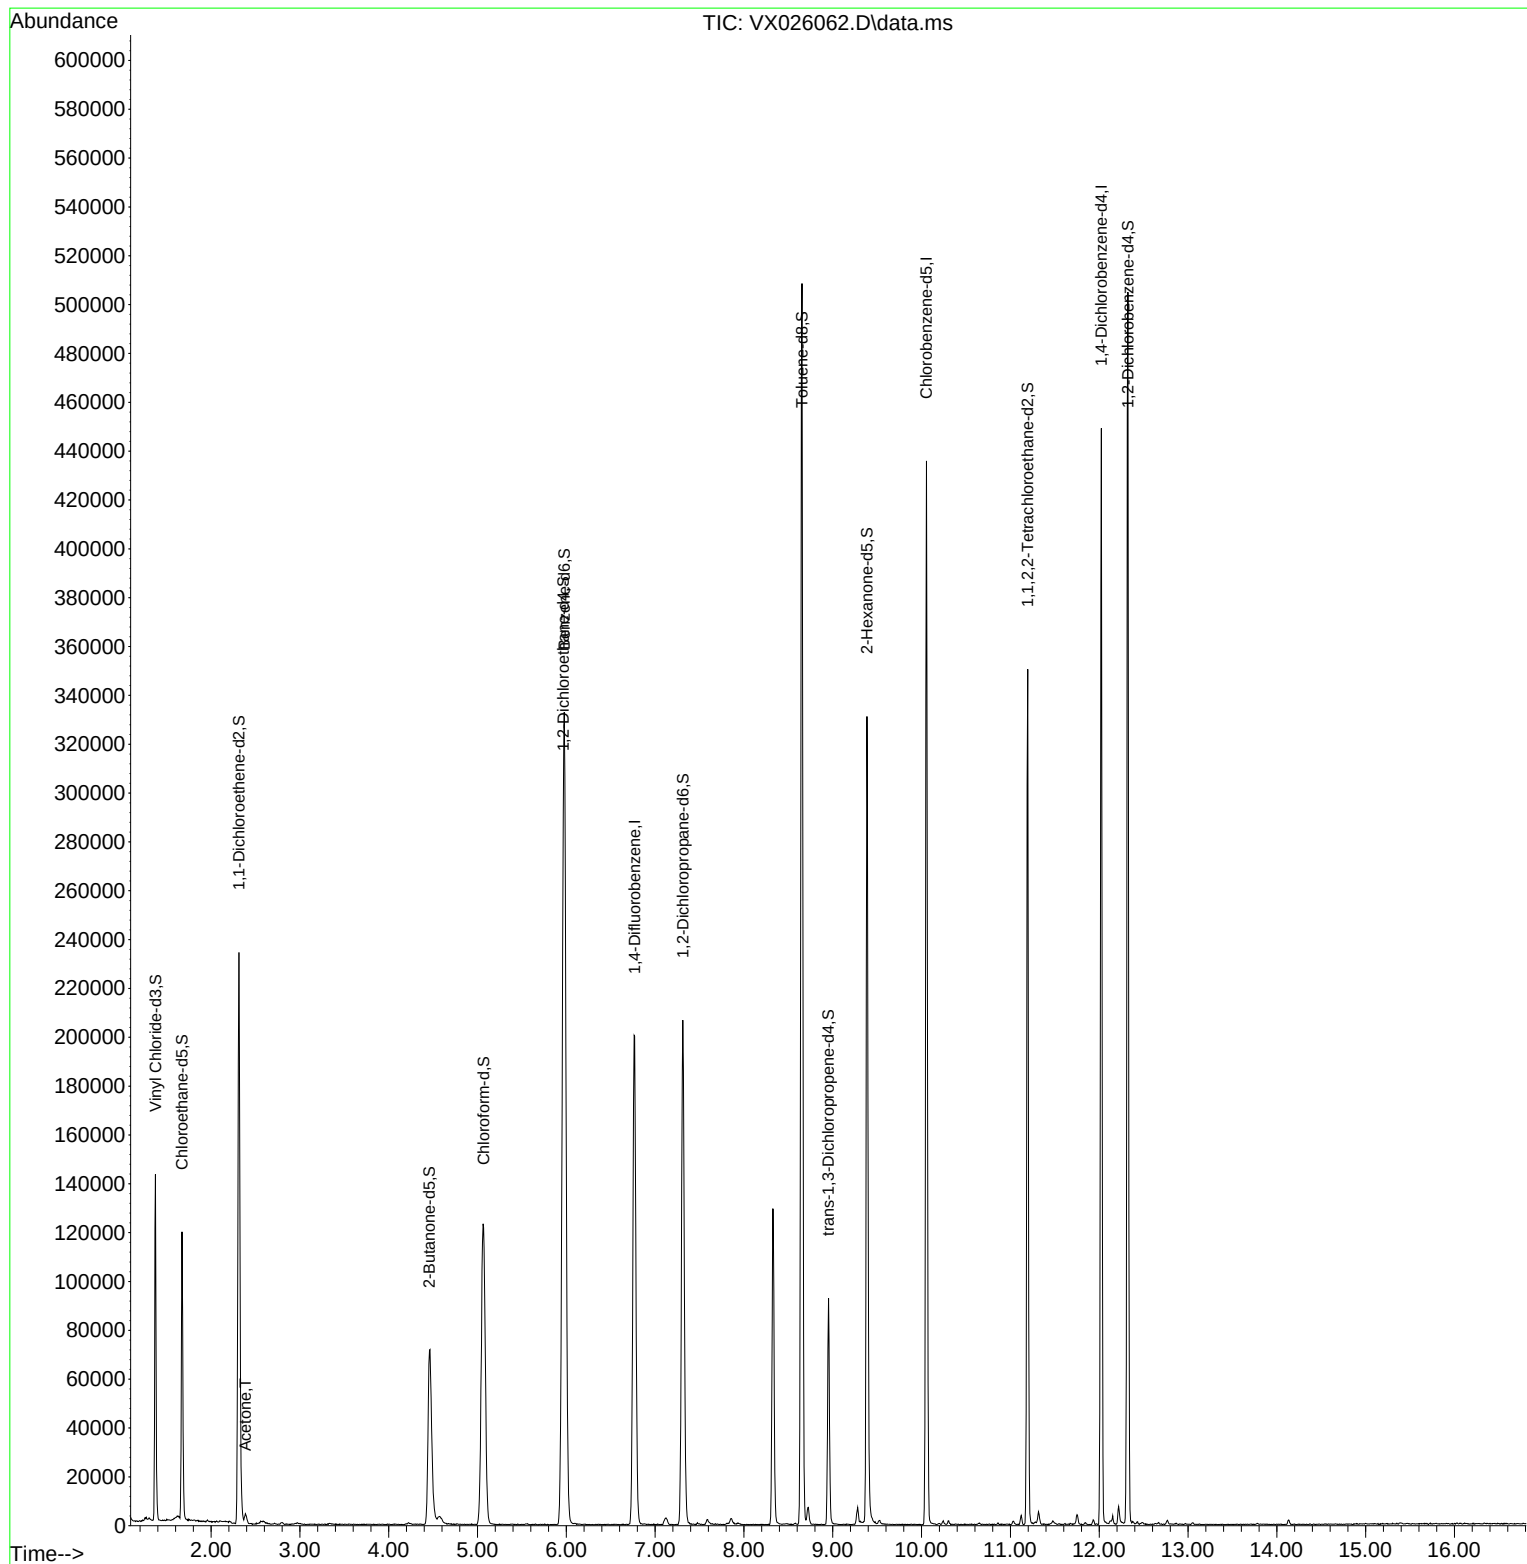

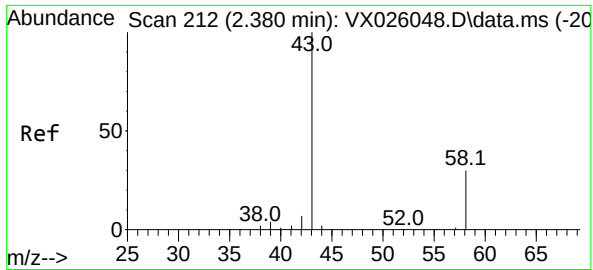

#13
 Acetone
 Concen: 6.832 ug/L
 RT: 2.386 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: VX026062.D
 Acq: 27 Dec 2021 15:22

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J23

Tgt Ion: 43 Resp: 4605
 Ion Ratio Lower Upper
 43 100
 58 25.4 0.0 65.6

