

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026050.D
 Acq On : 27 Dec 2021 10:38
 Operator : JC/MD
 Sample : VX1227WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK661

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis

Signal : TIC: VX026050.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	53	rVB	151450	151483	15.07%	2.032%
2	1.666	91	95	105	rVB	103264	134441	13.38%	1.804%
3	2.307	194	200	216	rVB	227204	370977	36.92%	4.977%
4	2.441	220	222	225	rVB2	292	251	0.02%	0.003%
5	2.502	228	232	233	rBV	557	497	0.05%	0.007%
6	2.703	262	265	267	rBV3	425	590	0.06%	0.008%
7	2.788	274	279	287	rVB4	1594	2856	0.28%	0.038%
8	3.026	316	318	322	rVB2	241	281	0.03%	0.004%
9	3.264	355	357	360	rVV2	263	264	0.03%	0.004%
10	3.380	375	376	380	rBV	256	279	0.03%	0.004%
11	3.483	389	393	396	rBV2	185	320	0.03%	0.004%
12	3.562	405	406	411	rVB	229	259	0.03%	0.003%
13	4.459	543	553	567	rBV	72238	224630	22.35%	3.014%
14	4.843	611	616	618	rBV2	252	442	0.04%	0.006%
15	5.062	639	652	673	rVB2	108574	396319	39.44%	5.317%
16	5.373	701	703	705	rBV2	299	268	0.03%	0.004%
17	5.489	717	722	728	rVB3	851	1682	0.17%	0.023%
18	5.654	745	749	751	rVV2	181	266	0.03%	0.004%
19	5.708	754	758	760	rVV	236	300	0.03%	0.004%
20	5.836	777	779	781	rVB	251	223	0.02%	0.003%
21	5.971	788	801	816	rBV2	340791	1004870	100.00%	13.482%
22	6.141	827	829	833	rBV2	256	366	0.04%	0.005%
23	6.233	843	844	847	rBV	330	280	0.03%	0.004%
24	6.355	859	864	865	rBV	212	297	0.03%	0.004%
25	6.763	921	931	943	rBV	208678	502650	50.02%	6.744%
26	7.001	966	970	972	rBV2	204	294	0.03%	0.004%
27	7.111	983	988	996	rVB5	2701	5307	0.53%	0.071%
28	7.312	1012	1021	1033	rBV	206136	456529	45.43%	6.125%
29	7.800	1099	1101	1108	rVB3	440	748	0.07%	0.010%
30	7.928	1118	1122	1130	rBV2	603	1202	0.12%	0.016%
31	8.031	1136	1139	1141	rBV	208	261	0.03%	0.004%
32	8.171	1159	1162	1164	rBV2	170	259	0.03%	0.003%
33	8.324	1179	1187	1198	rBV	143792	232312	23.12%	3.117%
34	8.488	1212	1214	1216	rVB2	384	278	0.03%	0.004%
35	8.580	1226	1229	1233	rVB	594	648	0.06%	0.009%
36	8.647	1233	1240	1248	rBV	522834	813482	80.95%	10.914%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026050.D
 Acq On : 27 Dec 2021 10:38
 Operator : JC/MD
 Sample : VX1227WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK661

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis

37	8.720	1248	1252	1258	rVB2	7581	11728	1.17%	0.157%
38	8.952	1284	1290	1302	rVB	98503	143840	14.31%	1.930%
39	9.104	1312	1315	1316	rBV2	445	554	0.06%	0.007%
40	9.275	1338	1343	1348	rBV2	3043	5431	0.54%	0.073%
41	9.385	1355	1361	1378	rVB	360187	503785	50.13%	6.759%
42	9.702	1408	1413	1417	rBV2	930	1178	0.12%	0.016%
43	10.055	1465	1471	1482	rVV	467308	622704	61.97%	8.354%
44	10.195	1491	1494	1498	rBV2	641	909	0.09%	0.012%
45	10.299	1507	1511	1519	rVB3	2546	3247	0.32%	0.044%
46	10.549	1549	1552	1554	rBV2	207	234	0.02%	0.003%
47	10.598	1558	1560	1564	rBV2	216	238	0.02%	0.003%
48	10.640	1564	1567	1573	rBV3	504	938	0.09%	0.013%
49	10.750	1583	1585	1588	rBV	376	333	0.03%	0.004%
50	11.122	1641	1646	1652	rVB	4722	5600	0.56%	0.075%
51	11.189	1652	1657	1666	rBV	353075	471512	46.92%	6.326%
52	11.384	1687	1689	1690	rBV	368	220	0.02%	0.003%
53	11.482	1698	1705	1707	rBV5	1818	3128	0.31%	0.042%
54	11.543	1713	1715	1718	rVB3	397	493	0.05%	0.007%
55	11.610	1724	1726	1728	rBV2	268	299	0.03%	0.004%
56	11.683	1736	1738	1740	rVB2	384	263	0.03%	0.004%
57	11.713	1740	1743	1745	rVV3	545	548	0.05%	0.007%
58	11.750	1745	1749	1754	rVV3	4344	6058	0.60%	0.081%
59	11.841	1761	1764	1767	rVB2	870	997	0.10%	0.013%
60	11.933	1775	1779	1783	rVB3	2197	2934	0.29%	0.039%
61	11.969	1783	1785	1788	rBV2	797	753	0.07%	0.010%
62	12.024	1788	1794	1804	rBV	492865	621681	61.87%	8.341%
63	12.128	1805	1811	1813	rVV4	1724	3263	0.32%	0.044%
64	12.146	1813	1814	1820	rVB2	2817	3001	0.30%	0.040%
65	12.323	1836	1843	1850	rBV	548617	706524	70.31%	9.479%
66	12.427	1856	1860	1864	rVB4	1539	2160	0.21%	0.029%
67	12.482	1864	1869	1875	rBV5	902	1743	0.17%	0.023%
68	12.610	1887	1890	1891	rVV2	230	238	0.02%	0.003%
69	12.622	1891	1892	1895	rVV	461	475	0.05%	0.006%
70	12.658	1896	1898	1903	rVV3	891	1137	0.11%	0.015%
71	12.768	1911	1916	1921	rBV3	1542	2223	0.22%	0.030%
72	12.853	1927	1930	1933	rVB	466	539	0.05%	0.007%
73	12.951	1944	1946	1947	rBV2	333	234	0.02%	0.003%
74	13.000	1952	1954	1956	rVV2	448	388	0.04%	0.005%
75	13.042	1958	1961	1962	rVV2	380	337	0.03%	0.005%
76	13.055	1962	1963	1967	rVV2	784	608	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
 Data File : VX026050.D
 Acq On : 27 Dec 2021 10:38
 Operator : JC/MD
 Sample : VX1227WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK661

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
 Title : VOC Analysis

77	13.116	1971	1973	1976	rBV3	349	448	0.04%	0.006%
78	13.250	1993	1995	1997	rBV2	254	226	0.02%	0.003%
79	13.469	2029	2031	2034	rBV	263	218	0.02%	0.003%
80	13.597	2048	2052	2053	rBB2	352	409	0.04%	0.005%
81	13.634	2056	2058	2060	rVB2	315	221	0.02%	0.003%
82	13.780	2078	2082	2088	rVB3	1403	1820	0.18%	0.024%
83	13.859	2093	2095	2098	rBV2	287	365	0.04%	0.005%
84	13.951	2107	2110	2111	rBV2	323	317	0.03%	0.004%
85	14.134	2135	2140	2144	rBV	2711	3727	0.37%	0.050%
86	14.274	2159	2163	2166	rBV3	245	420	0.04%	0.006%
87	14.378	2177	2180	2183	rBV3	310	449	0.04%	0.006%
88	14.554	2207	2209	2212	rVB	320	281	0.03%	0.004%
89	14.640	2221	2223	2225	rBV	400	281	0.03%	0.004%
90	14.695	2230	2232	2234	rBV	249	221	0.02%	0.003%
91	14.999	2280	2282	2284	rBV	391	283	0.03%	0.004%
92	15.097	2293	2298	2299	rBV2	369	511	0.05%	0.007%
93	15.262	2324	2325	2327	rBV	336	215	0.02%	0.003%
94	15.396	2343	2347	2351	rVB3	1200	1749	0.17%	0.023%
95	15.499	2362	2364	2368	rBV3	417	384	0.04%	0.005%
96	15.530	2368	2369	2371	rBV2	296	254	0.03%	0.003%
97	15.743	2402	2404	2406	rBV3	387	286	0.03%	0.004%
98	15.944	2435	2437	2442	rBV2	426	618	0.06%	0.008%
99	16.164	2470	2473	2476	rBV	521	521	0.05%	0.007%
100	16.438	2516	2518	2521	rBV2	469	521	0.05%	0.007%




Sum of corrected areas: 7453631

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026050.D
Acq On : 27 Dec 2021 10:38
Operator : JC/MD
Sample : VX1227WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK661

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

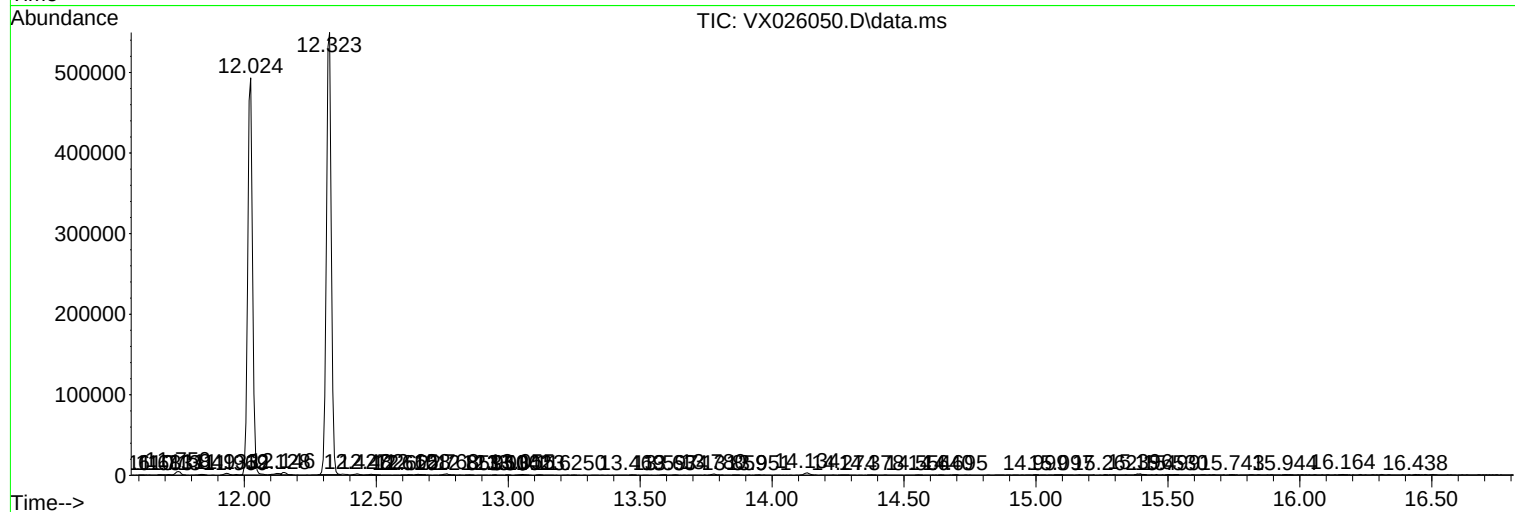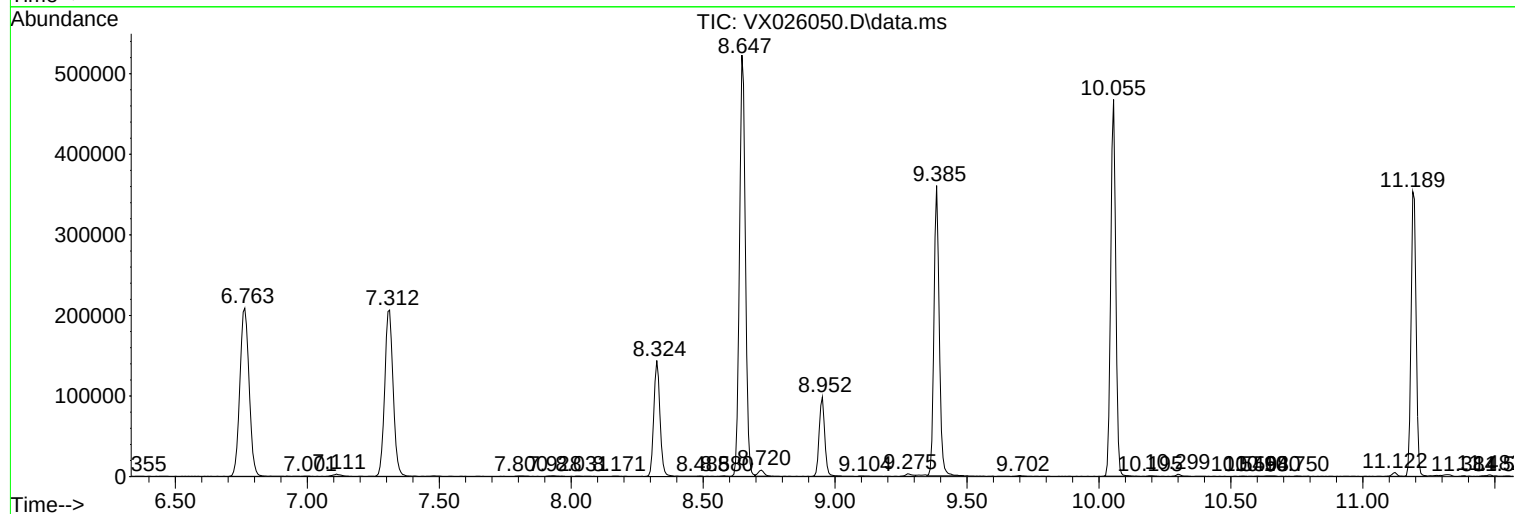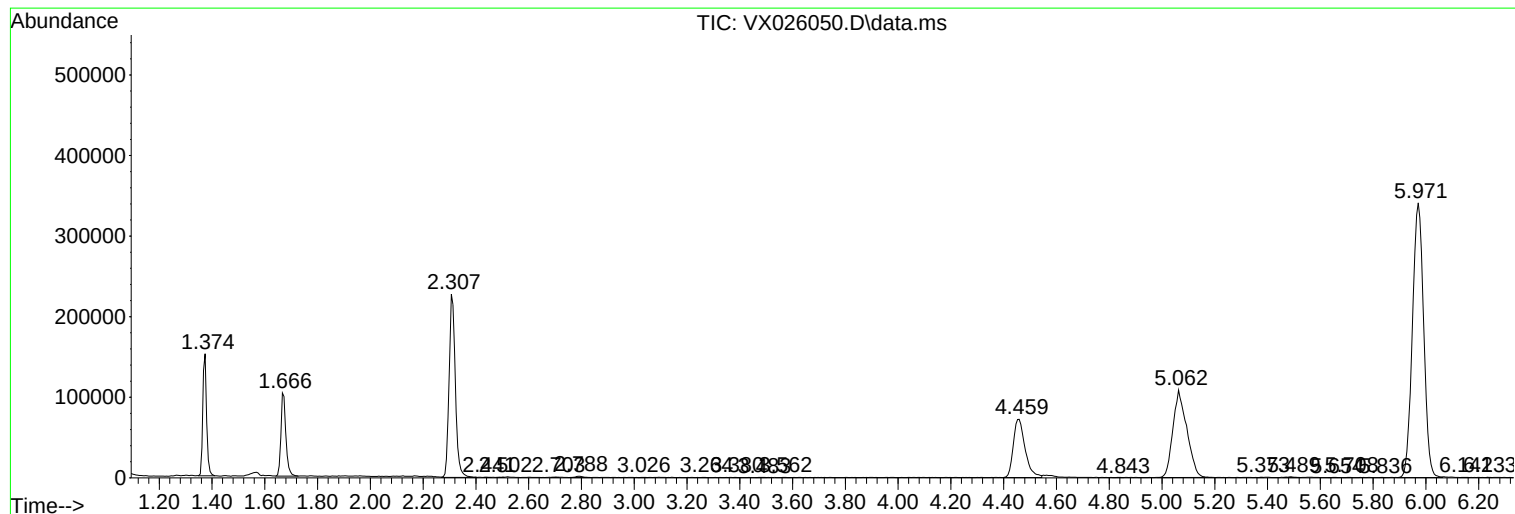

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026050.D
Acq On : 27 Dec 2021 10:38
Operator : JC/MD
Sample : VX1227WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK661

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122721\
Data File : VX026050.D
Acq On : 27 Dec 2021 10:38
Operator : JC/MD
Sample : VX1227WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK661

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc